

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0051721\
 Data File : P0077876.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 May 2021 14:07
 Operator : DD\AJ
 Sample : M2392-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 SB-03-COMP

Manual Integrations
 APPROVED

Ankita
 5/18/2021 4:19:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 16:08:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0051321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 14 05:52:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.349	3.629	1157708	562149	19.722m	22.093
2) SA Decachlor...	9.966	8.823	744953	434322	18.020m	18.072
Target Compounds						
31) L7 AR-1260-1	7.306	6.424	86168	63447	33.894	43.067 #
32) L7 AR-1260-2	7.571	6.620	195968	50210	70.169m	28.946 #
33) L7 AR-1260-3	7.931	6.770	44418	48825	22.284m	29.819 #
34) L7 AR-1260-4	8.153	7.248	101238	27295	46.359	22.560 #
35) L7 AR-1260-5	8.470	7.496	109858	63237	25.389	22.242

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051721\
Data File : P0077876.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 May 2021 14:07
Operator : DD\AJ
Sample : M2392-08
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SB-03-COMP


Manual Integrations
APPROVED

Ankita
5/18/2021 4:19:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 16:08:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 14 05:52:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

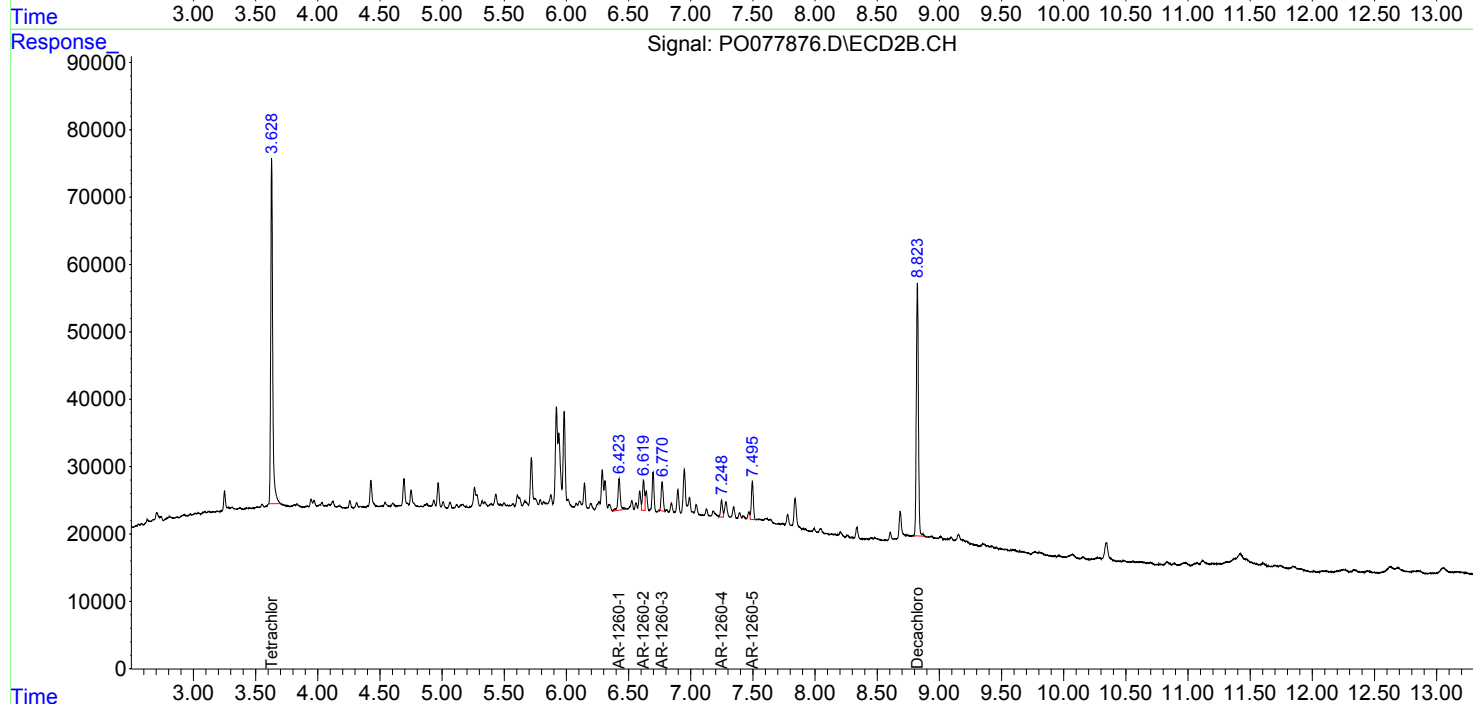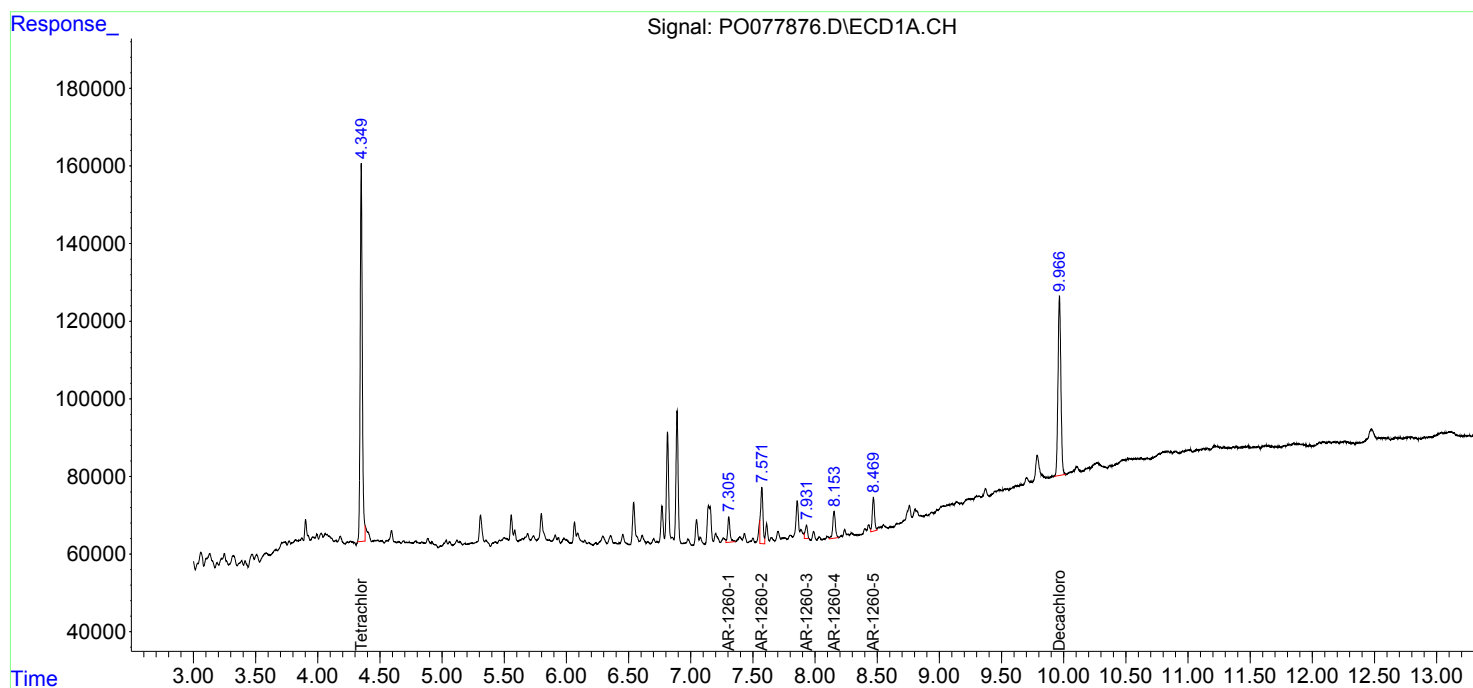

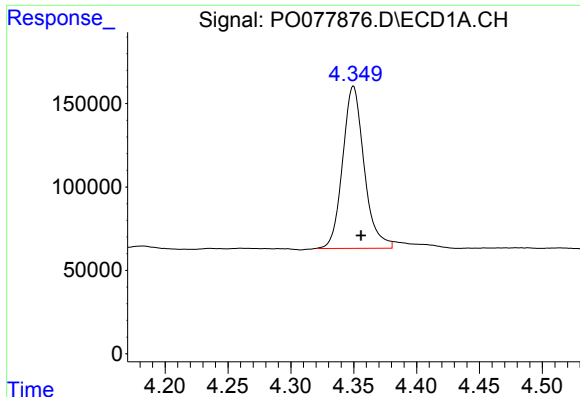


#1 Tetrachloro-m-xylene

R.T.: 4.349 min
Delta R.T.: -0.007 min
Response: 1157708
Conc: 19.72 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-03-COMP


Manual Integrations
APPROVED

Ankita
5/18/2021 4:19:17 PM

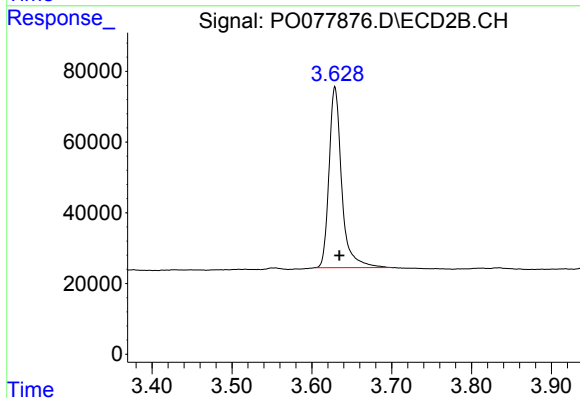


#1 Tetrachloro-m-xylene

R.T.: 3.629 min
Delta R.T.: -0.006 min
Response: 562149
Conc: 22.09 ng/ml

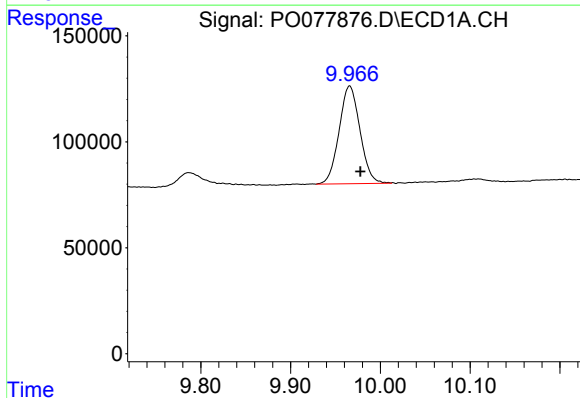


#2 Decachlorobiphenyl

R.T.: 9.966 min
Delta R.T.: -0.012 min
Response: 744953
Conc: 18.02 ng/ml m

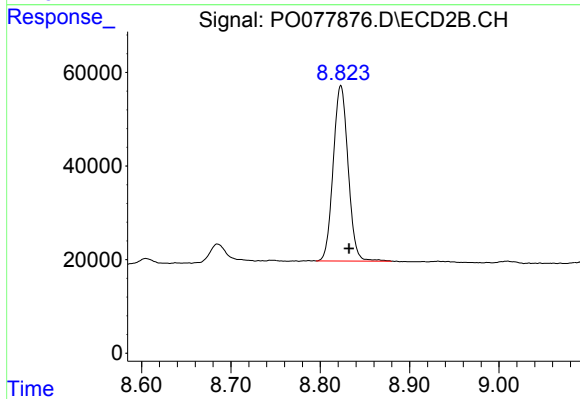

#2 Decachlorobiphenyl

R.T.: 8.823 min
Delta R.T.: -0.009 min
Response: 434322
Conc: 18.07 ng/ml

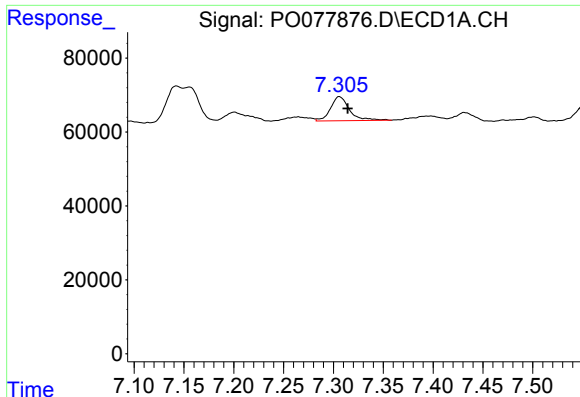


#31 AR-1260-1

R.T.: 7.306 min
Delta R.T.: -0.008 min
Response: 86168
Conc: 33.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-03-COMP


Manual Integrations
APPROVED

Ankita
5/18/2021 4:19:17 PM

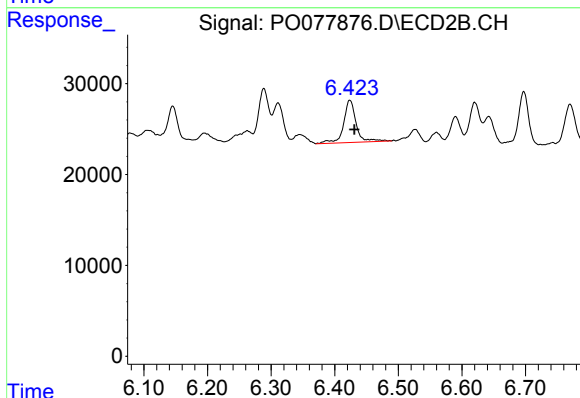


#31 AR-1260-1

R.T.: 6.424 min
Delta R.T.: -0.007 min
Response: 63447
Conc: 43.07 ng/ml

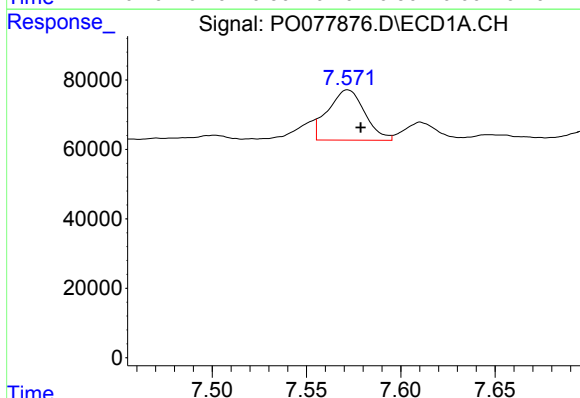


#32 AR-1260-2

R.T.: 7.571 min
Delta R.T.: -0.007 min
Response: 195968
Conc: 70.17 ng/ml m

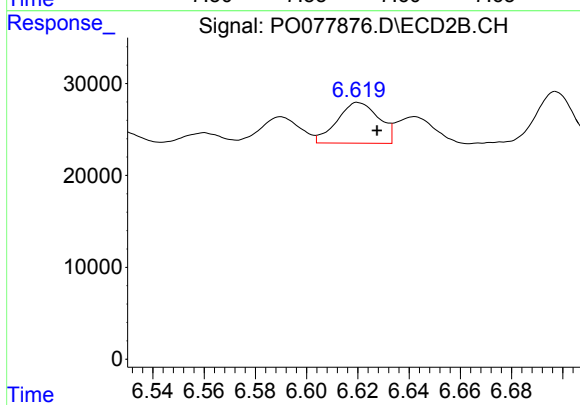

#32 AR-1260-2

R.T.: 6.620 min
Delta R.T.: -0.007 min
Response: 50210
Conc: 28.95 ng/ml

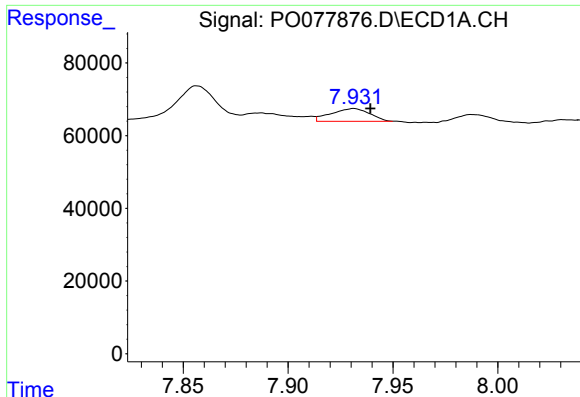


#33 AR-1260-3

R.T.: 7.931 min
Delta R.T.: -0.008 min
Response: 44418
Conc: 22.28 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-03-COMP


Manual Integrations
APPROVED

Ankita
5/18/2021 4:19:17 PM

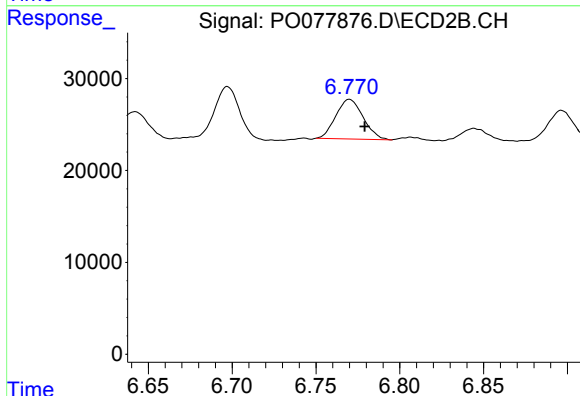


#33 AR-1260-3

R.T.: 6.770 min
Delta R.T.: -0.009 min
Response: 48825
Conc: 29.82 ng/ml

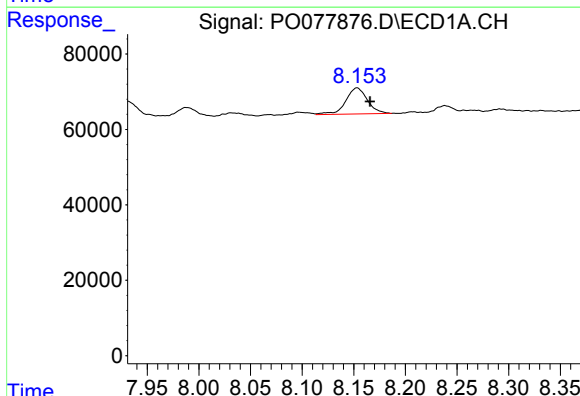


#34 AR-1260-4

R.T.: 8.153 min
Delta R.T.: -0.013 min
Response: 101238
Conc: 46.36 ng/ml

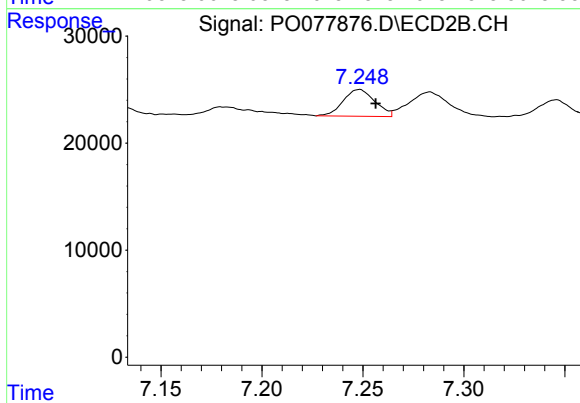

#34 AR-1260-4

R.T.: 7.248 min
Delta R.T.: -0.008 min
Response: 27295
Conc: 22.56 ng/ml

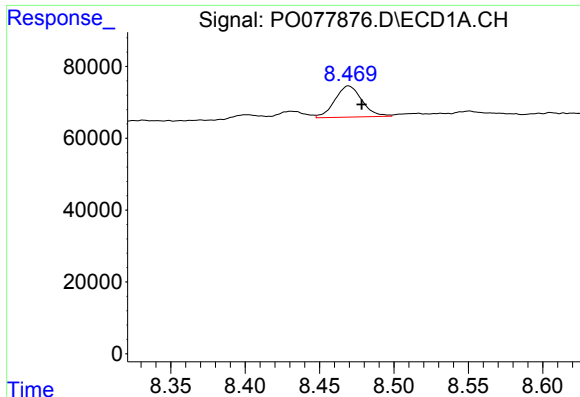


#35 AR-1260-5

R.T.: 8.470 min
Delta R.T.: -0.009 min
Response: 109858
Conc: 25.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-03-COMP

Manual Integrations
APPROVED

Ankita
5/18/2021 4:19:17 PM

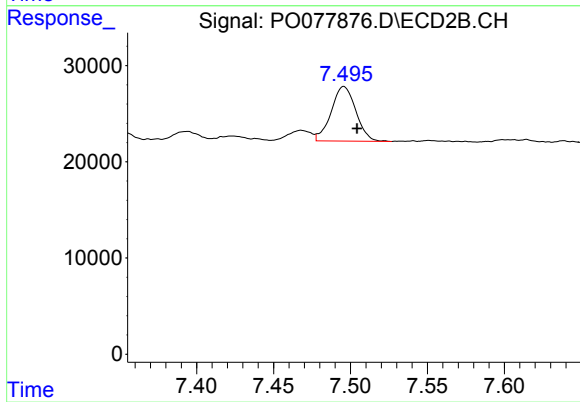

#35 AR-1260-5

R.T.: 7.496 min
Delta R.T.: -0.009 min
Response: 63237
Conc: 22.24 ng/ml