

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0051721\
 Data File : P0077881.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 May 2021 15:33
 Operator : DD\AJ
 Sample : M2392-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 SB-06-COMP

Manual Integrations
 APPROVED

Ankita
 5/18/2021 4:19:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 16:11:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0051321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 14 05:52:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.350	3.630	1349374	606208	22.987	23.824
2) SA Decachlor...	9.966	8.824	695533	450170	16.824	18.732
Target Compounds						
31) L7 AR-1260-1	7.306	6.424	203518	169400	80.054m	114.986 #
32) L7 AR-1260-2	7.571	6.621	246879	185426	88.398	106.899
33) L7 AR-1260-3	7.931	6.770	200545	153453	100.609m	93.718
34) L7 AR-1260-4	8.152	7.248	277858	87764	127.237	72.540m#
35) L7 AR-1260-5	8.470	7.496	370226	169014	85.563	59.445m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051721\
Data File : P0077881.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 May 2021 15:33
Operator : DD\AJ
Sample : M2392-17
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SB-06-COMP


Manual Integrations
APPROVED

Ankita
5/18/2021 4:19:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 16:11:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 14 05:52:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

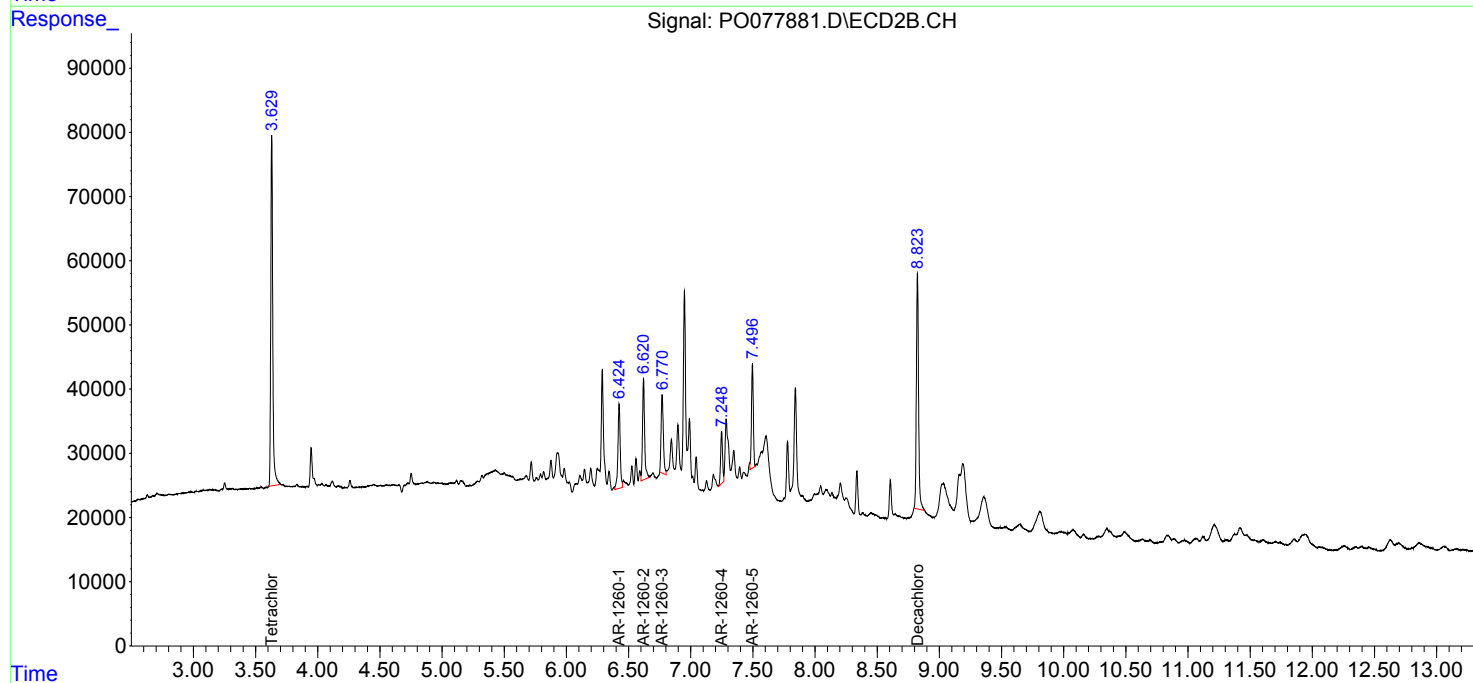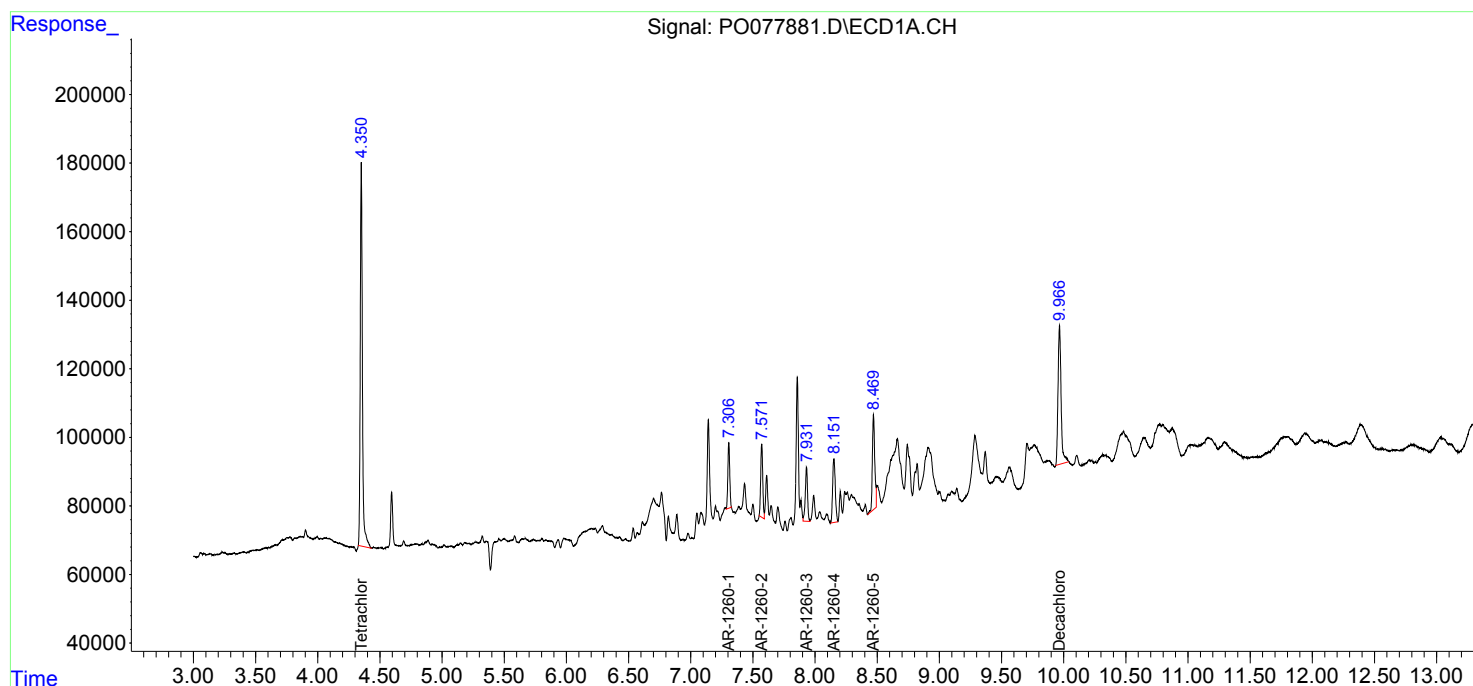

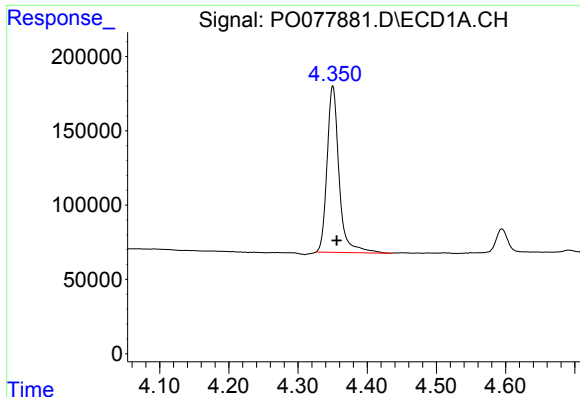


#1 Tetrachloro-m-xylene

R.T.: 4.350 min
Delta R.T.: -0.006 min
Response: 1349374
Conc: 22.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-06-COMP


Manual Integrations
APPROVED

Ankita
5/18/2021 4:19:25 PM

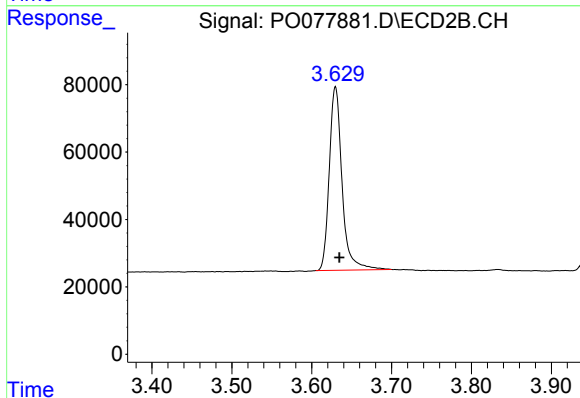


#1 Tetrachloro-m-xylene

R.T.: 3.630 min
Delta R.T.: -0.005 min
Response: 606208
Conc: 23.82 ng/ml

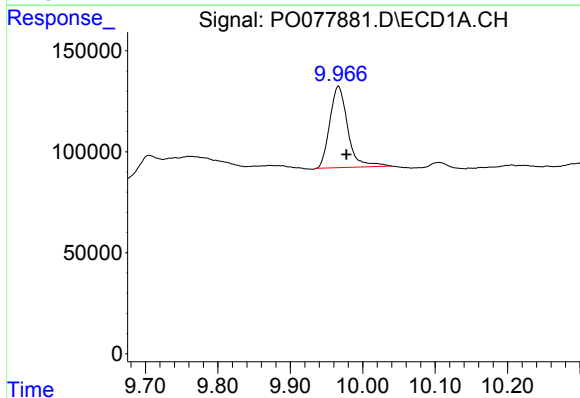


#2 Decachlorobiphenyl

R.T.: 9.966 min
Delta R.T.: -0.011 min
Response: 695533
Conc: 16.82 ng/ml

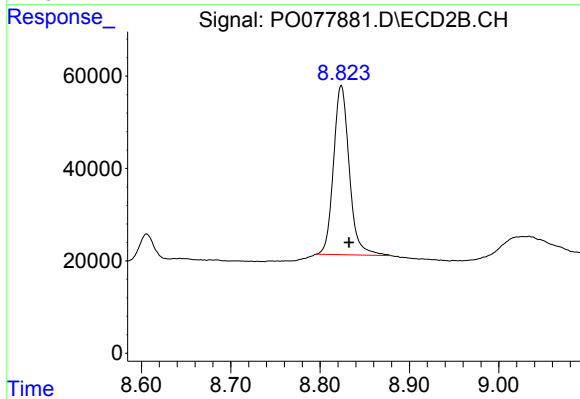

#2 Decachlorobiphenyl

R.T.: 8.824 min
Delta R.T.: -0.009 min
Response: 450170
Conc: 18.73 ng/ml

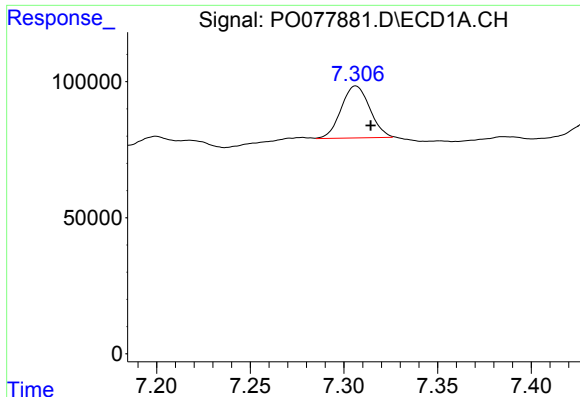


#31 AR-1260-1

R.T.: 7.306 min
Delta R.T.: -0.008 min
Response: 203518
Conc: 80.05 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-06-COMP


Manual Integrations
APPROVED

Ankita
5/18/2021 4:19:25 PM

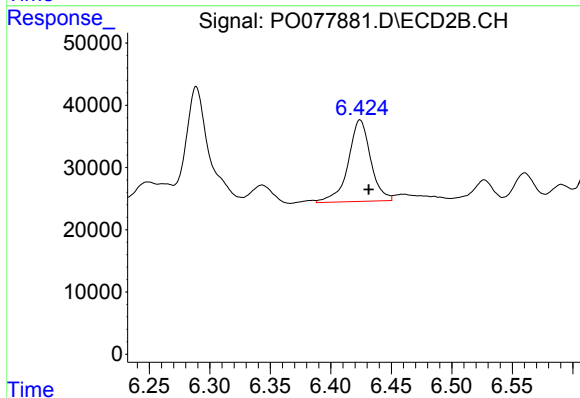


#31 AR-1260-1

R.T.: 6.424 min
Delta R.T.: -0.007 min
Response: 169400
Conc: 114.99 ng/ml

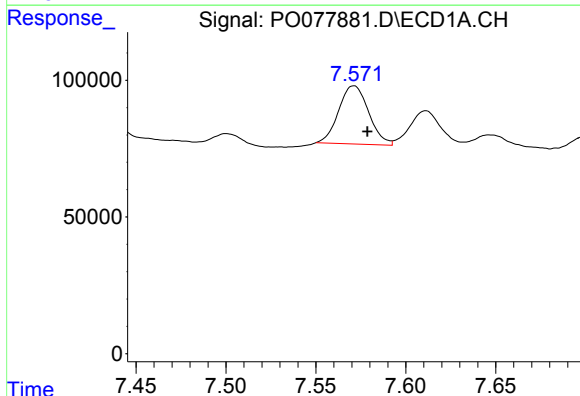


#32 AR-1260-2

R.T.: 7.571 min
Delta R.T.: -0.008 min
Response: 246879
Conc: 88.40 ng/ml

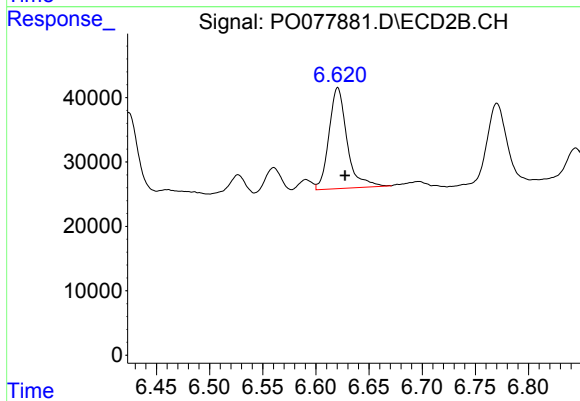

#32 AR-1260-2

R.T.: 6.621 min
Delta R.T.: -0.007 min
Response: 185426
Conc: 106.90 ng/ml

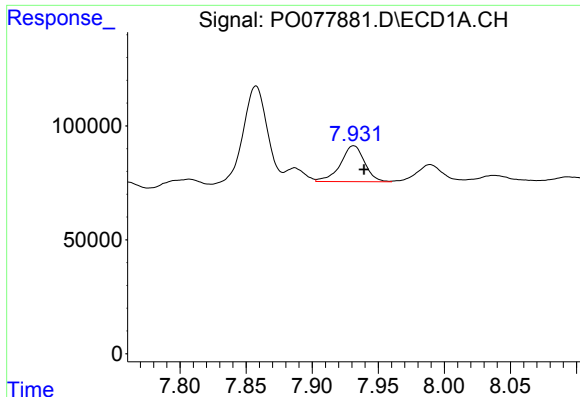


#33 AR-1260-3

R.T.: 7.931 min
Delta R.T.: -0.008 min
Response: 200545
Conc: 100.61 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-06-COMP


Manual Integrations
APPROVED

Ankita
5/18/2021 4:19:25 PM

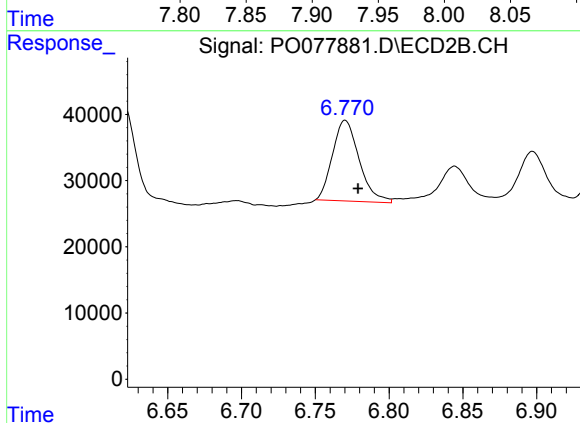


#33 AR-1260-3

R.T.: 6.770 min
Delta R.T.: -0.009 min
Response: 153453
Conc: 93.72 ng/ml

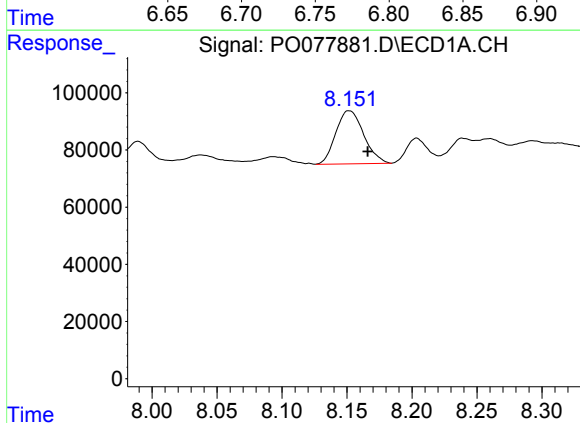


#34 AR-1260-4

R.T.: 8.152 min
Delta R.T.: -0.014 min
Response: 277858
Conc: 127.24 ng/ml

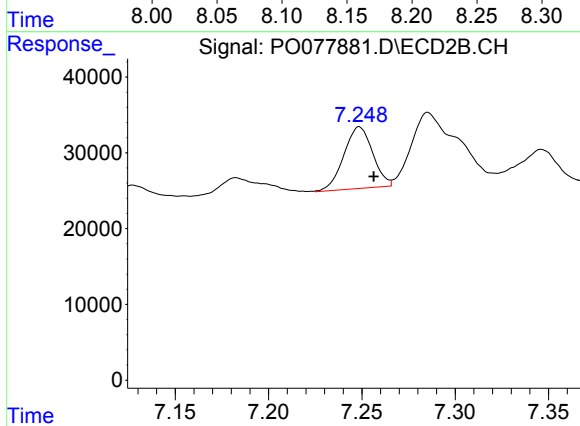

#34 AR-1260-4

R.T.: 7.248 min
Delta R.T.: -0.008 min
Response: 87764
Conc: 72.54 ng/ml m

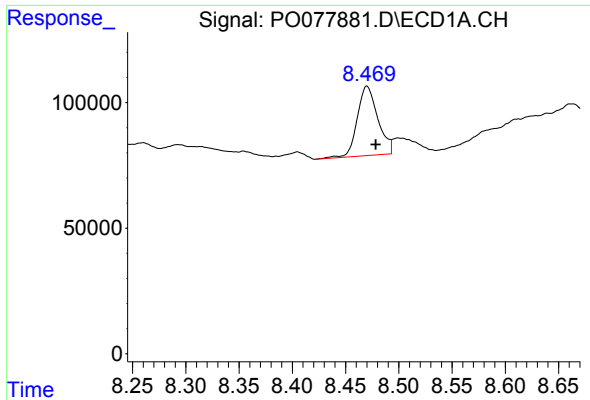


#35 AR-1260-5

R.T.: 8.470 min
Delta R.T.: -0.008 min
Response: 370226
Conc: 85.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-06-COMP

Manual Integrations
APPROVED

Ankita
5/18/2021 4:19:25 PM

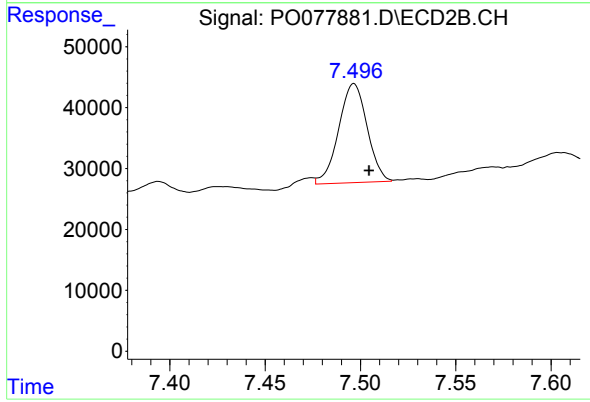

#35 AR-1260-5

R.T.: 7.496 min
Delta R.T.: -0.008 min
Response: 169014
Conc: 59.44 ng/ml m