

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051721\
 Data File : P0077903.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 May 2021 22:27
 Operator : DD\AJ
 Sample : M2421-12 10X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 K328-6A

Manual Integrations
 APPROVED

Ankita
 5/18/2021 4:19:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 04:47:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 14 05:52:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.347	3.628	194993	46108	3.322m	1.812m#
2) SA Decachlor...	9.962f	8.821	107303	69900	2.596	2.909

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051721\
Data File : P0077903.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 May 2021 22:27
Operator : DD\AJ
Sample : M2421-12 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
K328-6A


Manual Integrations
APPROVED

Ankita
5/18/2021 4:19:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 04:47:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 14 05:52:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

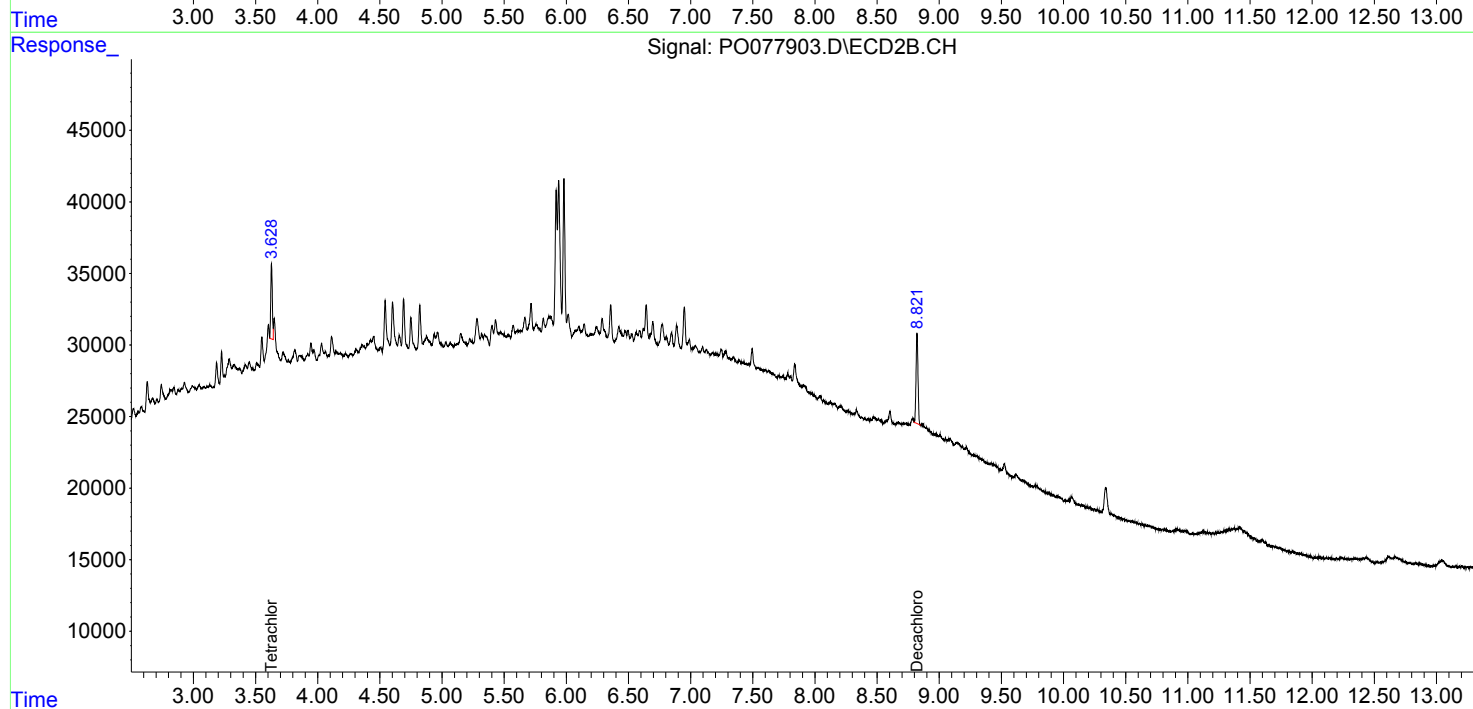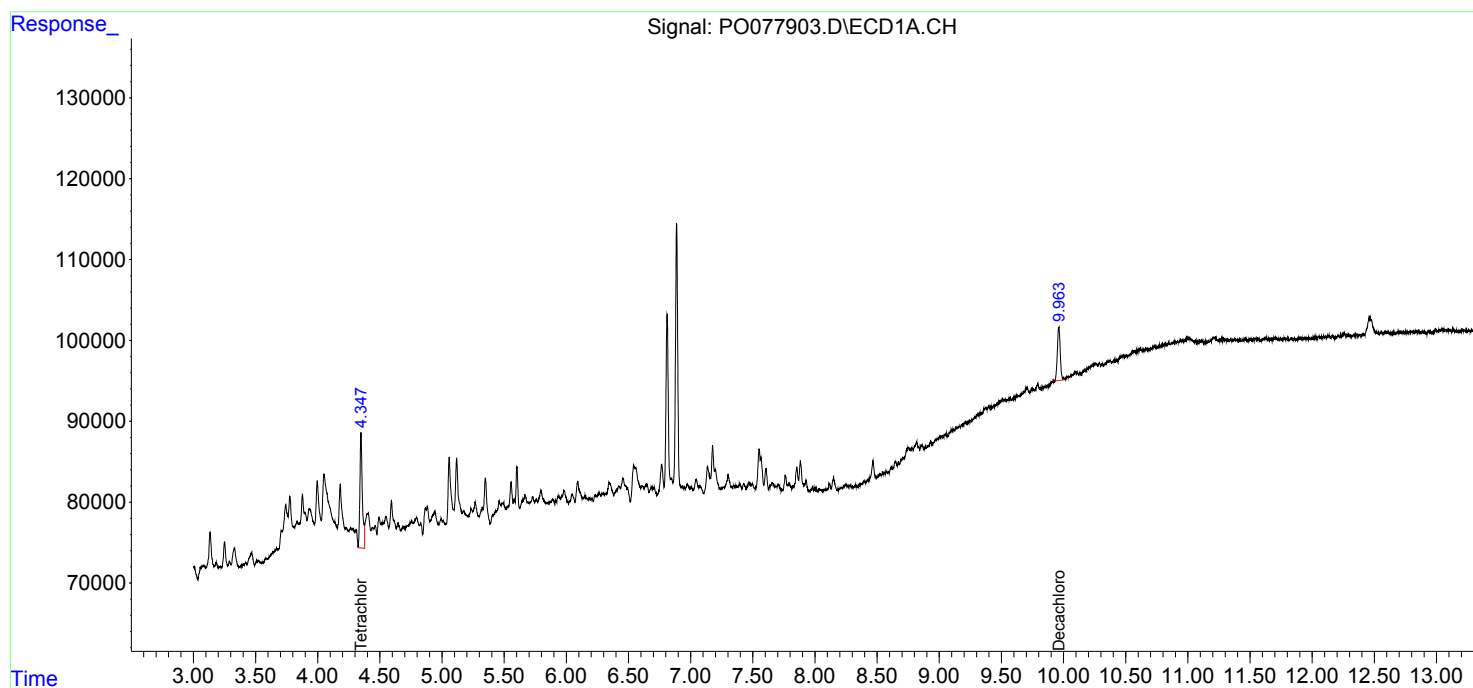

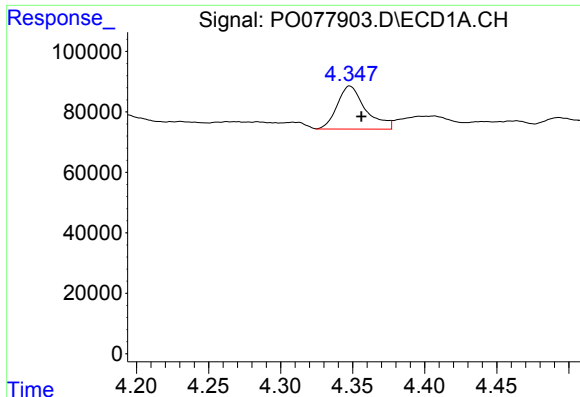


#1 Tetrachloro-m-xylene

R.T.: 4.347 min
Delta R.T.: -0.009 min
Response: 194993
Conc: 3.32 ng/ml m

Instrument :
ECD_O
ClientSampleId :
K328-6A


Manual Integrations
APPROVED

Ankita
5/18/2021 4:19:54 PM

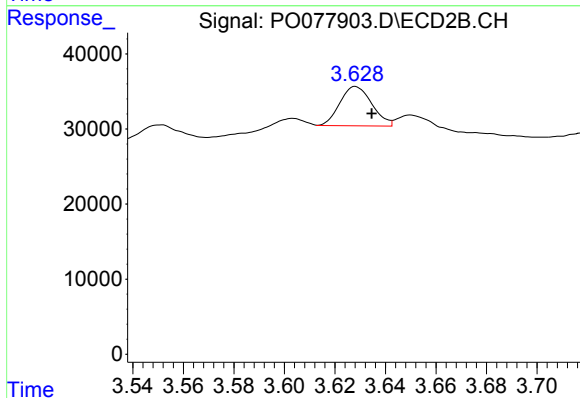


#1 Tetrachloro-m-xylene

R.T.: 3.628 min
Delta R.T.: -0.007 min
Response: 46108
Conc: 1.81 ng/ml m

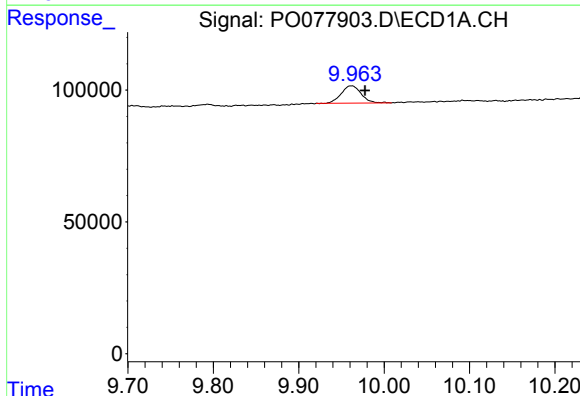

#2 Decachlorobiphenyl

R.T.: 9.962 min
Delta R.T.: -0.016 min
Response: 107303
Conc: 2.60 ng/ml

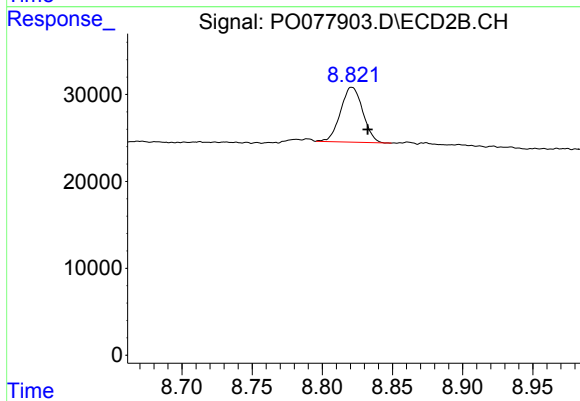

#2 Decachlorobiphenyl

R.T.: 8.821 min
Delta R.T.: -0.011 min
Response: 69900
Conc: 2.91 ng/ml