

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051721\
 Data File : P0077904.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 May 2021 22:44
 Operator : DD\AJ
 Sample : M2421-13 10X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 K328-DUP2

Manual Integrations
 APPROVED

Ankita
 5/18/2021 4:19:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 04:48:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 14 05:52:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.348	3.628	187575	66560	3.195m	2.616m
2) SA Decachlor...	9.963f	8.822	103562	70541	2.505	2.935

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051721\
Data File : PO077904.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 May 2021 22:44
Operator : DD\AJ
Sample : M2421-13 10X
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
K328-DUP2


Manual Integrations
APPROVED

Ankita
5/18/2021 4:19:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 04:48:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 14 05:52:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

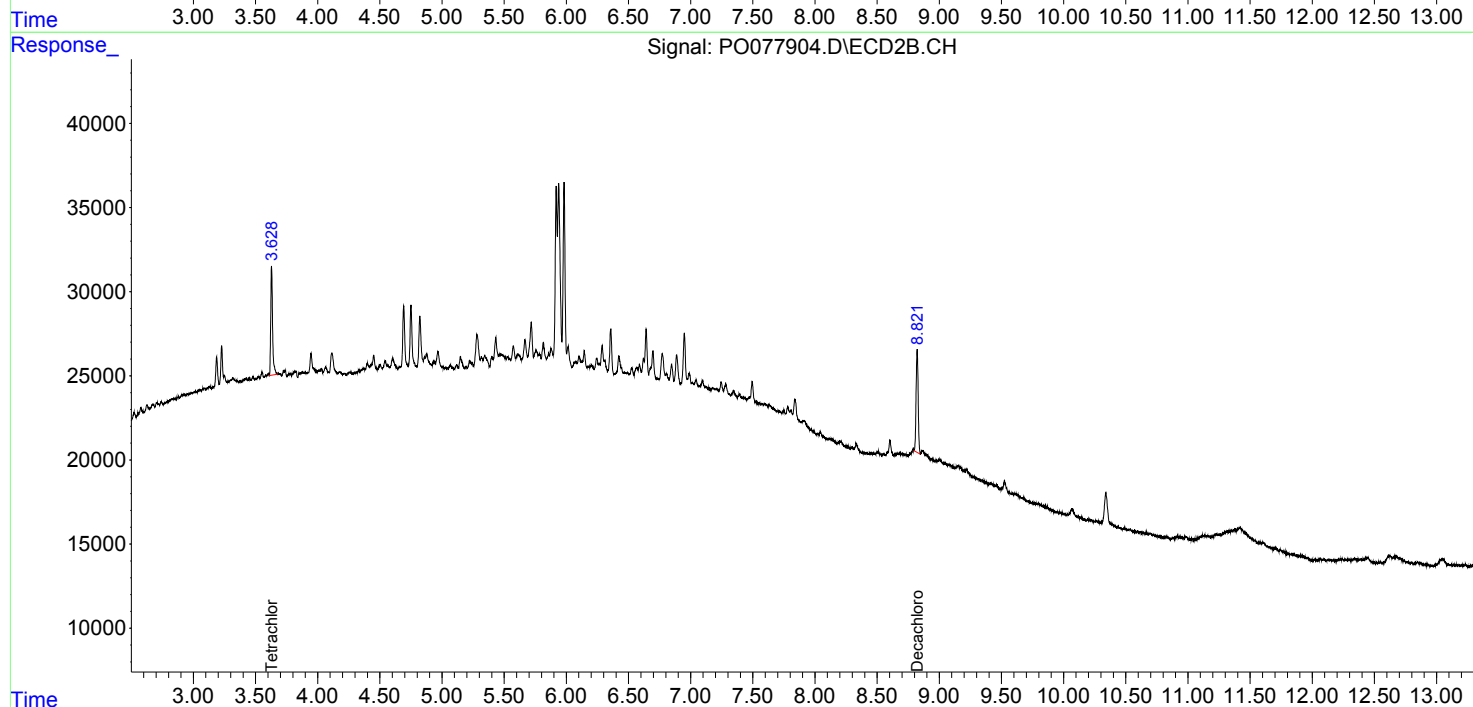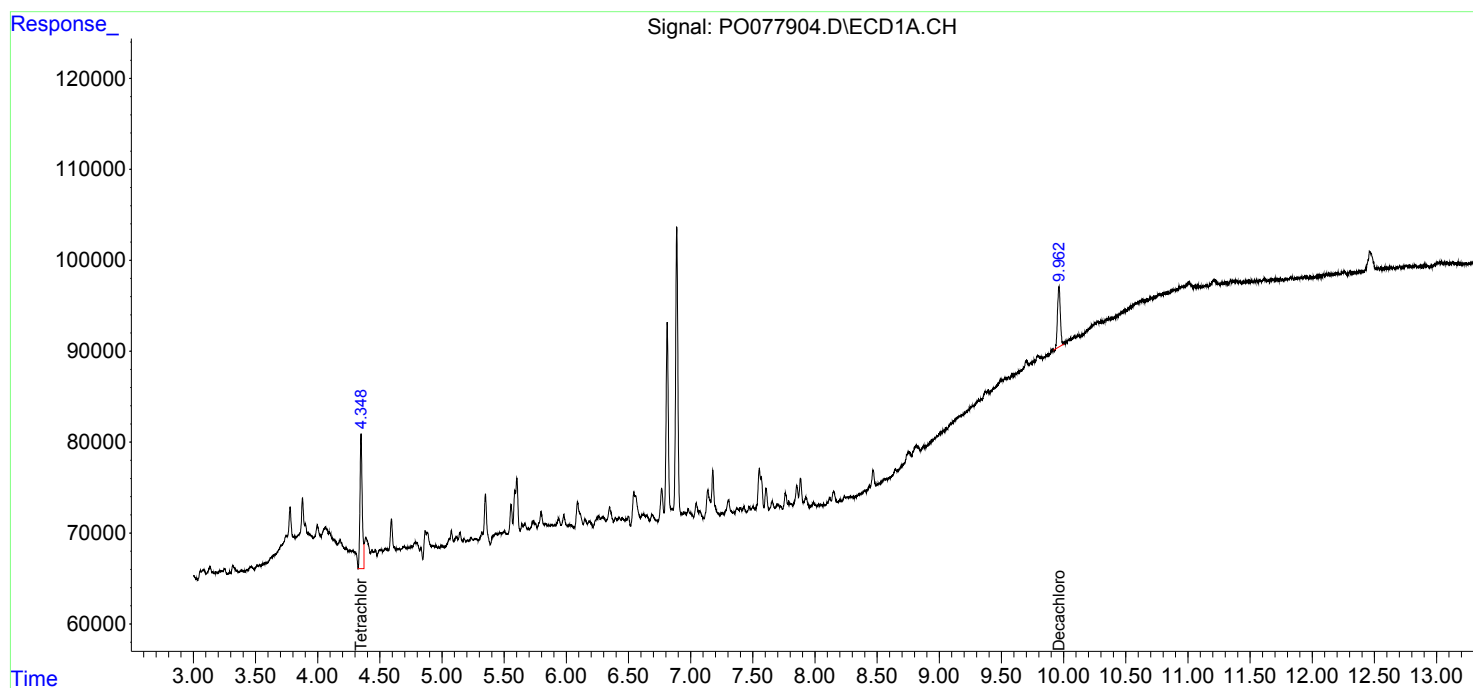

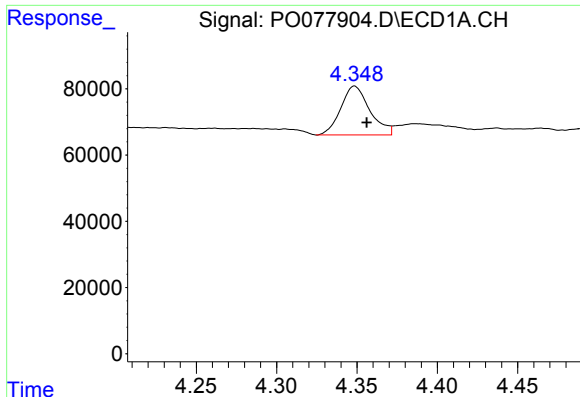


#1 Tetrachloro-m-xylene

R.T.: 4.348 min
Delta R.T.: -0.008 min
Response: 187575
Conc: 3.20 ng/ml m

Instrument :
ECD_O
ClientSampleId :
K328-DUP2


Manual Integrations
APPROVED

Ankita
5/18/2021 4:19:56 PM

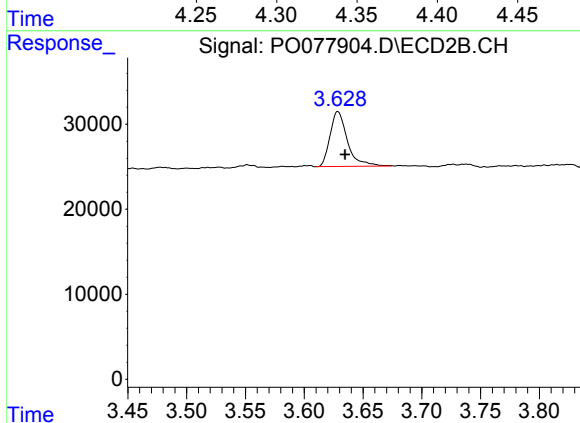


#1 Tetrachloro-m-xylene

R.T.: 3.628 min
Delta R.T.: -0.006 min
Response: 66560
Conc: 2.62 ng/ml m

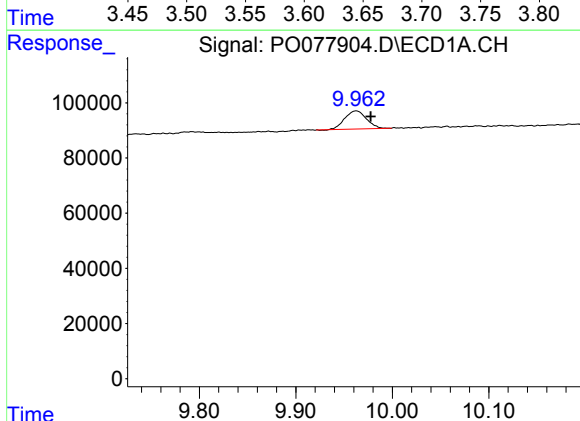

#2 Decachlorobiphenyl

R.T.: 9.963 min
Delta R.T.: -0.015 min
Response: 103562
Conc: 2.51 ng/ml

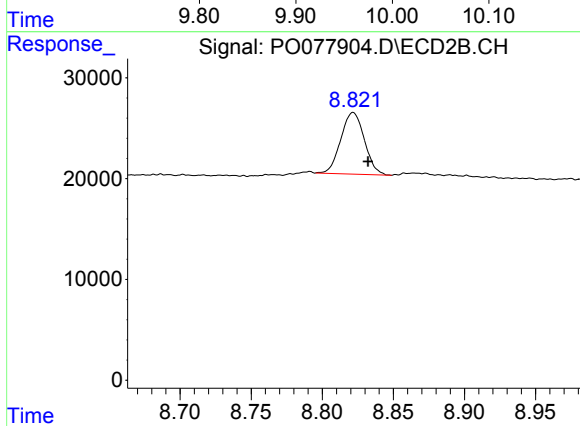

#2 Decachlorobiphenyl

R.T.: 8.822 min
Delta R.T.: -0.011 min
Response: 70541
Conc: 2.94 ng/ml