

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051721\
 Data File : P0077909.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 May 2021 00:10
 Operator : DD\AJ
 Sample : M2422-03 10X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 K328-11A

Manual Integrations
 APPROVED

Ankita
 5/18/2021 4:20:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 09:24:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 14 05:52:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.348	3.629	167630	63483	2.856	2.495
2) SA Decachlor...	9.963	8.821	111417	70346	2.695	2.927
Target Compounds						
31) L7 AR-1260-1	7.302	6.423	33512	20495	13.182	13.912
32) L7 AR-1260-2	7.569	6.622	43090	11478	15.429m	6.617 #
33) L7 AR-1260-3	7.930	6.772	21136	23655	10.604m	14.447 #
34) L7 AR-1260-4	8.151	7.247	25078	8361	11.484m	6.911 #
35) L7 AR-1260-5	8.468	7.494	36118	24155	8.347	8.496

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051721\
Data File : P0077909.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 May 2021 00:10
Operator : DD\AJ
Sample : M2422-03 10X
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
K328-11A


Manual Integrations
APPROVED

Ankita
5/18/2021 4:20:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 09:24:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 14 05:52:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

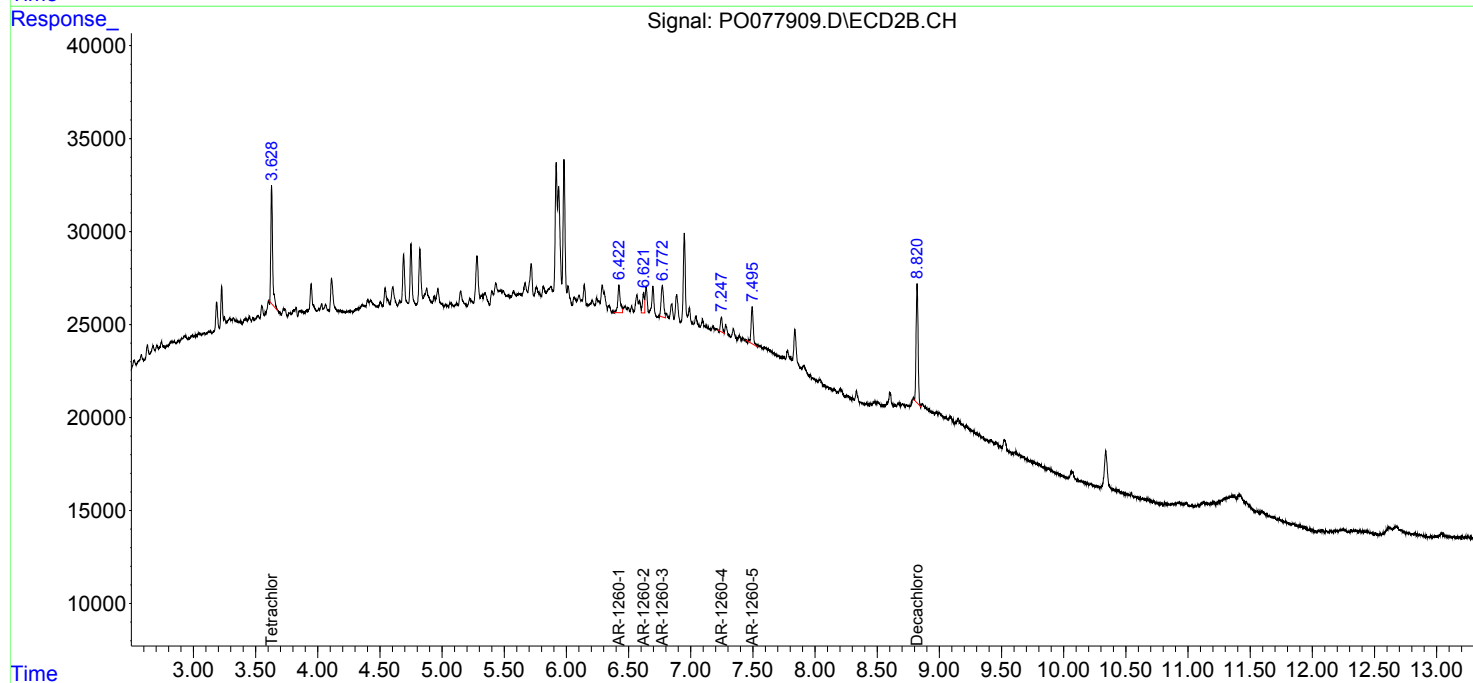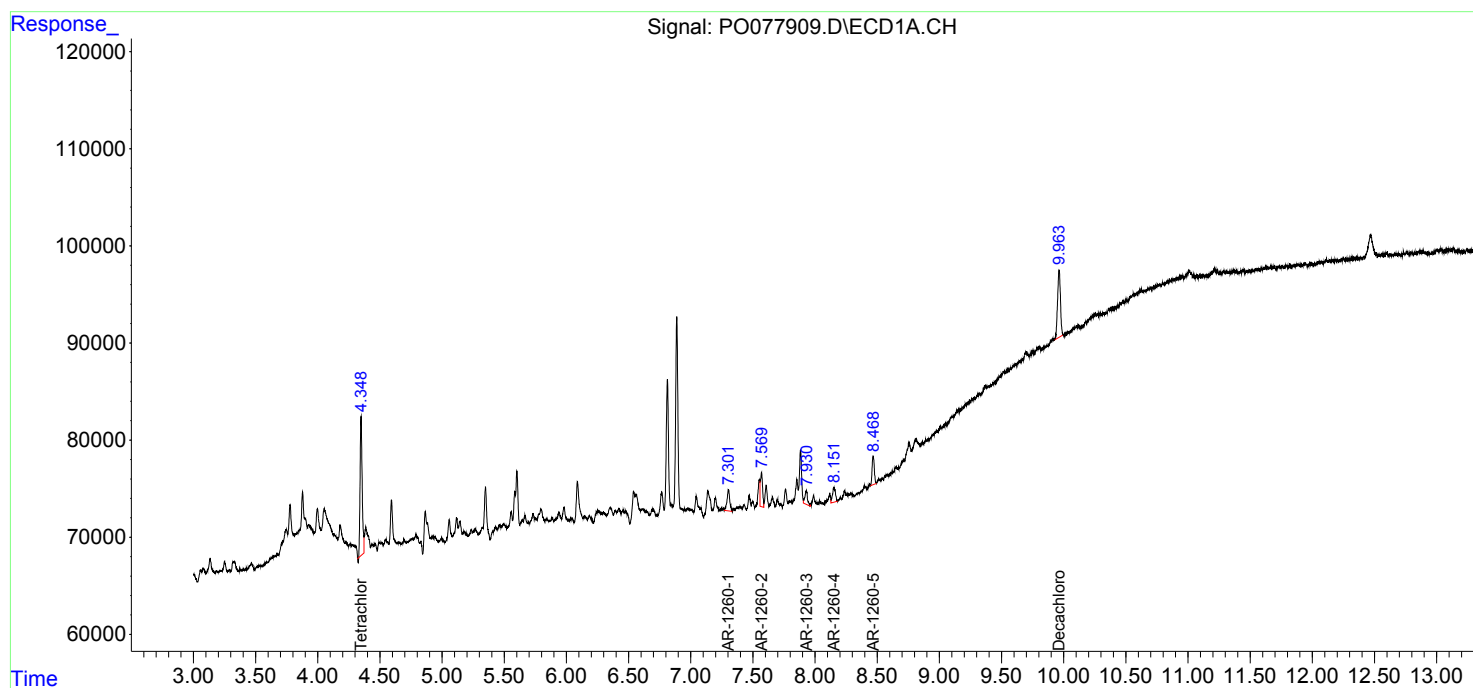

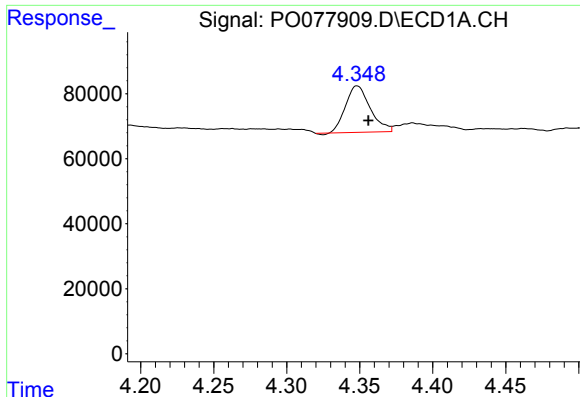


#1 Tetrachloro-m-xylene

R.T.: 4.348 min
Delta R.T.: -0.008 min
Response: 167630
Conc: 2.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
K328-11A


Manual Integrations
APPROVED

Ankita
5/18/2021 4:20:20 PM

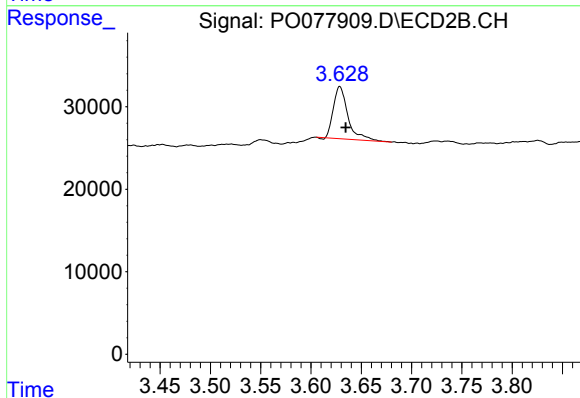


#1 Tetrachloro-m-xylene

R.T.: 3.629 min
Delta R.T.: -0.006 min
Response: 63483
Conc: 2.49 ng/ml

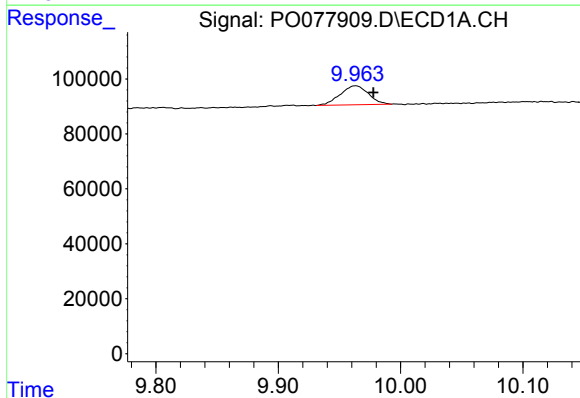


#2 Decachlorobiphenyl

R.T.: 9.963 min
Delta R.T.: -0.015 min
Response: 111417
Conc: 2.70 ng/ml

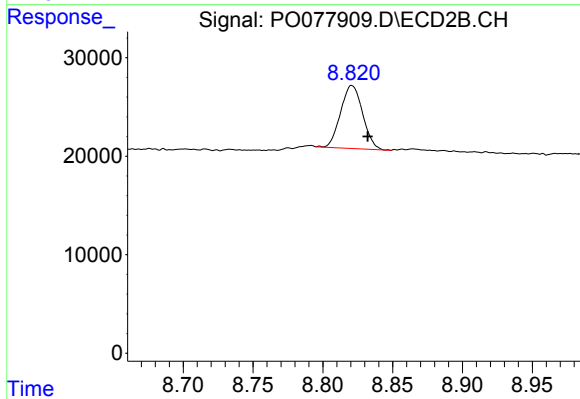

#2 Decachlorobiphenyl

R.T.: 8.821 min
Delta R.T.: -0.011 min
Response: 70346
Conc: 2.93 ng/ml

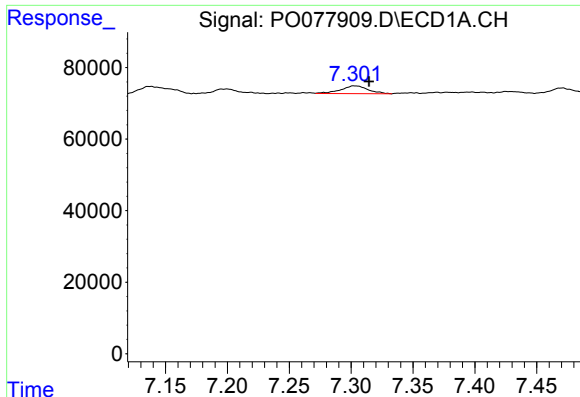


#31 AR-1260-1

R.T.: 7.302 min
Delta R.T.: -0.012 min
Response: 33512
Conc: 13.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
K328-11A


Manual Integrations
APPROVED

Ankita
5/18/2021 4:20:20 PM

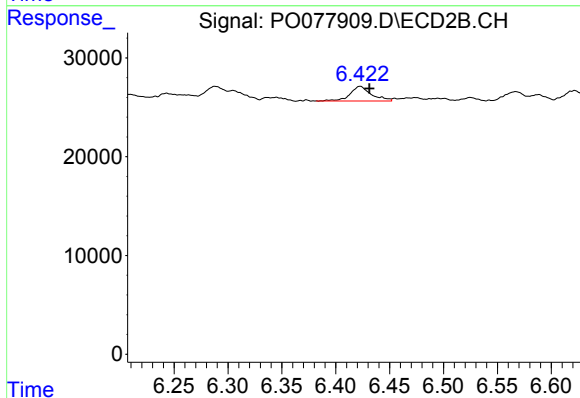


#31 AR-1260-1

R.T.: 6.423 min
Delta R.T.: -0.008 min
Response: 20495
Conc: 13.91 ng/ml

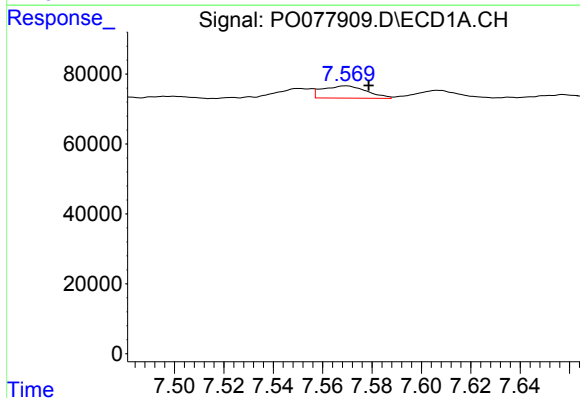


#32 AR-1260-2

R.T.: 7.569 min
Delta R.T.: -0.009 min
Response: 43090
Conc: 15.43 ng/ml m

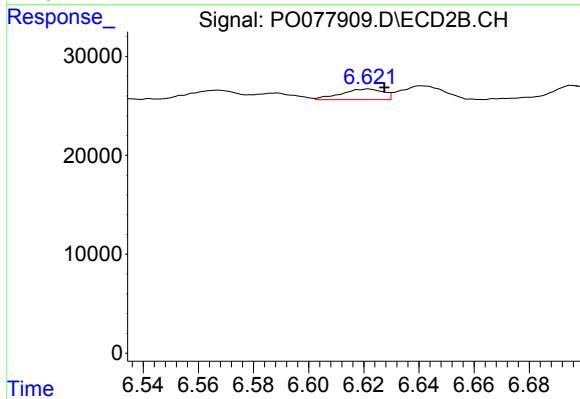

#32 AR-1260-2

R.T.: 6.622 min
Delta R.T.: -0.006 min
Response: 11478
Conc: 6.62 ng/ml

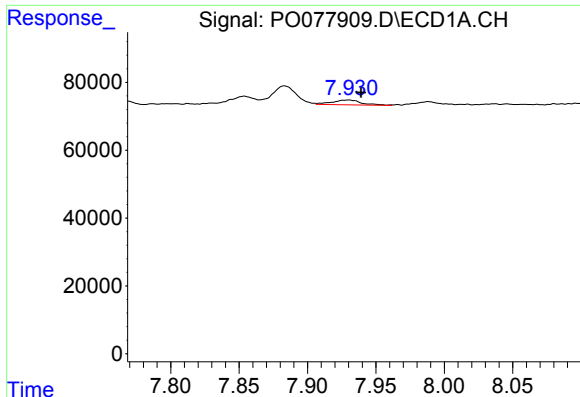


#33 AR-1260-3

R.T.: 7.930 min
Delta R.T.: -0.009 min
Response: 21136
Conc: 10.60 ng/ml m

Instrument :
ECD_O
ClientSampleId :
K328-11A


Manual Integrations
APPROVED

Ankita
5/18/2021 4:20:20 PM

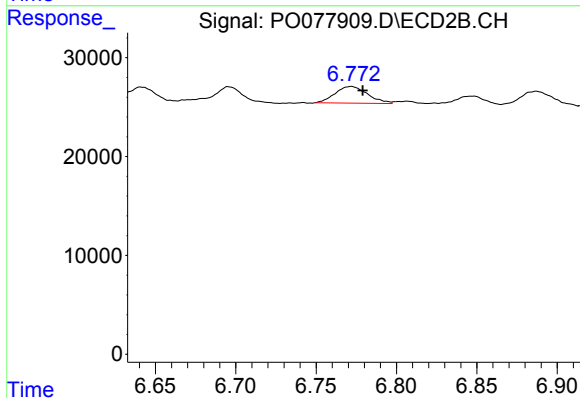


#33 AR-1260-3

R.T.: 6.772 min
Delta R.T.: -0.007 min
Response: 23655
Conc: 14.45 ng/ml

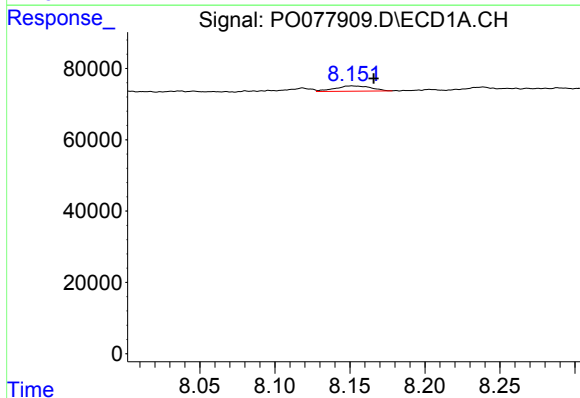


#34 AR-1260-4

R.T.: 8.151 min
Delta R.T.: -0.015 min
Response: 25078
Conc: 11.48 ng/ml m

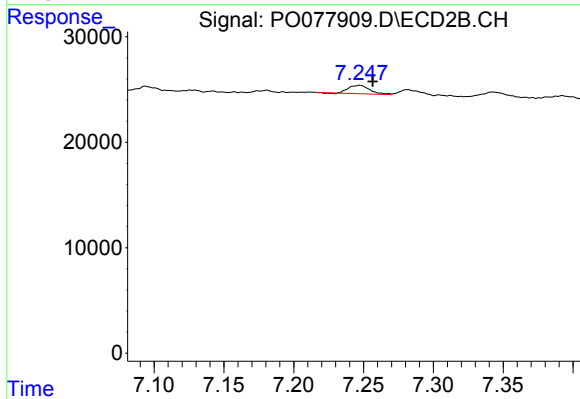

#34 AR-1260-4

R.T.: 7.247 min
Delta R.T.: -0.009 min
Response: 8361
Conc: 6.91 ng/ml

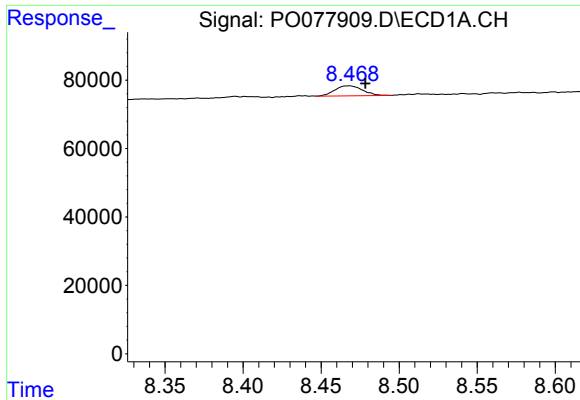


#35 AR-1260-5

R.T.: 8.468 min
Delta R.T.: -0.010 min
Response: 36118
Conc: 8.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
K328-11A

Manual Integrations
APPROVED

Ankita
5/18/2021 4:20:20 PM

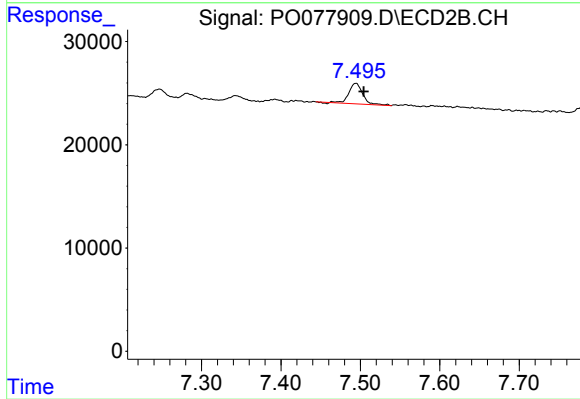

#35 AR-1260-5

R.T.: 7.494 min
Delta R.T.: -0.010 min
Response: 24155
Conc: 8.50 ng/ml