

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051721\
 Data File : P0077918.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 May 2021 3:19
 Operator : DD\AJ
 Sample : M2422-15 10X
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 K328-15A

Manual Integrations
 APPROVED

Ankita
 5/18/2021 4:20:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 04:57:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 14 05:52:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.348	3.628	125304	36745	2.135m	1.444m#
2) SA Decachlor...	9.961f	8.821	81174	57988	1.964	2.413
Target Compounds						
41) L9 AR-1268-1	8.738	7.777	79662	50485	13.631m	13.897
42) L9 AR-1268-2	8.818	7.840	69031	62761	12.508	19.036 #
43) L9 AR-1268-3	9.003	8.044	35264	25417	7.764	8.877
44) L9 AR-1268-4	9.369	8.334	20395	21021	11.040	17.202m#
45) L9 AR-1268-5	9.697	8.604	116353	81653	7.909	9.509

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051721\
Data File : P0077918.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 May 2021 3:19
Operator : DD\AJ
Sample : M2422-15 10X
Misc :
ALS Vial : 52 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
K328-15A


Manual Integrations
APPROVED

Ankita
5/18/2021 4:20:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 04:57:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 14 05:52:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

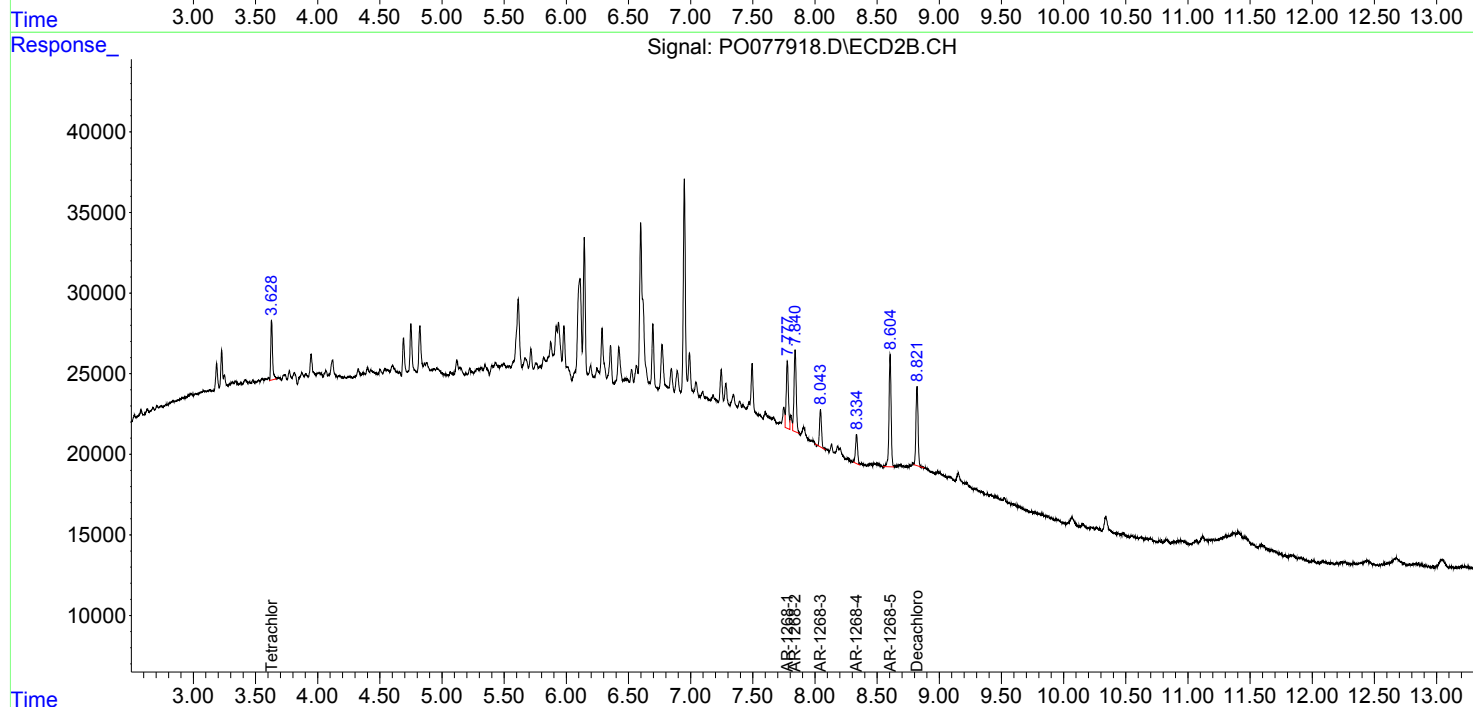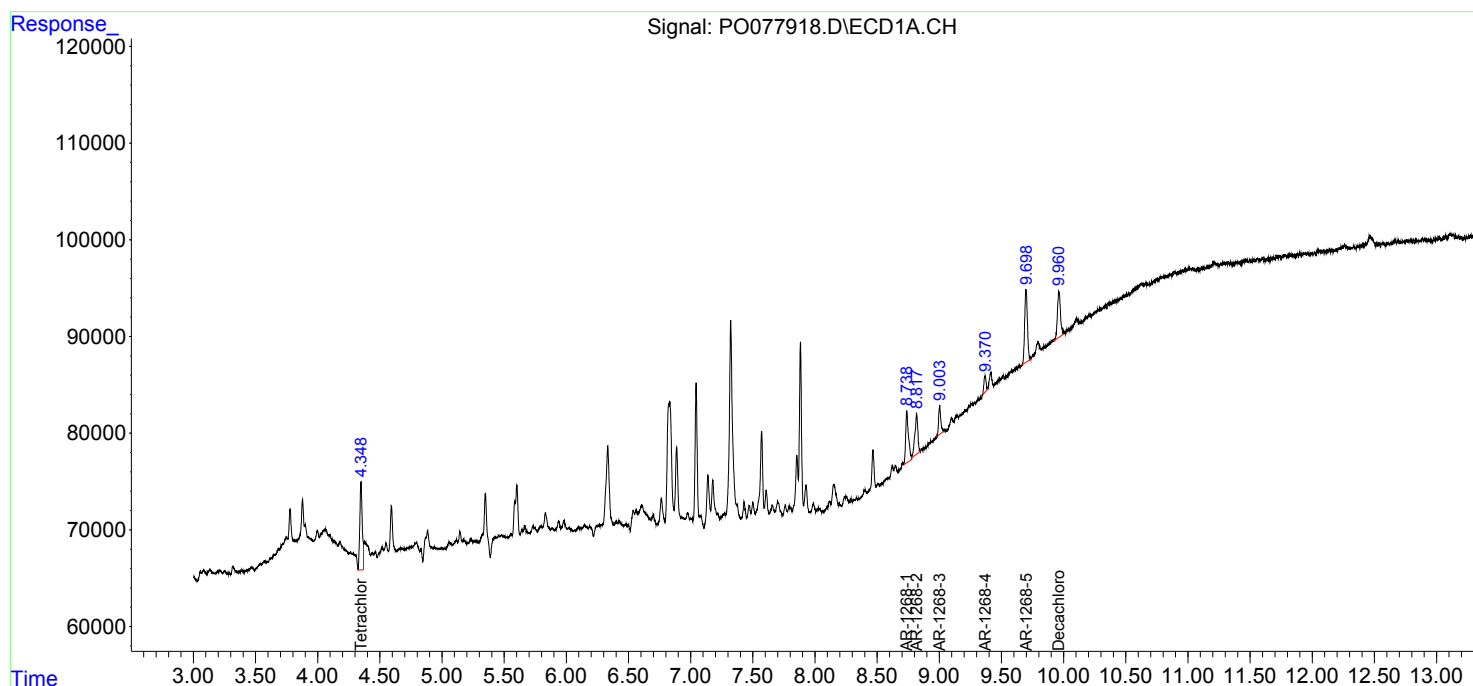

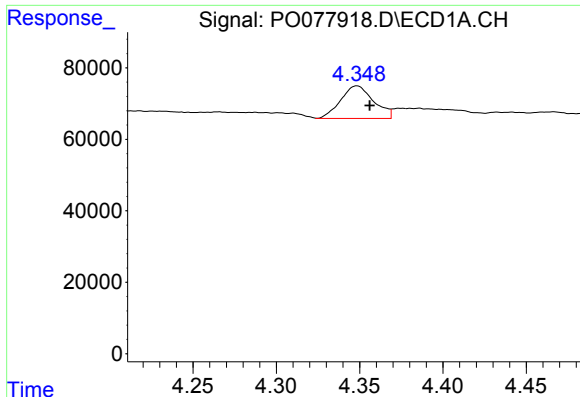


#1 Tetrachloro-m-xylene

R.T.: 4.348 min
Delta R.T.: -0.008 min
Response: 125304
Conc: 2.13 ng/ml m

Instrument :
ECD_O
ClientSampleId :
K328-15A


Manual Integrations
APPROVED

Ankita
5/18/2021 4:20:33 PM

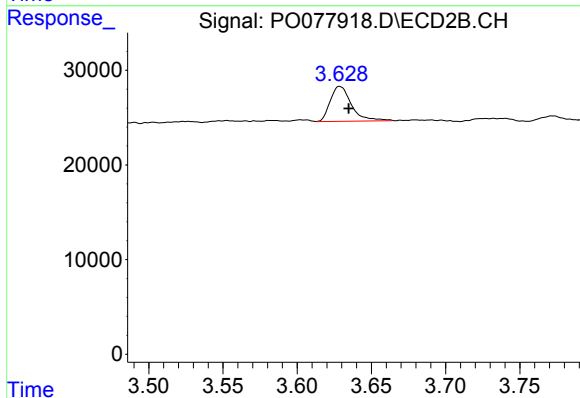


#1 Tetrachloro-m-xylene

R.T.: 3.628 min
Delta R.T.: -0.007 min
Response: 36745
Conc: 1.44 ng/ml m

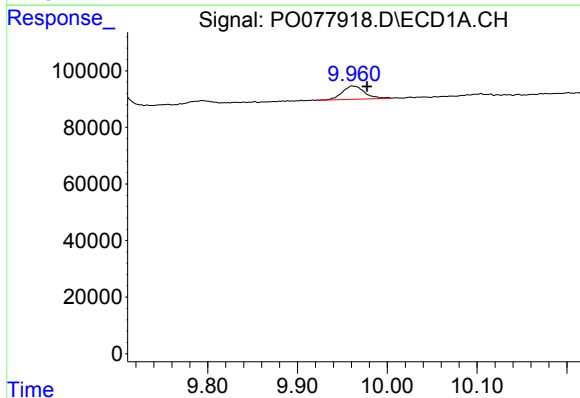


#2 Decachlorobiphenyl

R.T.: 9.961 min
Delta R.T.: -0.017 min
Response: 81174
Conc: 1.96 ng/ml

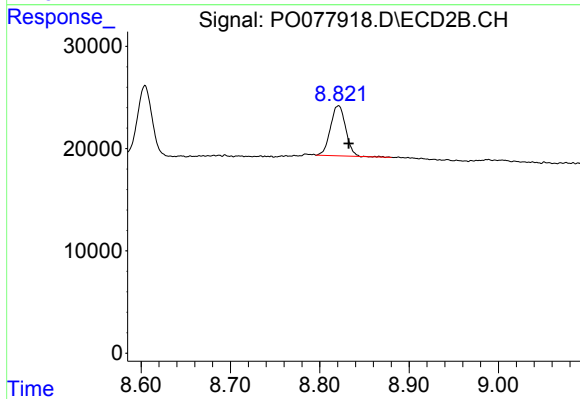

#2 Decachlorobiphenyl

R.T.: 8.821 min
Delta R.T.: -0.011 min
Response: 57988
Conc: 2.41 ng/ml

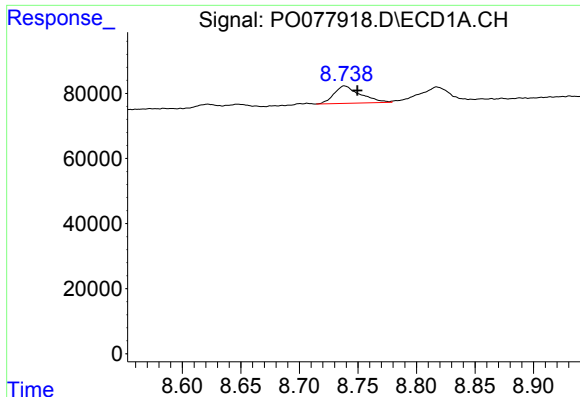


#41 AR-1268-1

R.T.: 8.738 min
Delta R.T.: -0.012 min
Response: 79662
Conc: 13.63 ng/ml m

Instrument :
ECD_O
ClientSampleId :
K328-15A


Manual Integrations
APPROVED

Ankita
5/18/2021 4:20:33 PM

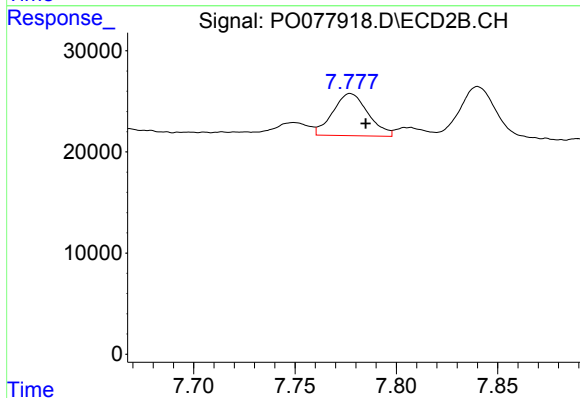


#41 AR-1268-1

R.T.: 7.777 min
Delta R.T.: -0.008 min
Response: 50485
Conc: 13.90 ng/ml

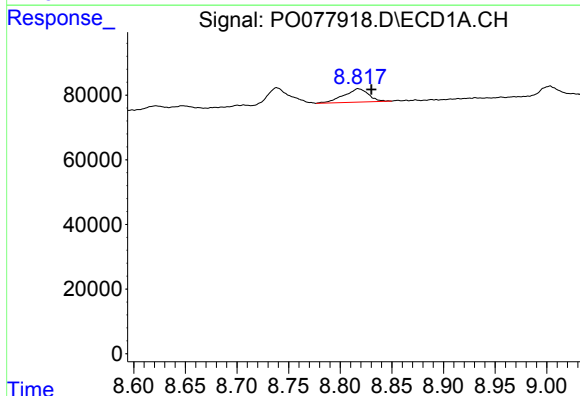


#42 AR-1268-2

R.T.: 8.818 min
Delta R.T.: -0.013 min
Response: 69031
Conc: 12.51 ng/ml

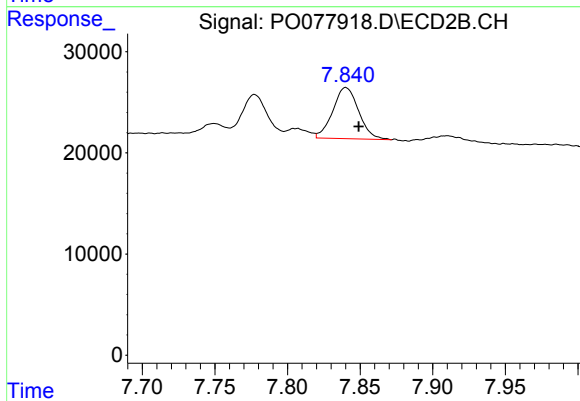

#42 AR-1268-2

R.T.: 7.840 min
Delta R.T.: -0.009 min
Response: 62761
Conc: 19.04 ng/ml

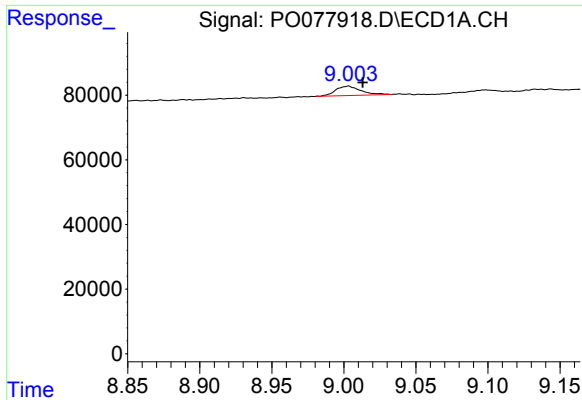


#43 AR-1268-3

R.T.: 9.003 min
Delta R.T.: -0.010 min
Response: 35264
Conc: 7.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
K328-15A


Manual Integrations
APPROVED

Ankita
5/18/2021 4:20:33 PM

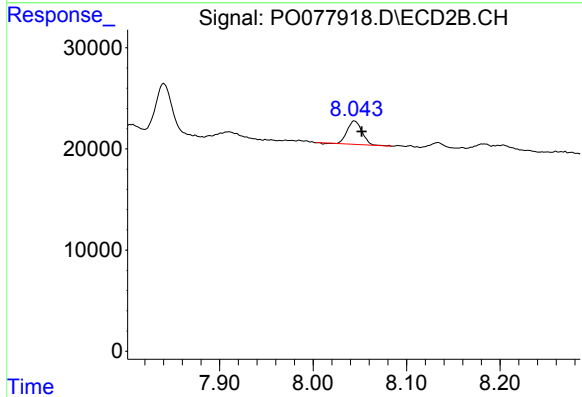


#43 AR-1268-3

R.T.: 8.044 min
Delta R.T.: -0.008 min
Response: 25417
Conc: 8.88 ng/ml

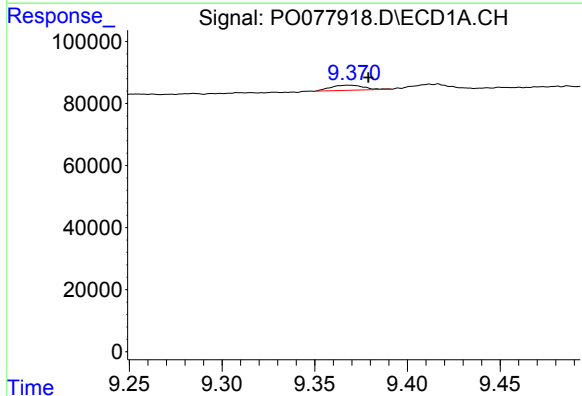


#44 AR-1268-4

R.T.: 9.369 min
Delta R.T.: -0.010 min
Response: 20395
Conc: 11.04 ng/ml

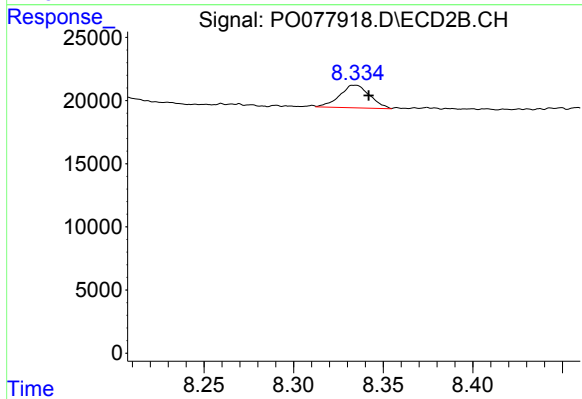

#44 AR-1268-4

R.T.: 8.334 min
Delta R.T.: -0.008 min
Response: 21021
Conc: 17.20 ng/ml m

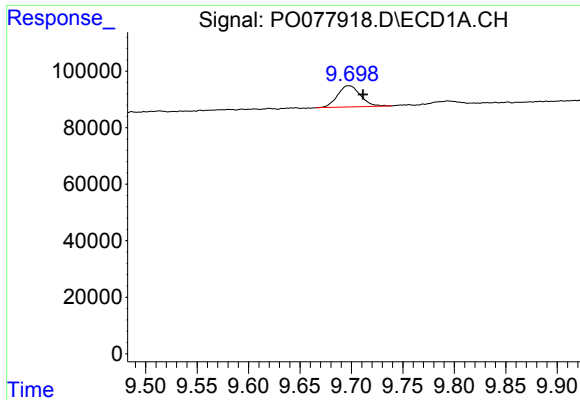


#45 AR-1268-5

R.T.: 9.697 min
Delta R.T.: -0.014 min
Response: 116353
Conc: 7.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
K328-15A

Manual Integrations
APPROVED

Ankita
5/18/2021 4:20:33 PM

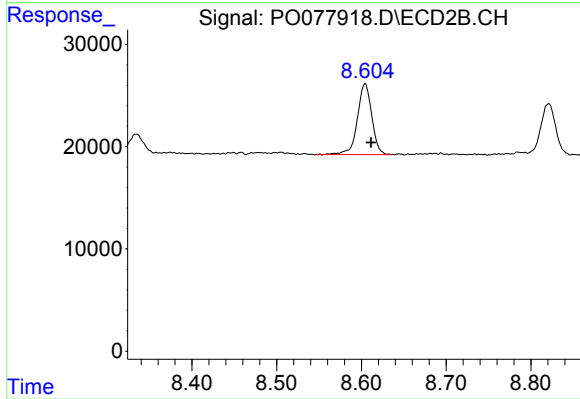

#45 AR-1268-5

R.T.: 8.604 min
Delta R.T.: -0.007 min
Response: 81653
Conc: 9.51 ng/ml