

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051724\
 Data File : P0103941.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2024 03:06
 Operator : YP/AJ
 Sample : P2511-09 10X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1598

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/20/2024
 Supervised By :Ankita Jodhani 05/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 04:12:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 16 04:14:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.449	3.580	18995128	8180135	2.468m	3.247m#
2) SA Decachlor...	10.209	8.536	5319329	1245681	1.122m	0.958m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051724\
Data File : PO103941.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2024 03:06
Operator : YP/AJ
Sample : P2511-09 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
1598


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/20/2024
Supervised By :Ankita Jodhani 05/20/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 04:12:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050624.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 16 04:14:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

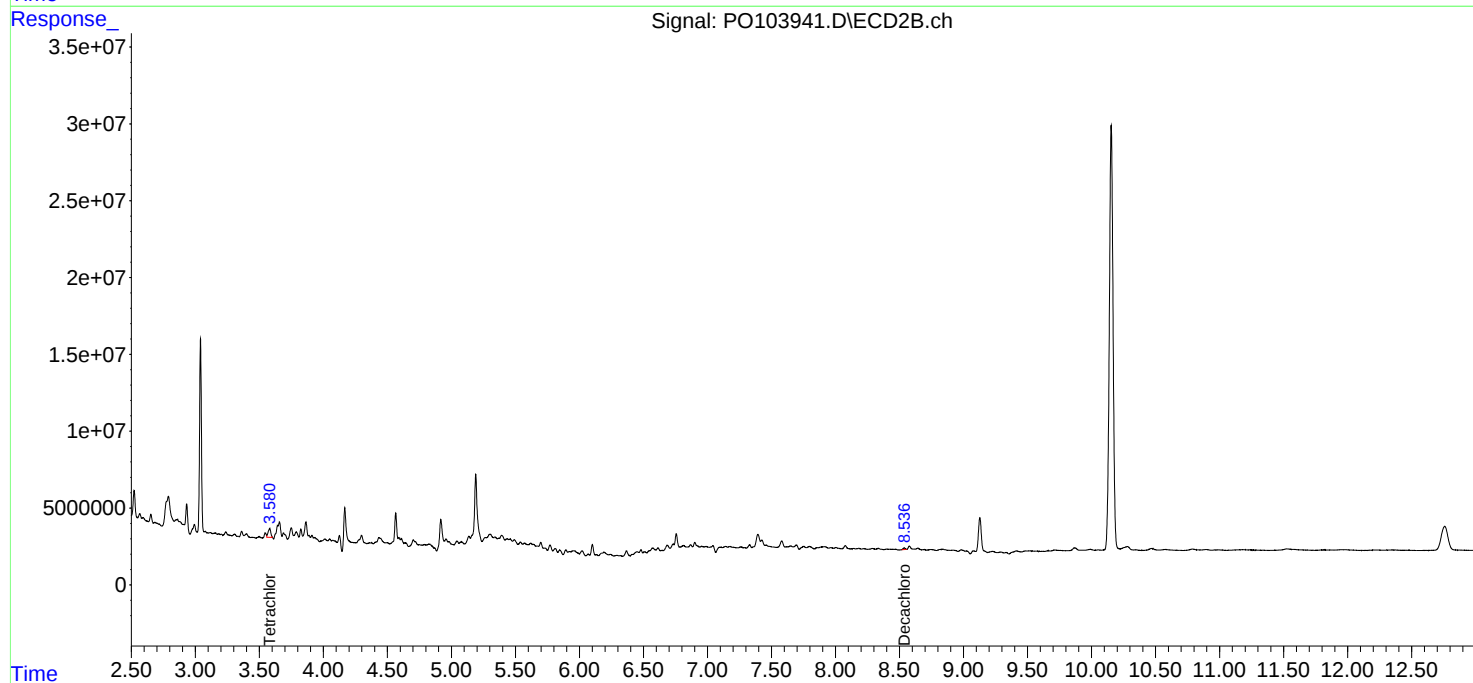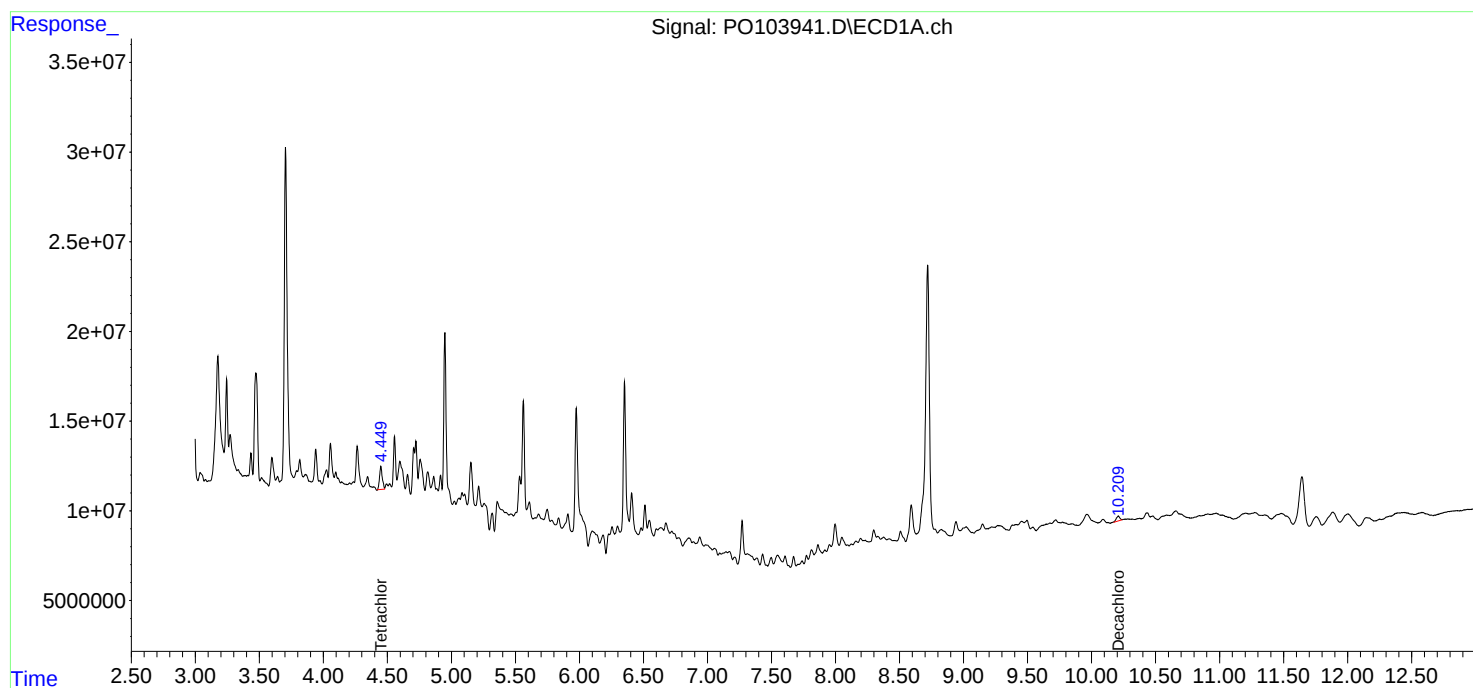

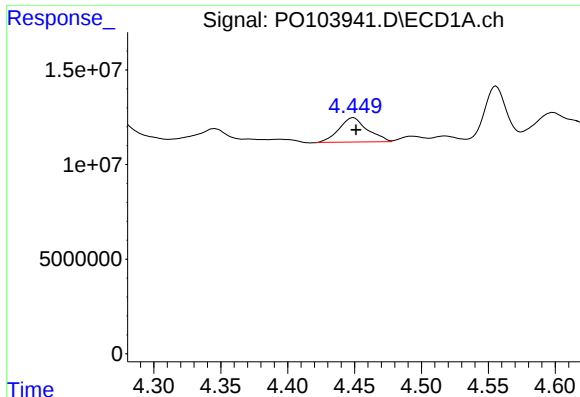


#1 Tetrachloro-m-xylene

R.T.: 4.449 min
Delta R.T.: -0.002 min
Response: 18995128
Conc: 2.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
1598


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/20/2024
Supervised By :Ankita Jodhani 05/20/2024

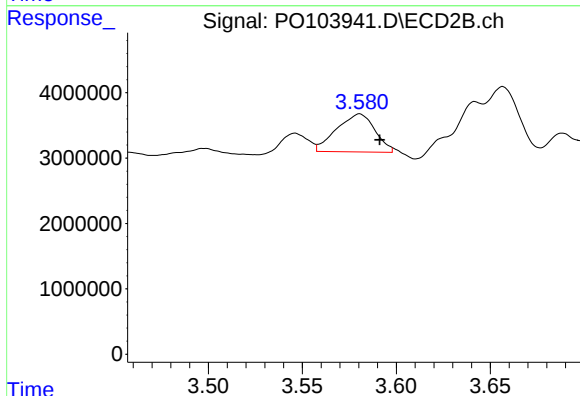


#1 Tetrachloro-m-xylene

R.T.: 3.580 min
Delta R.T.: -0.011 min
Response: 8180135
Conc: 3.25 ng/ml m

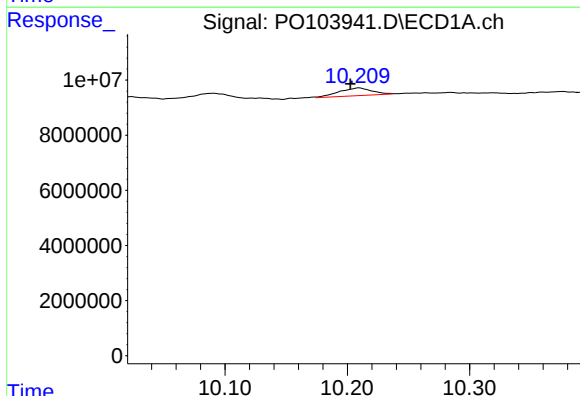

#2 Decachlorobiphenyl

R.T.: 10.209 min
Delta R.T.: 0.006 min
Response: 5319329
Conc: 1.12 ng/ml m

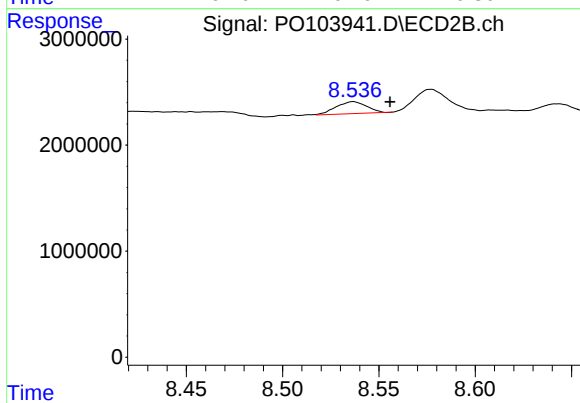

#2 Decachlorobiphenyl

R.T.: 8.536 min
Delta R.T.: -0.020 min
Response: 1245681
Conc: 0.96 ng/ml m