

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051724\
 Data File : P0103942.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2024 03:23
 Operator : YP/AJ
 Sample : P2501-01 (Sig #1); P2501-09 (Sig #2)
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 33351

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/20/2024
 Supervised By :Ankita Jodhani 05/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 04:12:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 16 04:14:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.449	3.583	108.2E6	49160595	14.065m	19.514 #
2) SA Decachlor...	10.219	8.554	178.8E6	19100086	37.723m	14.682m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051724\
Data File : PO103942.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2024 03:23
Operator : YP/AJ
Sample : P2501-01 (Sig #1); P2501-09 (Sig #2)
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
33351


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/20/2024
Supervised By :Ankita Jodhani 05/20/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 04:12:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050624.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 16 04:14:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

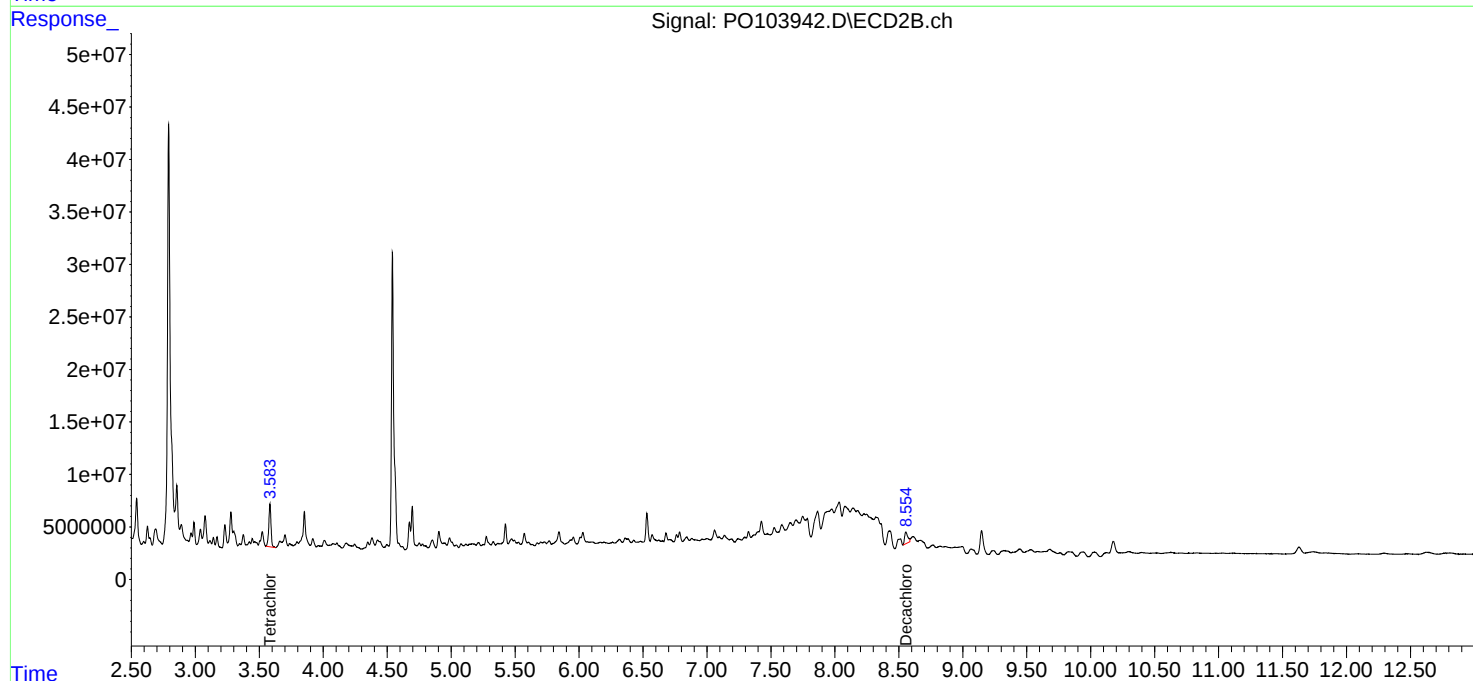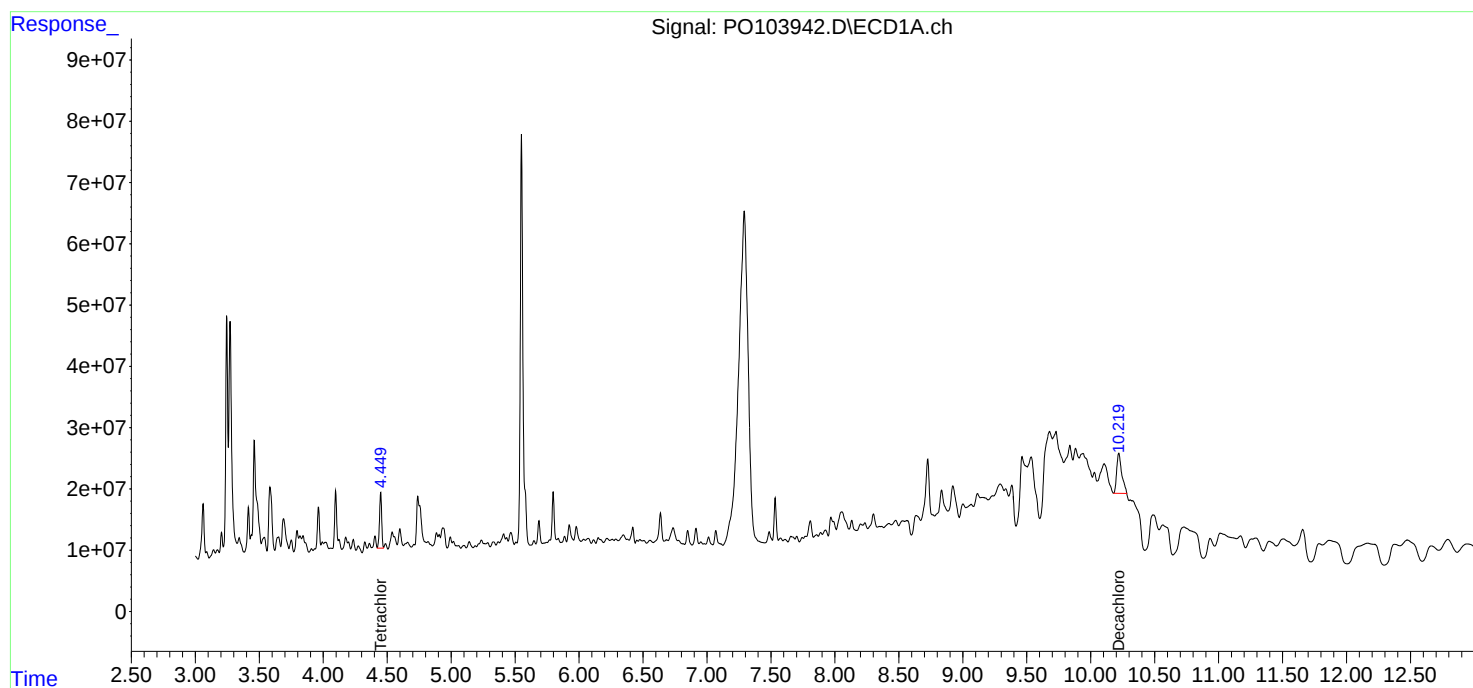

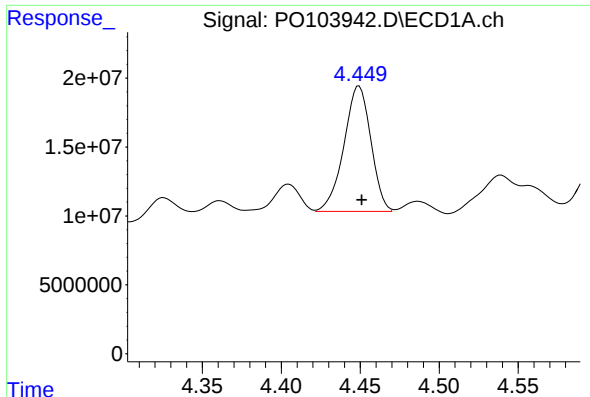


#1 Tetrachloro-m-xylene

R.T.: 4.449 min
Delta R.T.: -0.002 min
Response: 108238632
Conc: 14.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
33351


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/20/2024
Supervised By :Ankita Jodhani 05/20/2024

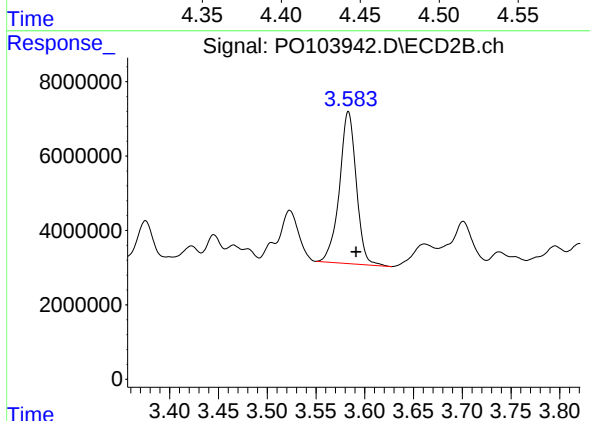


#1 Tetrachloro-m-xylene

R.T.: 3.583 min
Delta R.T.: -0.008 min
Response: 49160595
Conc: 19.51 ng/ml

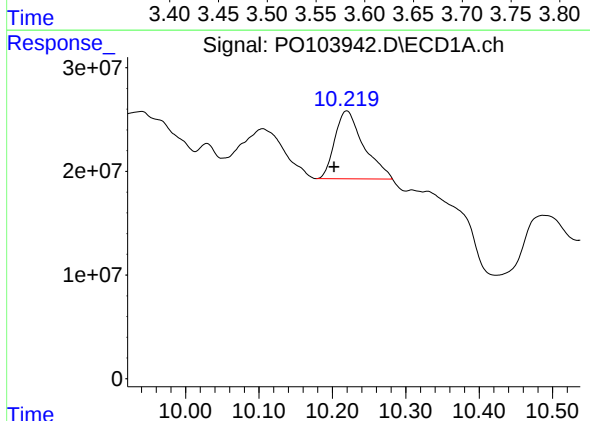

#2 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: 0.017 min
Response: 178818094
Conc: 37.72 ng/ml m

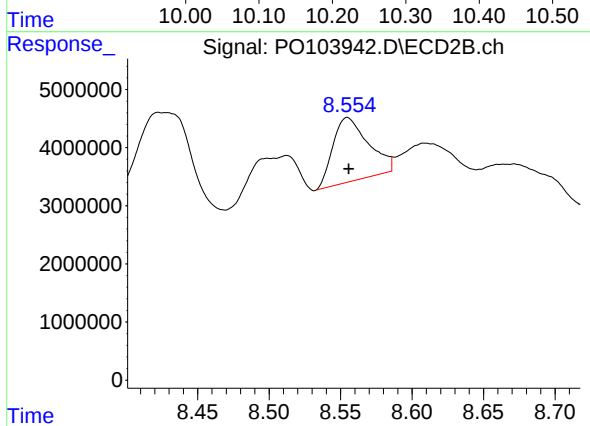

#2 Decachlorobiphenyl

R.T.: 8.554 min
Delta R.T.: -0.001 min
Response: 19100086
Conc: 14.68 ng/ml m