

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051725\
 Data File : P0111141.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2025 15:08
 Operator : YP/AJ
 Sample : Q2032-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-37

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/19/2025
 Supervised By :mohammad ahmed 05/20/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 15:38:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 07:11:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.682	3.679	110.3E6	93333301	18.748	17.121
2) SA Decachlor...	8.724	8.674	64418809	24007790	12.477	12.976m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051725\
Data File : P0111141.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2025 15:08
Operator : YP/AJ
Sample : Q2032-07
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-37


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/19/2025
Supervised By :mohammad ahmed 05/20/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 15:38:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 07:11:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

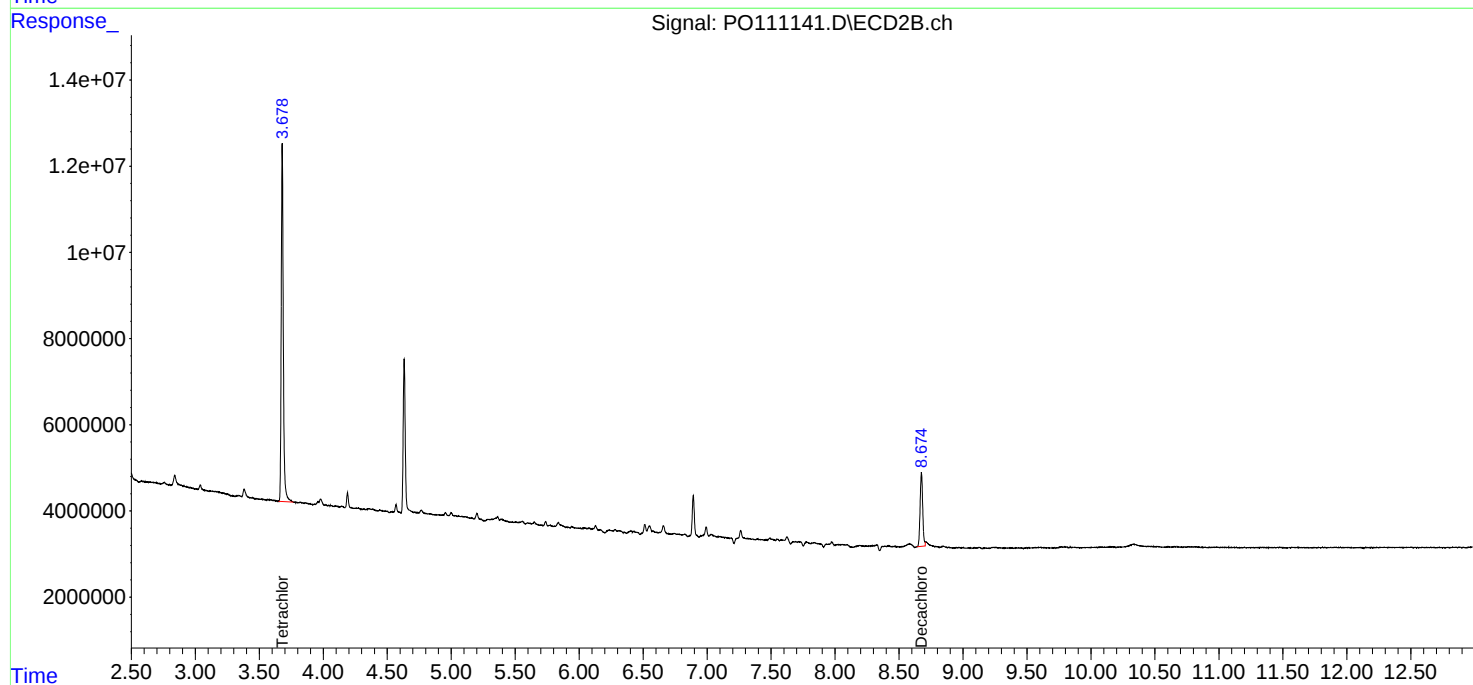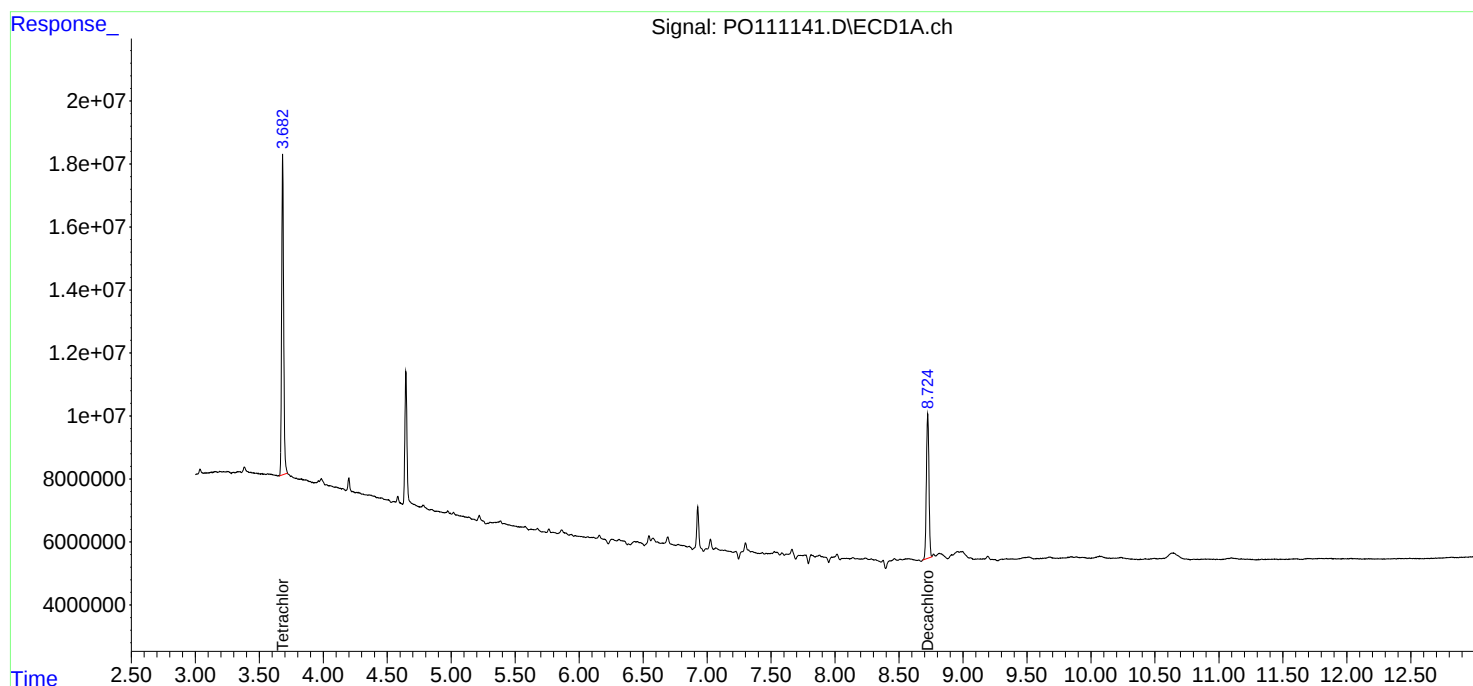

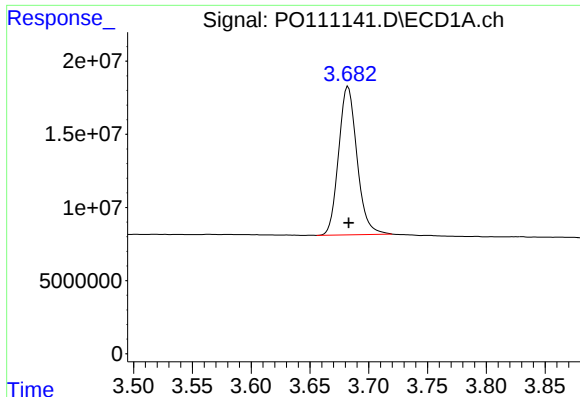

#1 Tetrachloro-m-xylene

R.T.: 3.682 min
Delta R.T.: 0.000 min
Response: 110300379
Conc: 18.75 ng/ml

Instrument :

ECD_O

ClientSampleId :


TP-37

Manual Integrations

APPROVED


Reviewed By :Yogesh Patel 05/19/2025

Supervised By :mohammad ahmed 05/20/2025

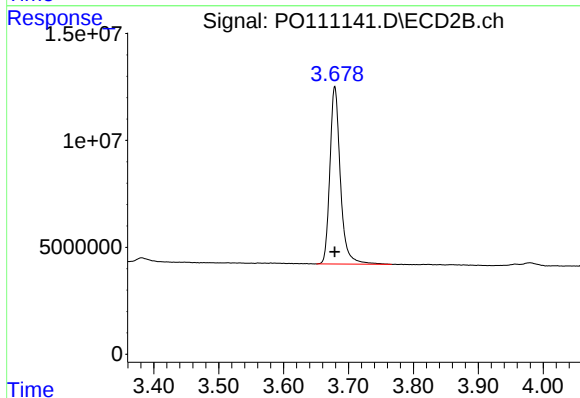


#1 Tetrachloro-m-xylene

R.T.: 3.679 min
Delta R.T.: 0.000 min
Response: 93333301
Conc: 17.12 ng/ml

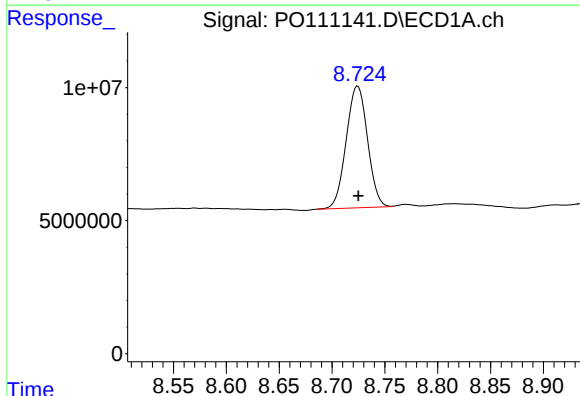

#2 Decachlorobiphenyl

R.T.: 8.724 min
Delta R.T.: 0.000 min
Response: 64418809
Conc: 12.48 ng/ml

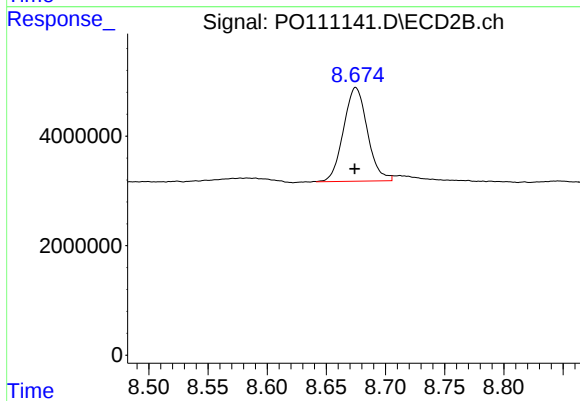

#2 Decachlorobiphenyl

R.T.: 8.674 min
Delta R.T.: 0.000 min
Response: 24007790
Conc: 12.98 ng/ml m