

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051822\
 Data File : P0086171.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 May 2022 5:54
 Operator : YP\AJ
 Sample : N2909-02 10X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HED845X-1-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 07:33:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 12 05:35:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.479	3.678	201609	74534	1.985	1.710
2) SA Decachlor...	10.337	8.741	133818	60887	2.525	1.794 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051822\
Data File : P0086171.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 May 2022 5:54
Operator : YP\AJ
Sample : N2909-02 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HED845X-1-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 07:33:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 12 05:35:26 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

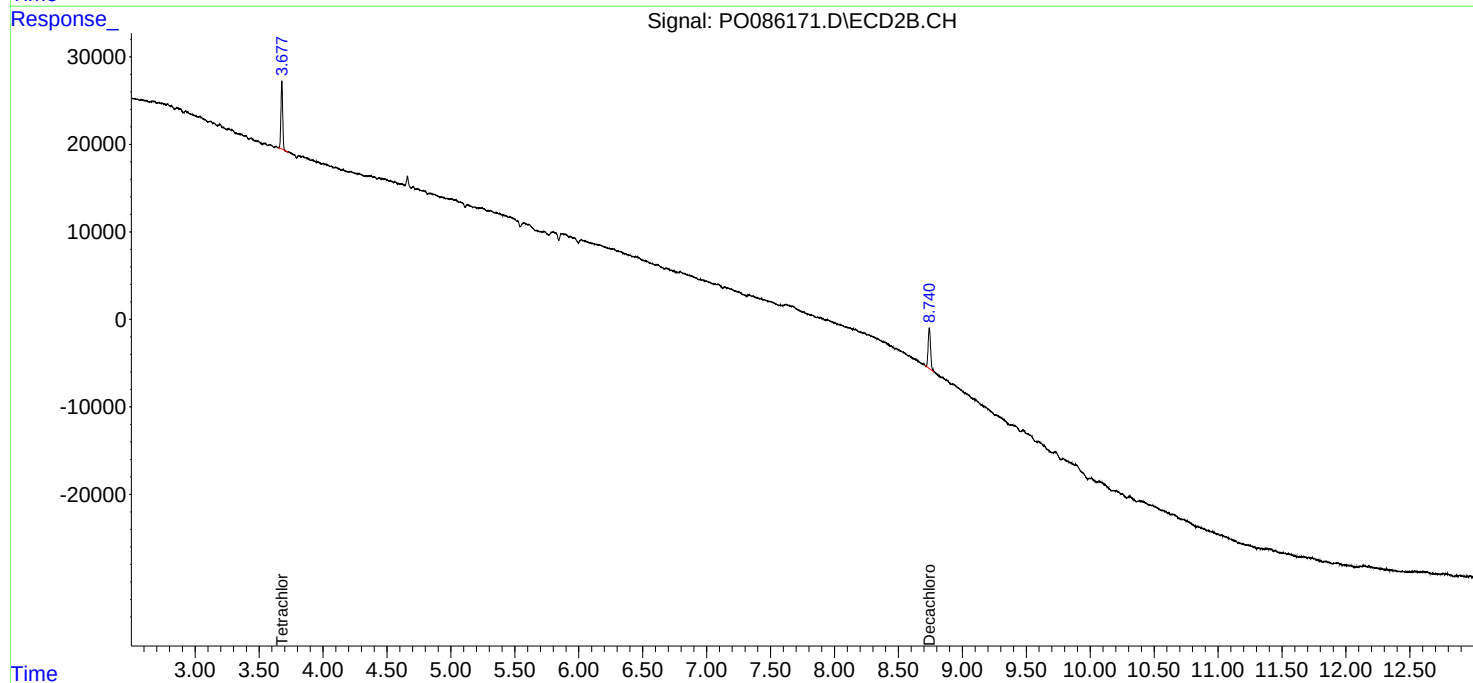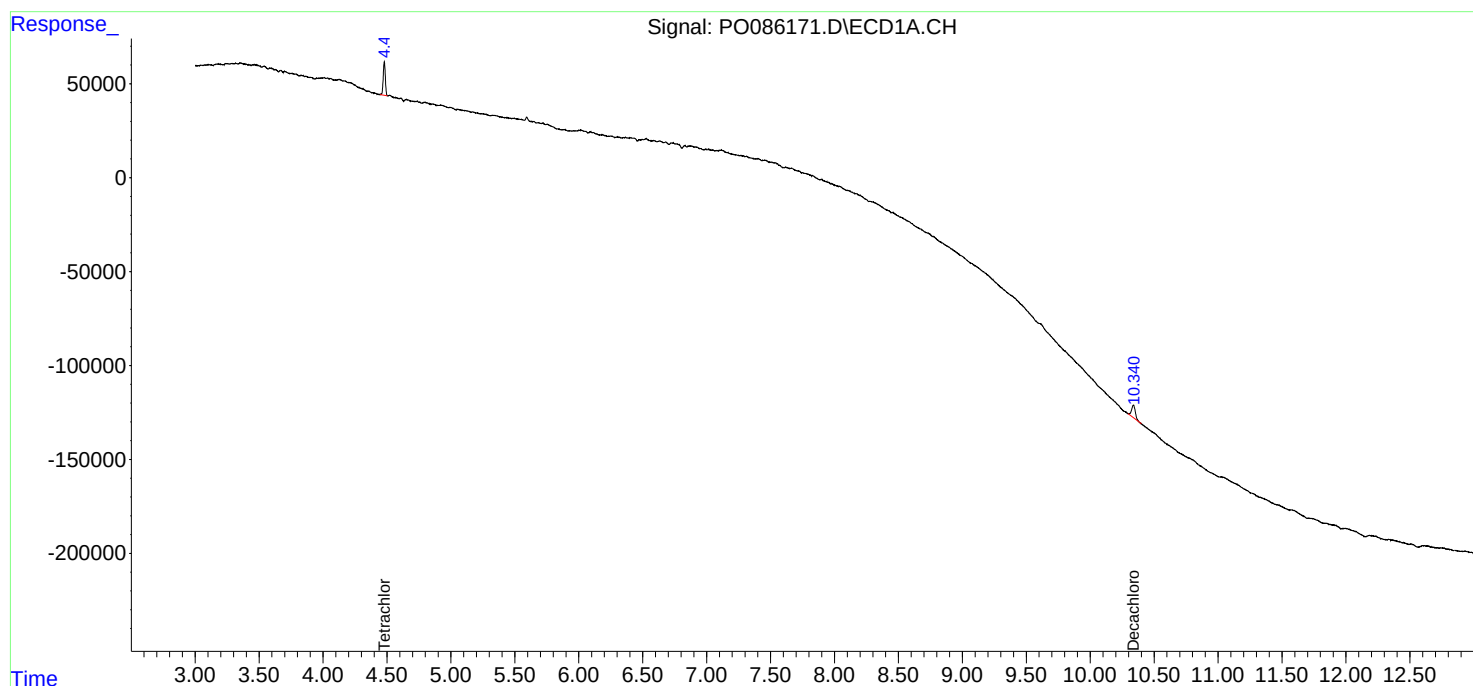


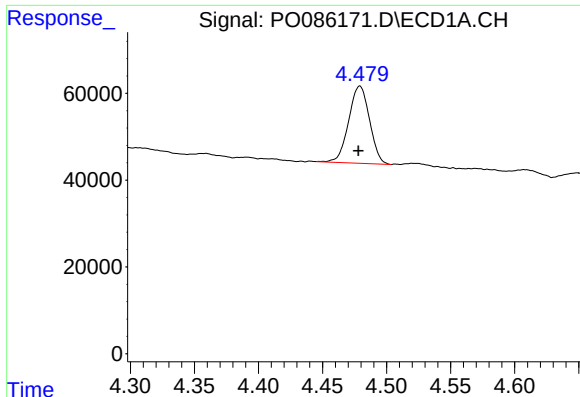

#1 Tetrachloro-m-xylene


R.T.: 4.479 min
Delta R.T.: 0.001 min
Response: 201609
Conc: 1.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
HED845X-1-2

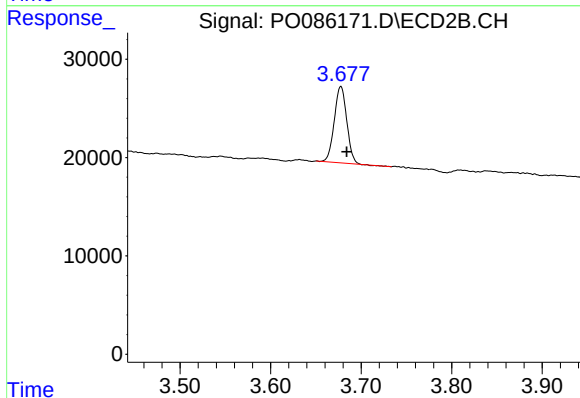


#1 Tetrachloro-m-xylene

R.T.: 3.678 min
Delta R.T.: -0.006 min
Response: 74534
Conc: 1.71 ng/ml

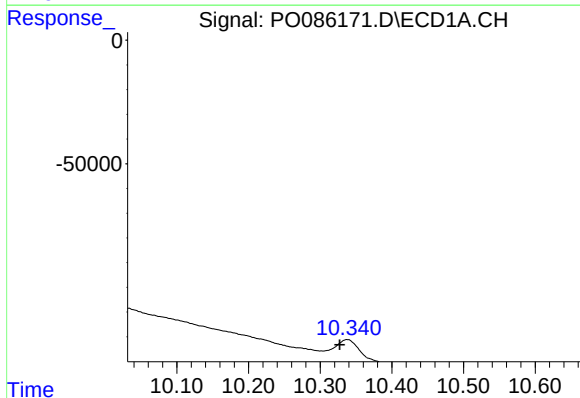

#2 Decachlorobiphenyl

R.T.: 10.337 min
Delta R.T.: 0.010 min
Response: 133818
Conc: 2.53 ng/ml

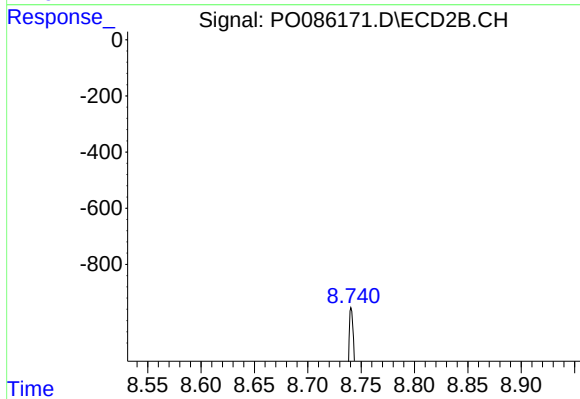

#2 Decachlorobiphenyl

R.T.: 8.741 min
Delta R.T.: -0.018 min
Response: 60887
Conc: 1.79 ng/ml