

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051921\
 Data File : P0077980.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 May 2021 10:55
 Operator : DD\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Ankita
 5/20/2021 2:05:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 12:04:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.345	3.623	3629602	1566244	49.110	51.835m
2) SA Decachlor...	9.959	8.817	2396735	1385950	48.477	47.664
Target Compounds						
26) L6 AR-1254-1	6.533	5.712	1211874	787133	488.266m	456.415
27) L6 AR-1254-2	6.761	5.870	1905386	736062	491.011m	459.186
28) L6 AR-1254-3	7.136	6.283	1928072	1127079	491.436m	472.224
29) L6 AR-1254-4	7.429	6.520	1393481	692748	513.121m	477.145
30) L6 AR-1254-5	7.853	6.943	1500385	1067572	513.043m	469.689

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051921\
Data File : P0077980.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 May 2021 10:55
Operator : DD\AJ
Sample : AR1254CCC500
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
5/20/2021 2:05:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 12:04:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

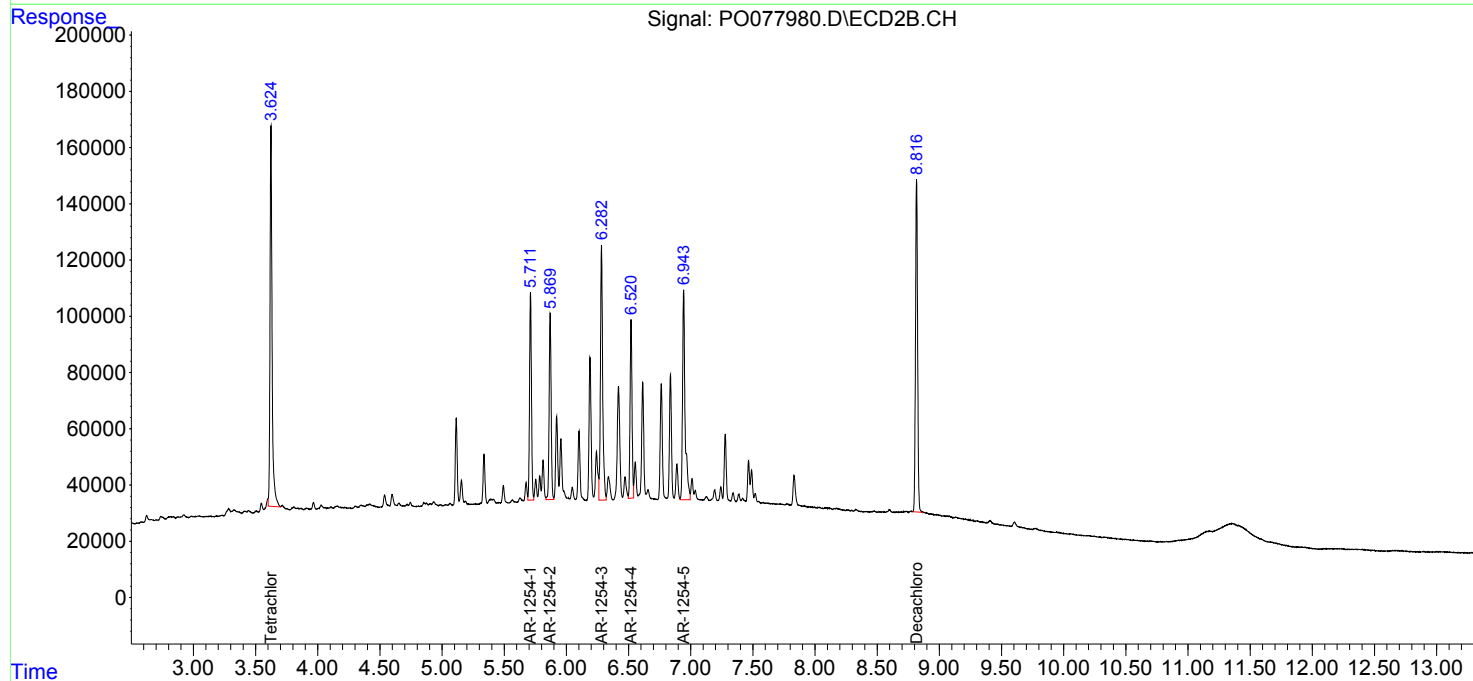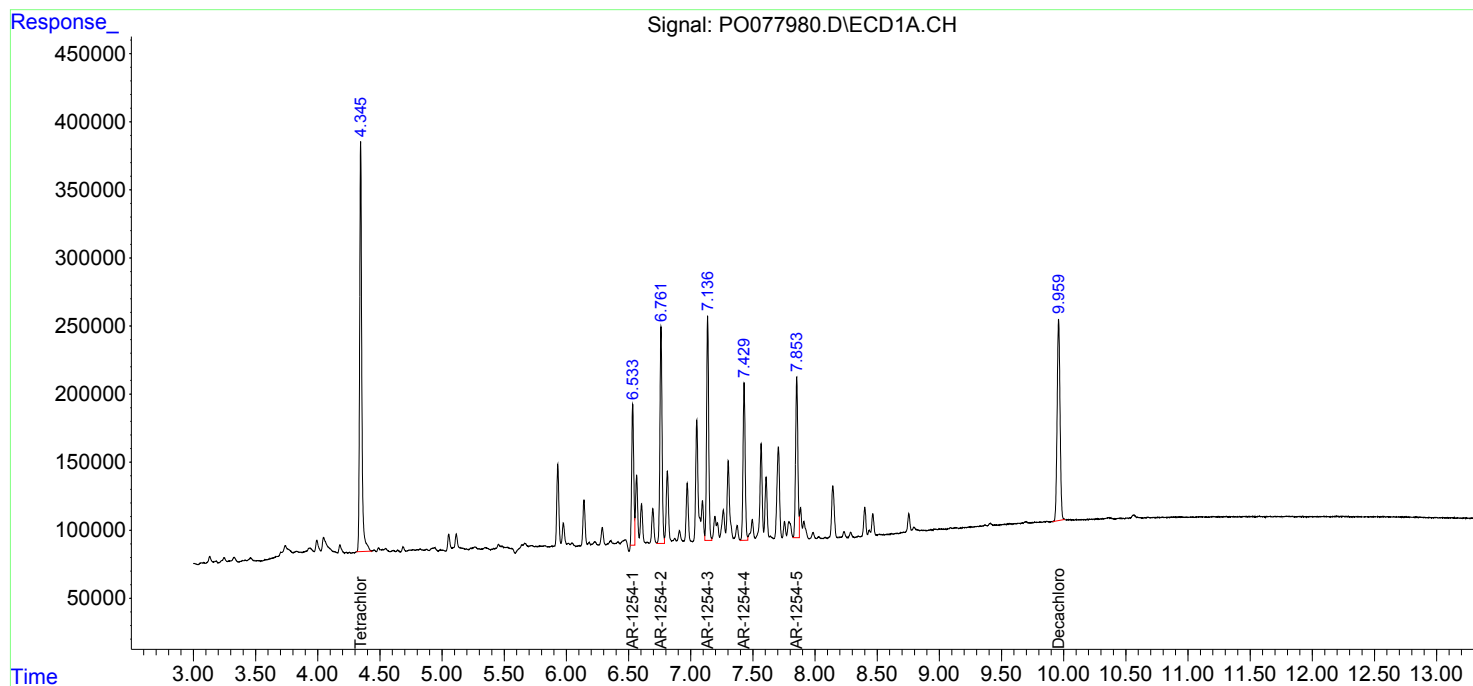

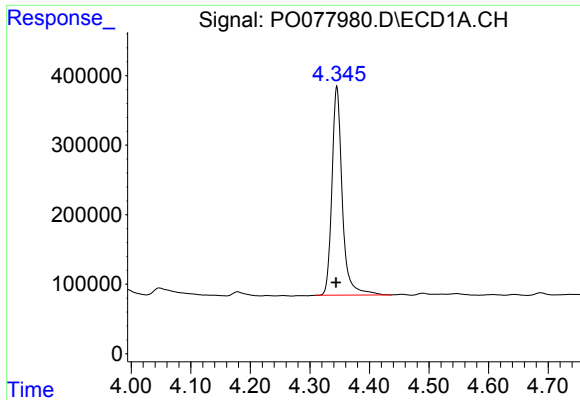


#1 Tetrachloro-m-xylene

R.T.: 4.345 min
Delta R.T.: 0.001 min
Response: 3629602
Conc: 49.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
5/20/2021 2:05:44 PM

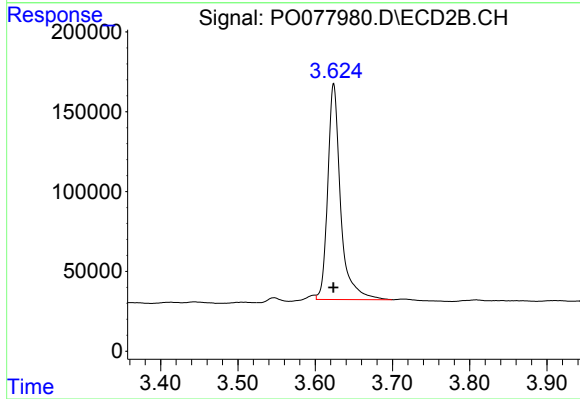


#1 Tetrachloro-m-xylene

R.T.: 3.623 min
Delta R.T.: 0.000 min
Response: 1566244
Conc: 51.83 ng/ml m

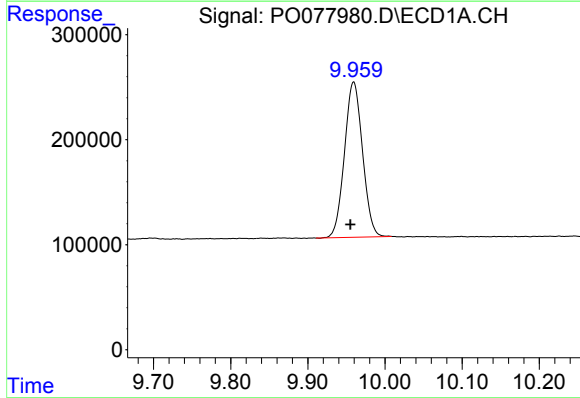


#2 Decachlorobiphenyl

R.T.: 9.959 min
Delta R.T.: 0.004 min
Response: 2396735
Conc: 48.48 ng/ml

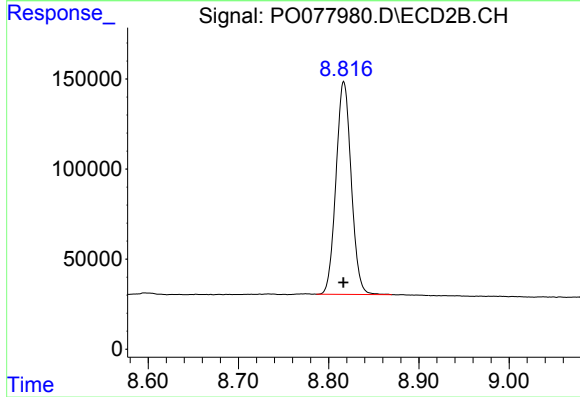

#2 Decachlorobiphenyl

R.T.: 8.817 min
Delta R.T.: 0.000 min
Response: 1385950
Conc: 47.66 ng/ml

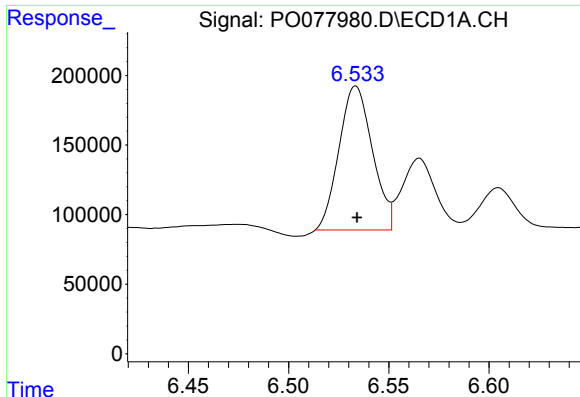


#26 AR-1254-1

R.T.: 6.533 min
Delta R.T.: 0.000 min
Response: 1211874
Conc: 488.27 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
5/20/2021 2:05:44 PM

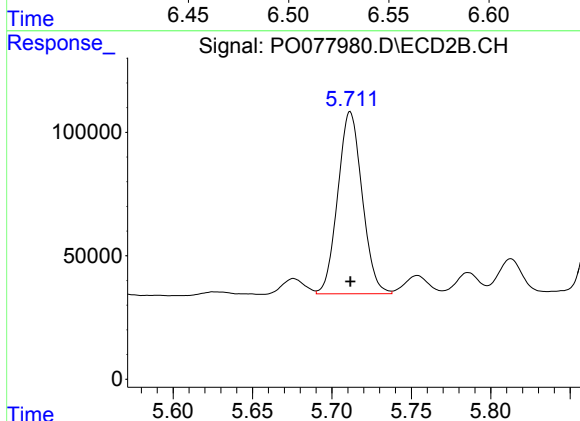


#26 AR-1254-1

R.T.: 5.712 min
Delta R.T.: 0.000 min
Response: 787133
Conc: 456.42 ng/ml

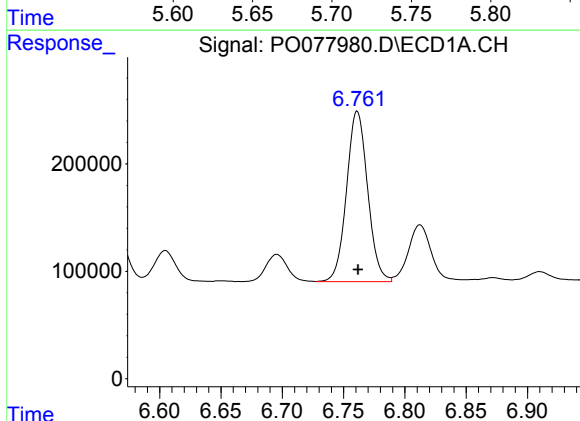


#27 AR-1254-2

R.T.: 6.761 min
Delta R.T.: -0.001 min
Response: 1905386
Conc: 491.01 ng/ml m

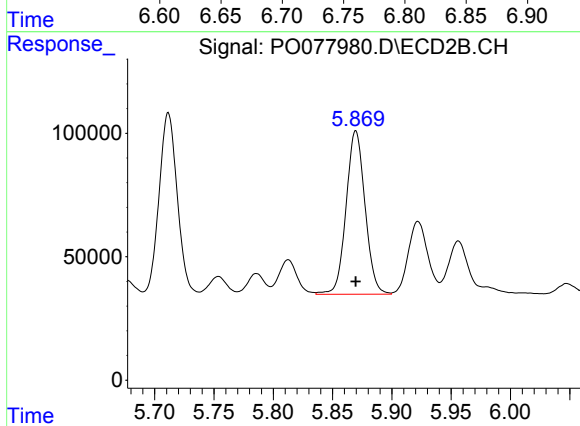

#27 AR-1254-2

R.T.: 5.870 min
Delta R.T.: 0.000 min
Response: 736062
Conc: 459.19 ng/ml

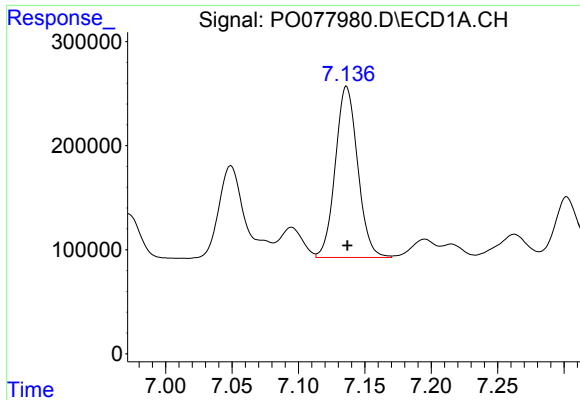


#28 AR-1254-3

R.T.: 7.136 min
Delta R.T.: -0.001 min
Response: 1928072
Conc: 491.44 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
5/20/2021 2:05:44 PM

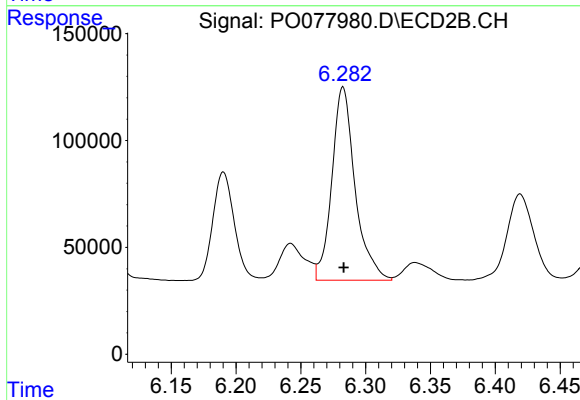


#28 AR-1254-3

R.T.: 6.283 min
Delta R.T.: 0.000 min
Response: 1127079
Conc: 472.22 ng/ml

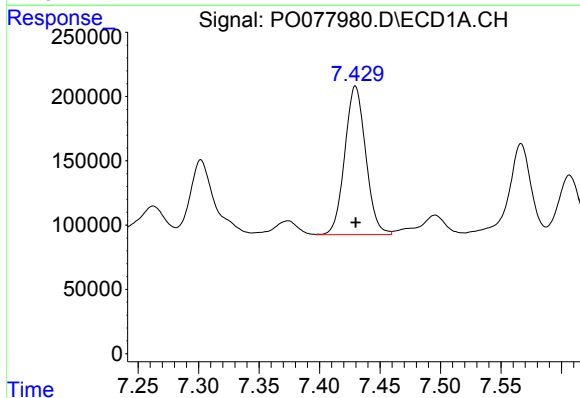


#29 AR-1254-4

R.T.: 7.429 min
Delta R.T.: 0.000 min
Response: 1393481
Conc: 513.12 ng/ml m

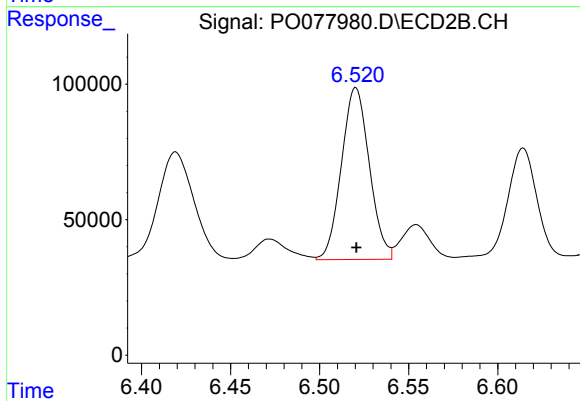

#29 AR-1254-4

R.T.: 6.520 min
Delta R.T.: 0.000 min
Response: 692748
Conc: 477.15 ng/ml

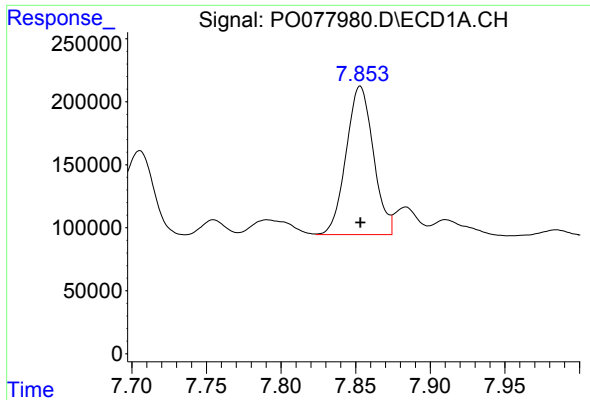


#30 AR-1254-5

R.T.: 7.853 min
Delta R.T.: 0.000 min
Response: 1500385
Conc: 513.04 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Ankita
5/20/2021 2:05:44 PM

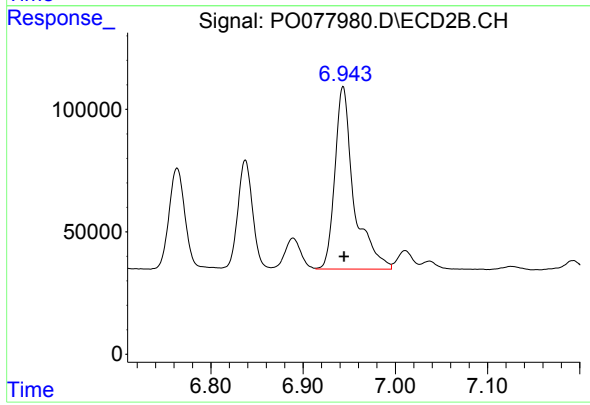

#30 AR-1254-5

R.T.: 6.943 min
Delta R.T.: -0.001 min
Response: 1067572
Conc: 469.69 ng/ml