

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051921\
 Data File : P0077983.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 May 2021 11:47
 Operator : DD\AJ
 Sample : M2368-01DL 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-33184-33186DL

Manual Integrations
 APPROVED

Ankita
 5/20/2021 2:05:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 12:06:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.344	3.622	452512	48705	6.123	1.612 #
2) SA Decachlor...	9.959	8.816	73974	43606	1.496	1.500
Target Compounds						
11) L3 AR-1232-1	4.777	4.059	1704286	772522	1114.192	1111.331
12) L3 AR-1232-2	5.351	4.872	1175056	470728	1490.655	707.597m#
13) L3 AR-1232-3	5.663	5.060	1041646	244358	717.398m	719.059
14) L3 AR-1232-4	5.832	5.156	518230	206759	721.676	652.674
15) L3 AR-1232-5	5.933	5.337	371572	199331	756.773	572.888

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051921\
Data File : P0077983.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 May 2021 11:47
Operator : DD\AJ
Sample : M2368-01DL 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-33184-33186DL


Manual Integrations
APPROVED

Ankita
5/20/2021 2:05:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 12:06:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

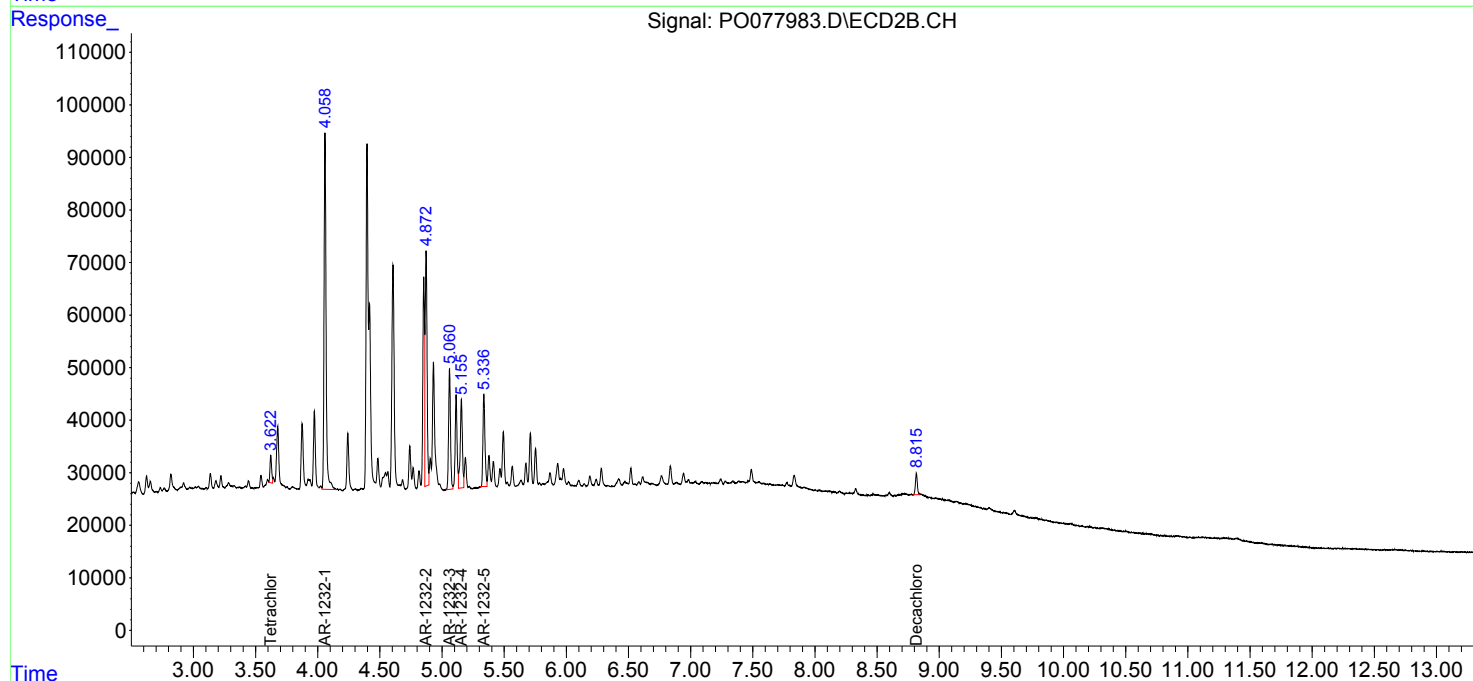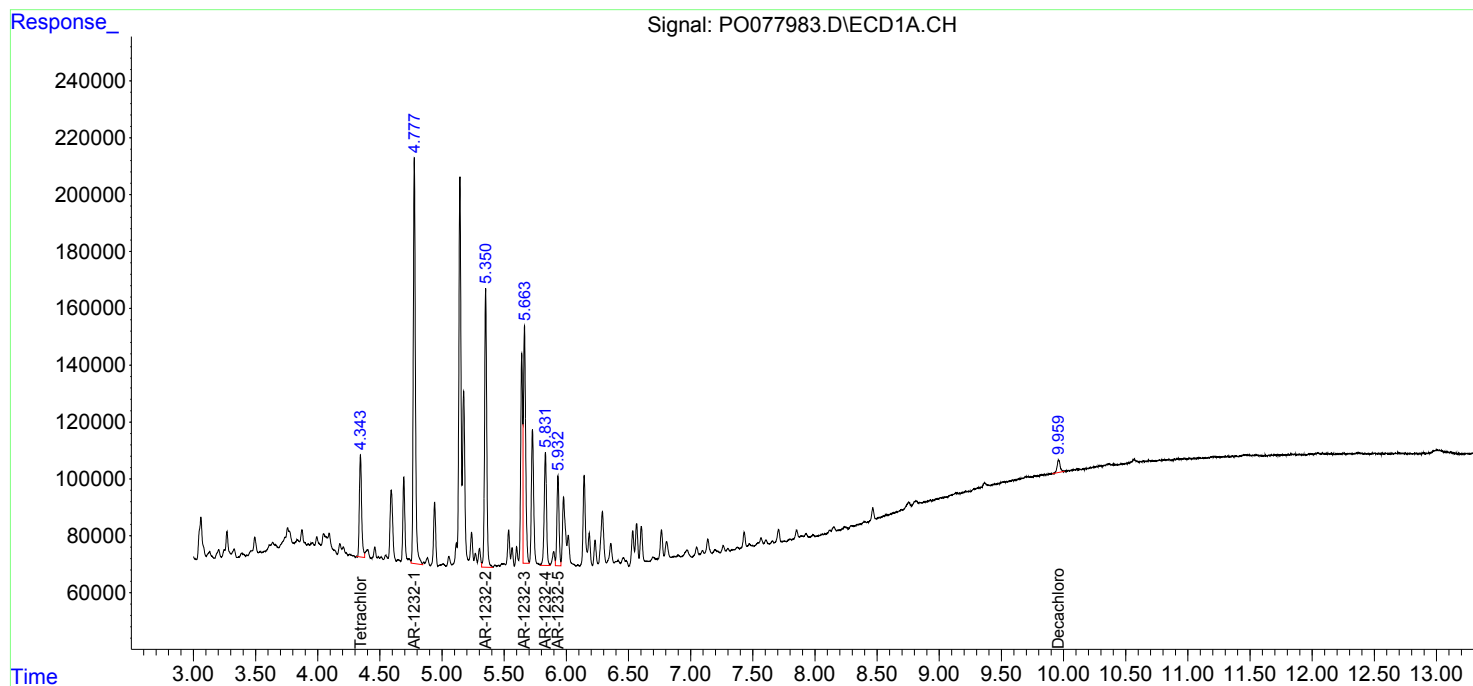

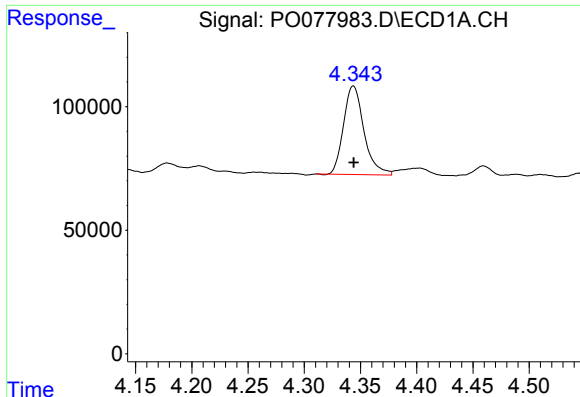


#1 Tetrachloro-m-xylene

R.T.: 4.344 min
Delta R.T.: 0.000 min
Response: 452512
Conc: 6.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-33184-33186DL


Manual Integrations
APPROVED

Ankita
5/20/2021 2:05:55 PM

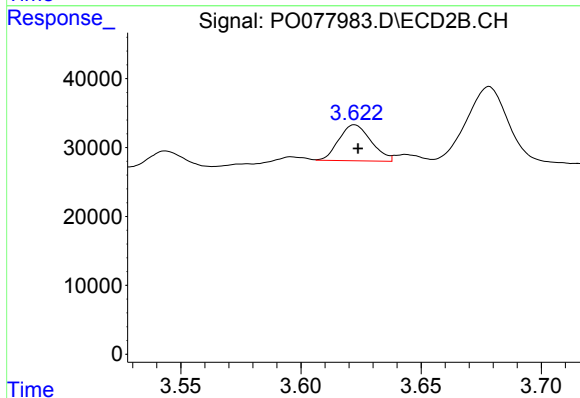


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.001 min
Response: 48705
Conc: 1.61 ng/ml

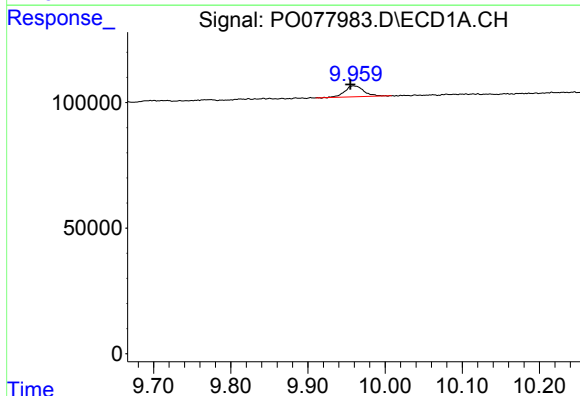


#2 Decachlorobiphenyl

R.T.: 9.959 min
Delta R.T.: 0.004 min
Response: 73974
Conc: 1.50 ng/ml

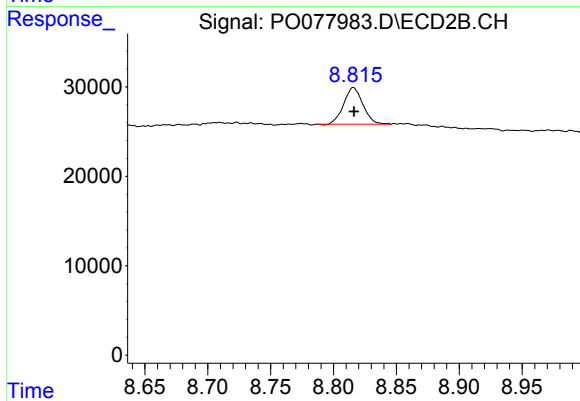

#2 Decachlorobiphenyl

R.T.: 8.816 min
Delta R.T.: 0.000 min
Response: 43606
Conc: 1.50 ng/ml

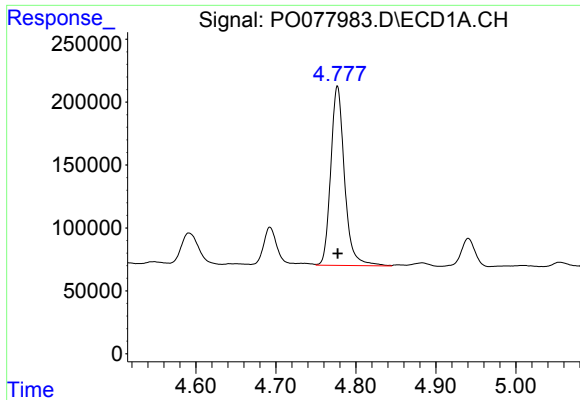


#11 AR-1232-1

R.T.: 4.777 min
Delta R.T.: 0.000 min
Response: 1704286
Conc: 1114.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-33184-33186DL


Manual Integrations
APPROVED

Ankita
5/20/2021 2:05:55 PM

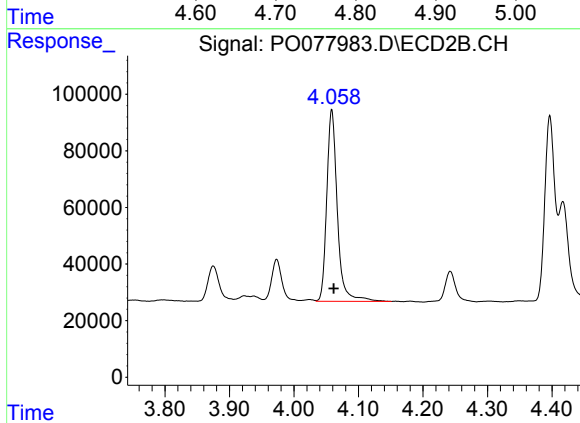


#11 AR-1232-1

R.T.: 4.059 min
Delta R.T.: -0.003 min
Response: 772522
Conc: 1111.33 ng/ml

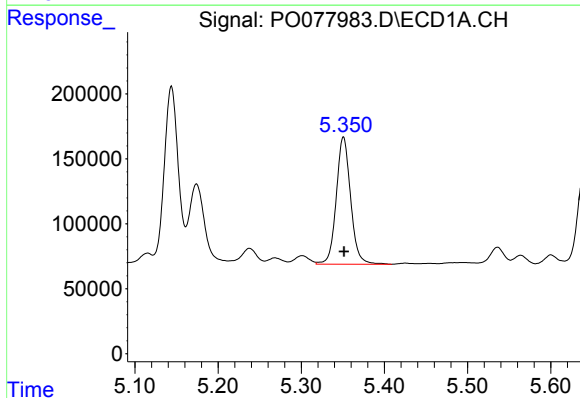


#12 AR-1232-2

R.T.: 5.351 min
Delta R.T.: 0.000 min
Response: 1175056
Conc: 1490.65 ng/ml

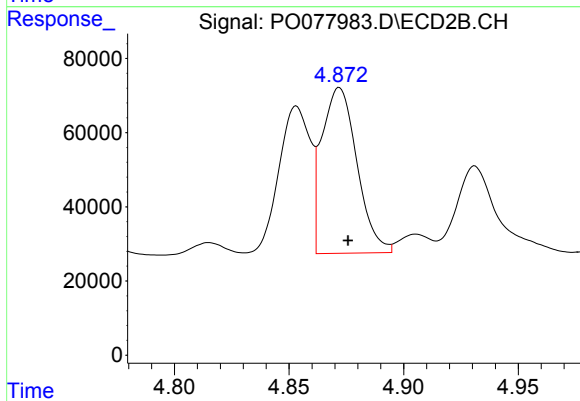

#12 AR-1232-2

R.T.: 4.872 min
Delta R.T.: -0.004 min
Response: 470728
Conc: 707.60 ng/ml m

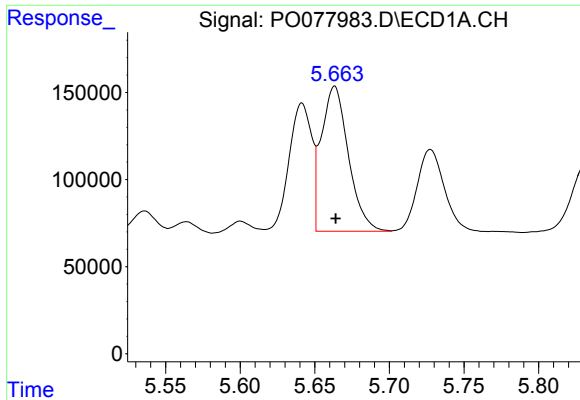


#13 AR-1232-3

R.T.: 5.663 min
Delta R.T.: 0.000 min
Response: 1041646
Conc: 717.40 ng/ml m

Instrument :
ECD_O
ClientSampleId :
COMP-33184-33186DL


Manual Integrations
APPROVED

Ankita
5/20/2021 2:05:55 PM

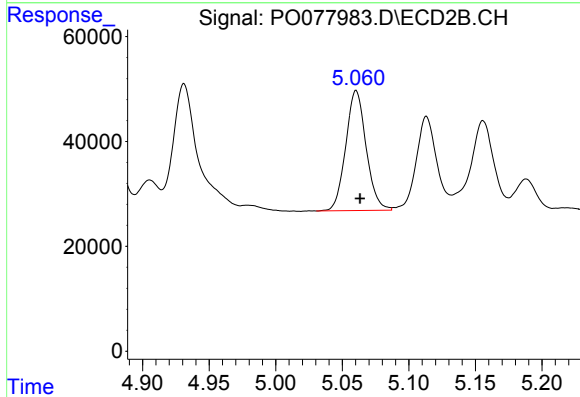


#13 AR-1232-3

R.T.: 5.060 min
Delta R.T.: -0.003 min
Response: 244358
Conc: 719.06 ng/ml

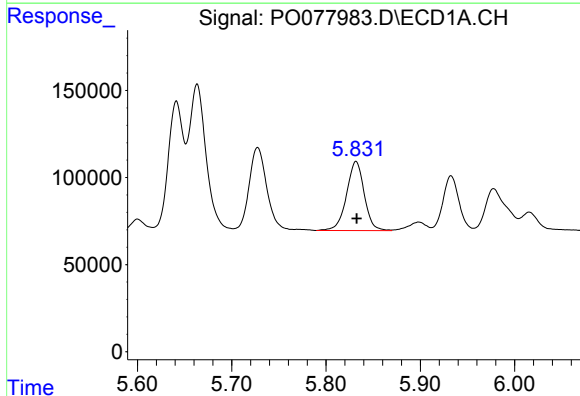


#14 AR-1232-4

R.T.: 5.832 min
Delta R.T.: 0.000 min
Response: 518230
Conc: 721.68 ng/ml

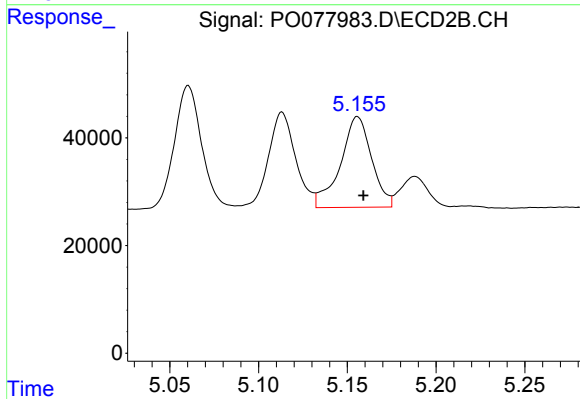

#14 AR-1232-4

R.T.: 5.156 min
Delta R.T.: -0.003 min
Response: 206759
Conc: 652.67 ng/ml

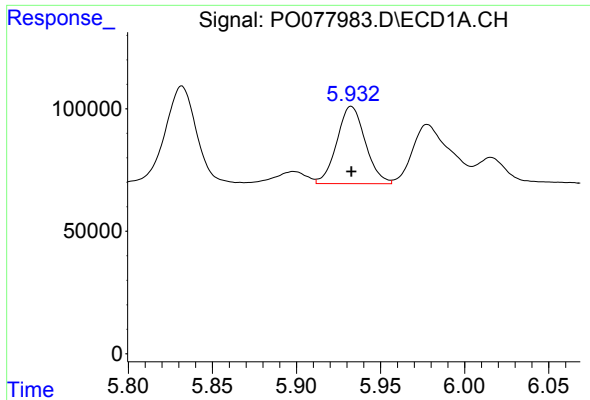


#15 AR-1232-5

R.T.: 5.933 min
Delta R.T.: 0.000 min
Response: 371572
Conc: 756.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-33184-33186DL

Manual Integrations
APPROVED

Ankita
5/20/2021 2:05:55 PM

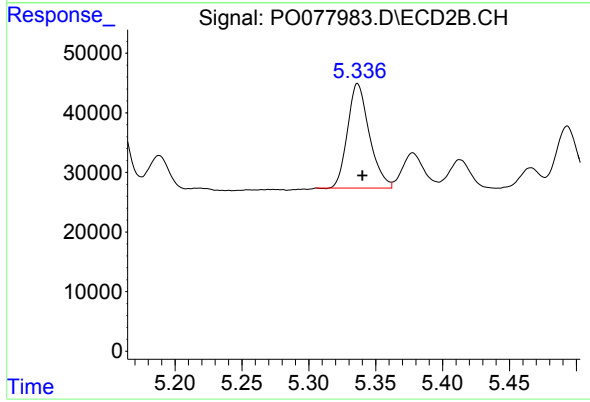

#15 AR-1232-5

R.T.: 5.337 min
Delta R.T.: -0.003 min
Response: 199331
Conc: 572.89 ng/ml