Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051921\
Data File : PO077997.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 May 2021 16:05
Operator : DD\AJ
Sample : PB136515BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB136515BL

Manual Integrations APPROVED
Ankita
5/20/2021 2:06:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 02:28:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
	System Monitoring Compounds						
1)	SA Tetrachlo...	4.344	3.623	1449156	715125	19.608m	23.667m
2)	SA Decachlor...	9.959	8.816	1036442	614080	20.963	21.119
	Target Compounds						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051921\
Data File : PO077997.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 May 2021 16:05
Operator : DD\AJ
Sample : PB136515BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB136515BL

Manual Integrations APPROVED
Ankita
5/20/2021 2:06:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 02:28:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

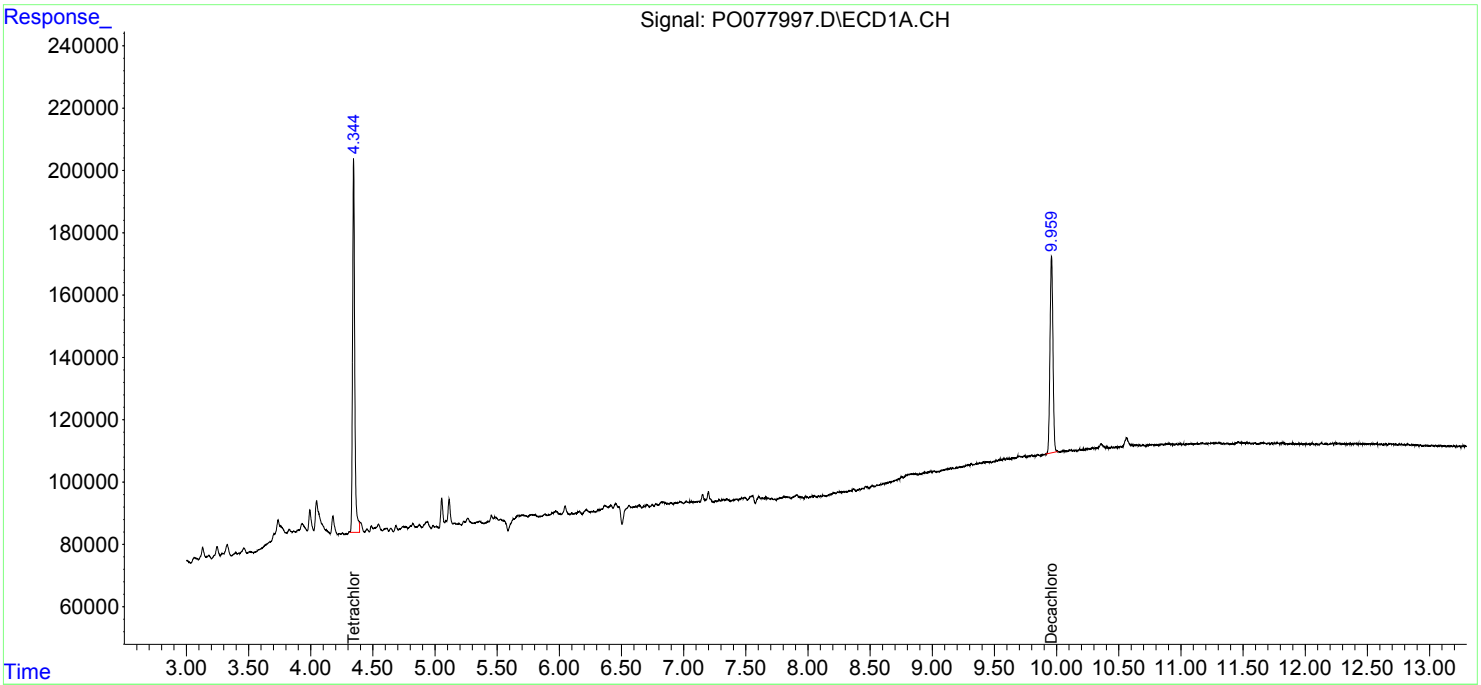

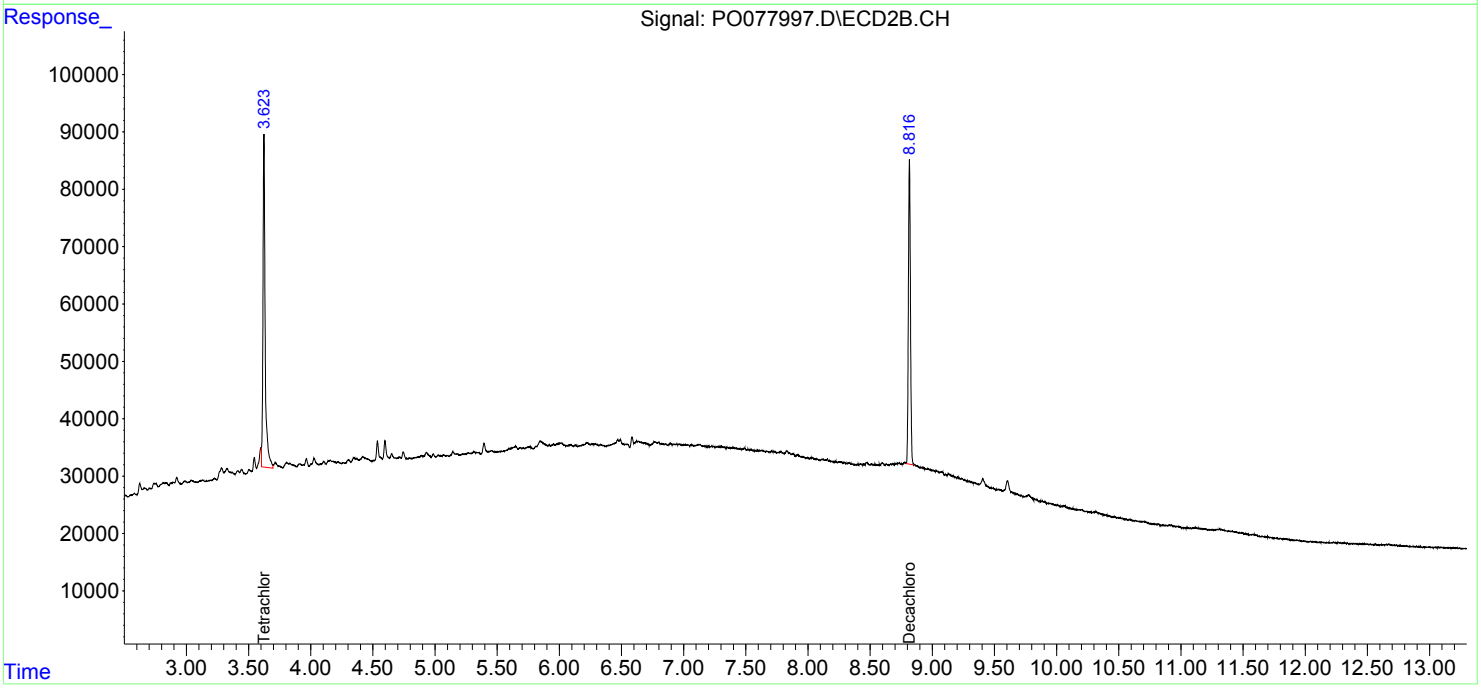

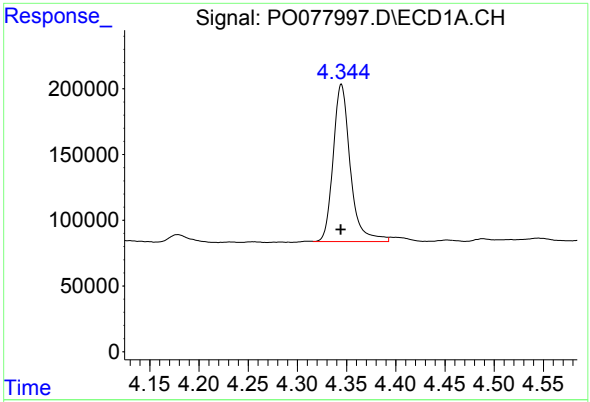

#1 Tetrachloro-m-xylene

R.T.: 4.344 min
Delta R.T.: 0.000 min
Response: 1449156
Conc: 19.61 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PB136515BL

Manual Integrations APPROVED
Ankita
5/20/2021 2:06:16 PM

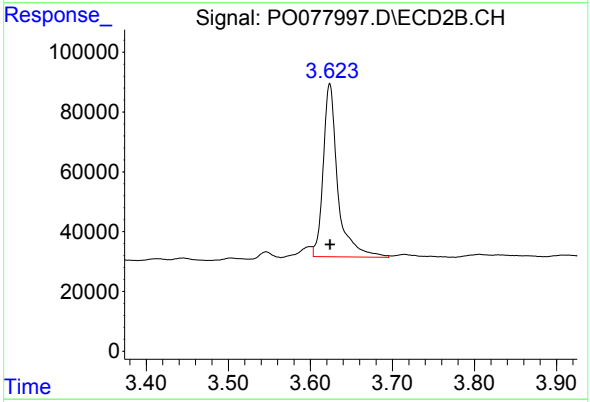

#1 Tetrachloro-m-xylene

R.T.: 3.623 min
Delta R.T.: 0.000 min
Response: 715125
Conc: 23.67 ng/ml m

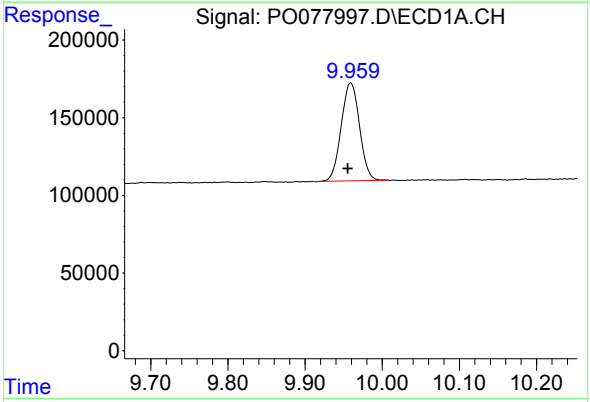

#2 Decachlorobiphenyl

R.T.: 9.959 min
Delta R.T.: 0.004 min
Response: 1036442
Conc: 20.96 ng/ml

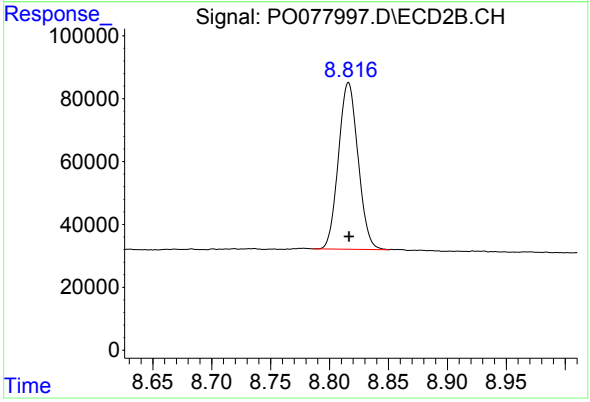

#2 Decachlorobiphenyl

R.T.: 8.816 min
Delta R.T.: 0.000 min
Response: 614080
Conc: 21.12 ng/ml