

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0051921\
 Data File : P0078003.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 May 2021 17:48
 Operator : DD\AJ
 Sample : M2437-05
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 TP-2

Manual Integrations
 APPROVED

Ankita
 5/20/2021 2:06:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 02:30:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.343	3.623	1653655	716842	22.375m	23.724m
2) SA Decachlor...	9.957	8.816	1396770	798509	28.251	27.461
Target Compounds						
31) L7 AR-1260-1	7.299	6.416	179132	81793	63.833m	51.049m
32) L7 AR-1260-2	7.565	6.614	221630	97461	65.881m	50.483m
33) L7 AR-1260-3	7.924	6.762	144811	58231	59.349m	31.740m#
34) L7 AR-1260-4	8.146	7.240	170794	45478	63.759m	30.169 #
35) L7 AR-1260-5	8.464	7.489	184525	133520	35.929m	38.288m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051921\
Data File : P0078003.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 May 2021 17:48
Operator : DD\AJ
Sample : M2437-05
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
Client Sampled :
TP-2


Manual Integrations
APPROVED

Ankita
5/20/2021 2:06:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 02:30:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

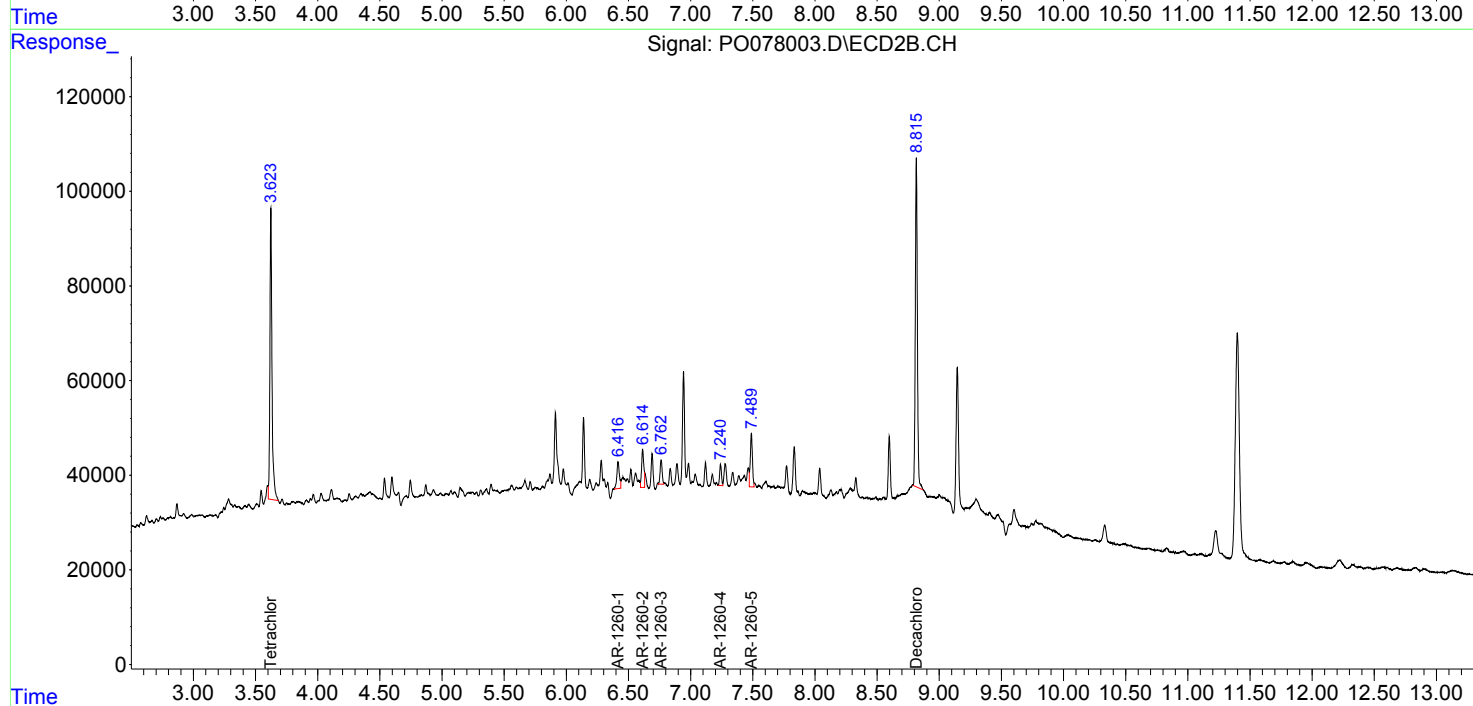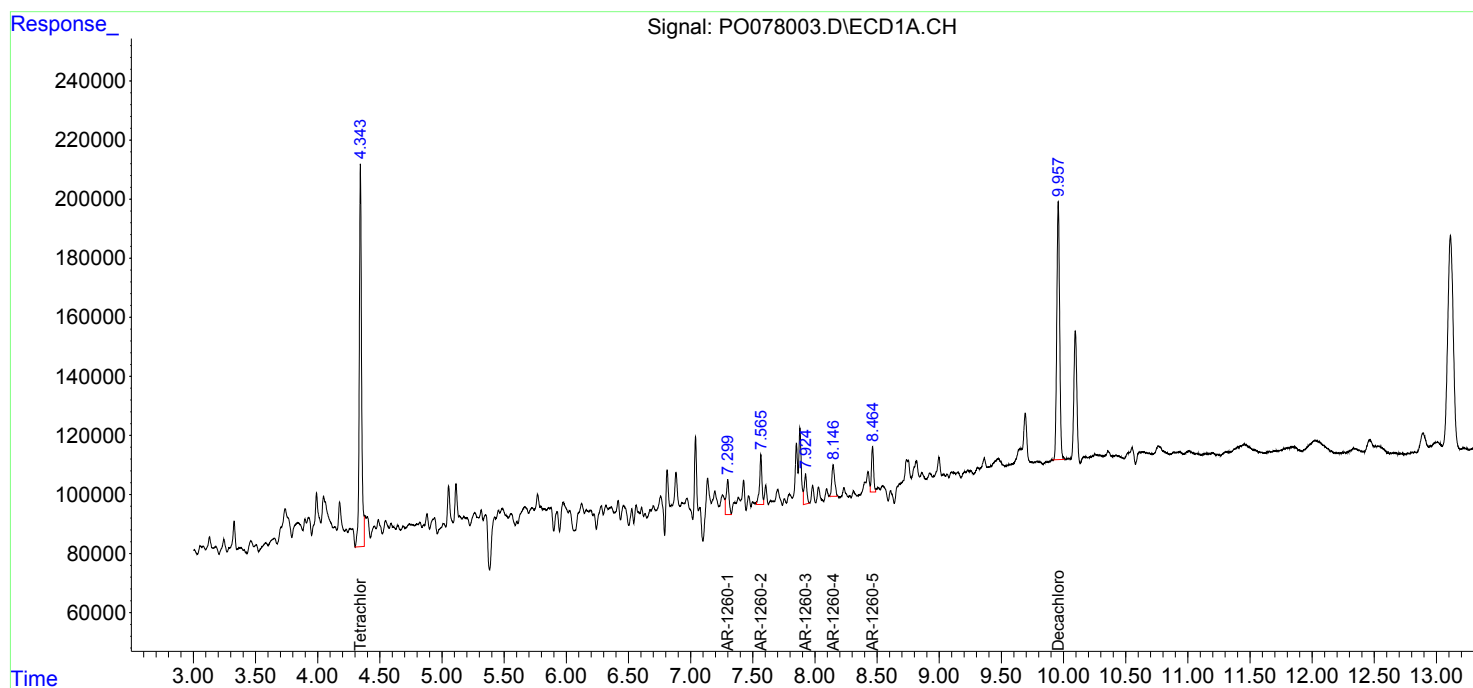

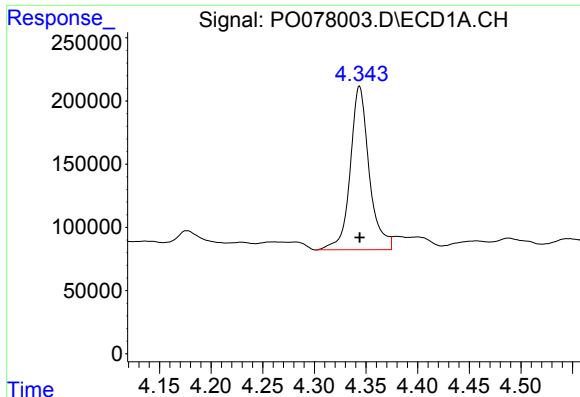


#1 Tetrachloro-m-xylene

R.T.: 4.343 min
Delta R.T.: 0.000 min
Response: 1653655
Conc: 22.37 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
5/20/2021 2:06:23 PM

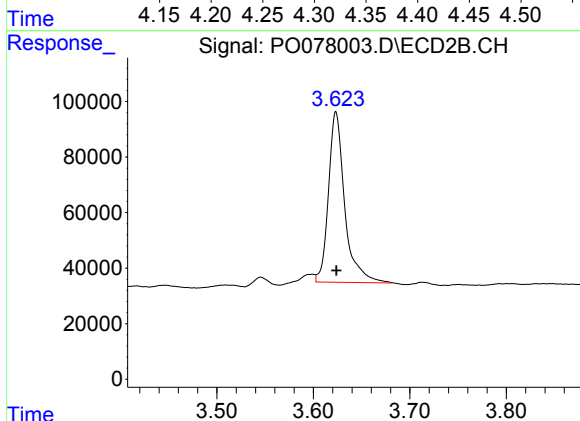


#1 Tetrachloro-m-xylene

R.T.: 3.623 min
Delta R.T.: 0.000 min
Response: 716842
Conc: 23.72 ng/ml m

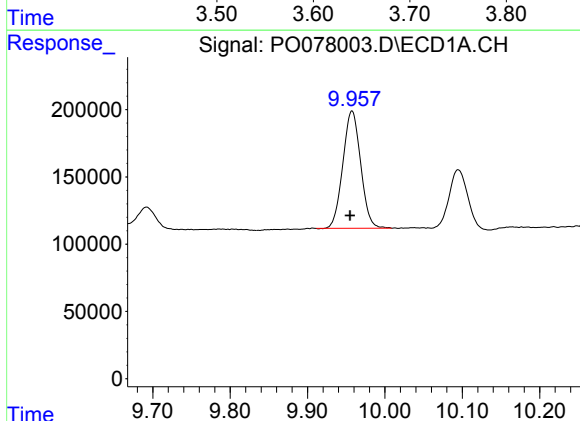


#2 Decachlorobiphenyl

R.T.: 9.957 min
Delta R.T.: 0.002 min
Response: 1396770
Conc: 28.25 ng/ml

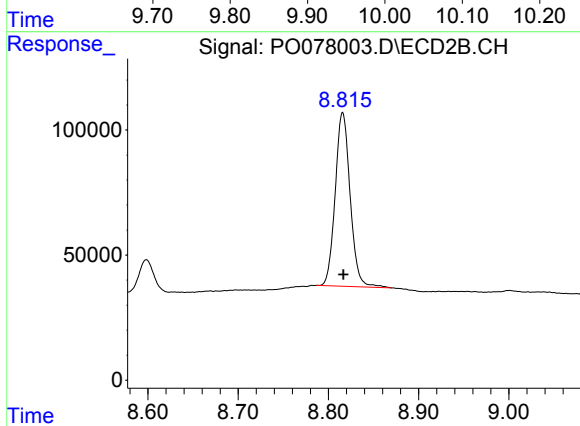

#2 Decachlorobiphenyl

R.T.: 8.816 min
Delta R.T.: 0.000 min
Response: 798509
Conc: 27.46 ng/ml

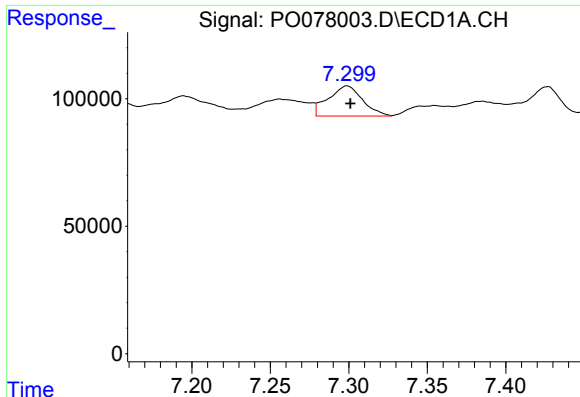


#31 AR-1260-1

R.T.: 7.299 min
Delta R.T.: -0.002 min
Response: 179132
Conc: 63.83 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
5/20/2021 2:06:23 PM

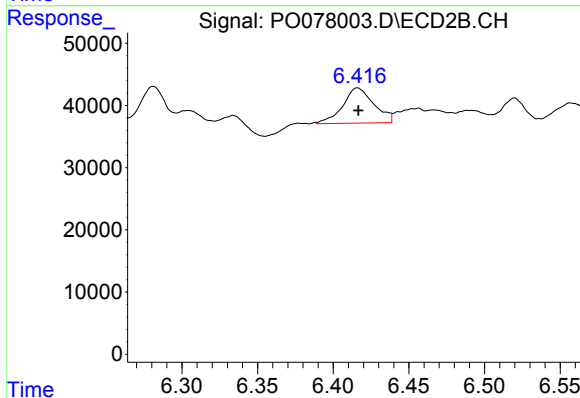


#31 AR-1260-1

R.T.: 6.416 min
Delta R.T.: 0.000 min
Response: 81793
Conc: 51.05 ng/ml m

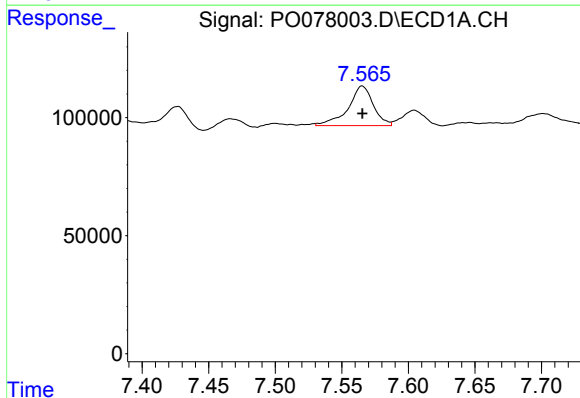


#32 AR-1260-2

R.T.: 7.565 min
Delta R.T.: 0.000 min
Response: 221630
Conc: 65.88 ng/ml m

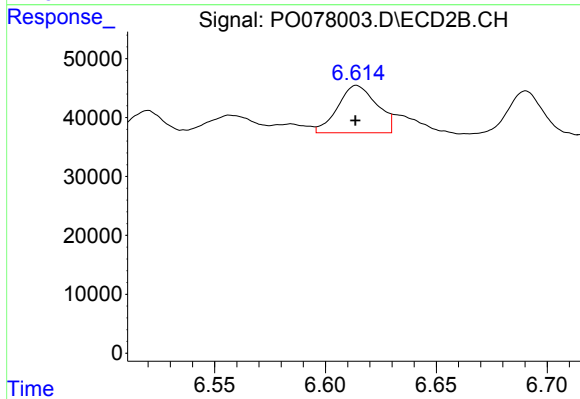

#32 AR-1260-2

R.T.: 6.614 min
Delta R.T.: 0.000 min
Response: 97461
Conc: 50.48 ng/ml m

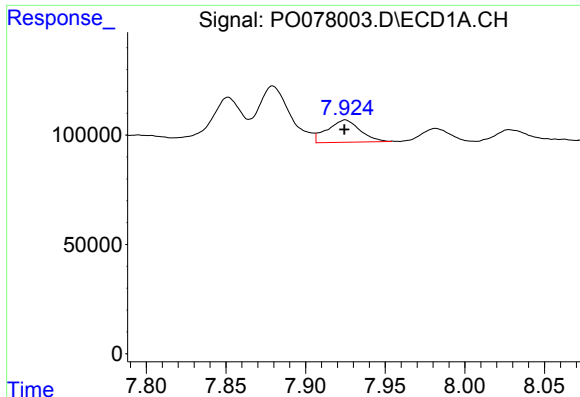


#33 AR-1260-3

R.T.: 7.924 min
Delta R.T.: 0.000 min
Response: 144811
Conc: 59.35 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
5/20/2021 2:06:23 PM

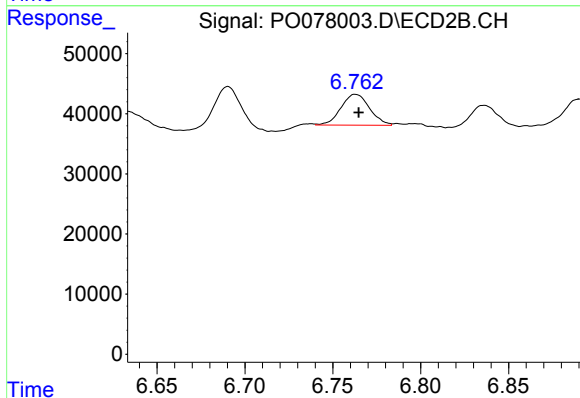


#33 AR-1260-3

R.T.: 6.762 min
Delta R.T.: -0.003 min
Response: 58231
Conc: 31.74 ng/ml m

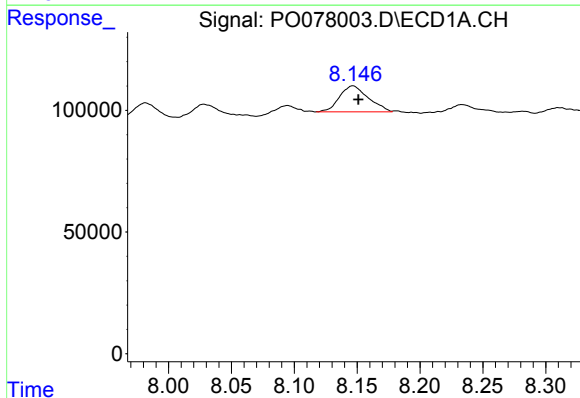


#34 AR-1260-4

R.T.: 8.146 min
Delta R.T.: -0.004 min
Response: 170794
Conc: 63.76 ng/ml m

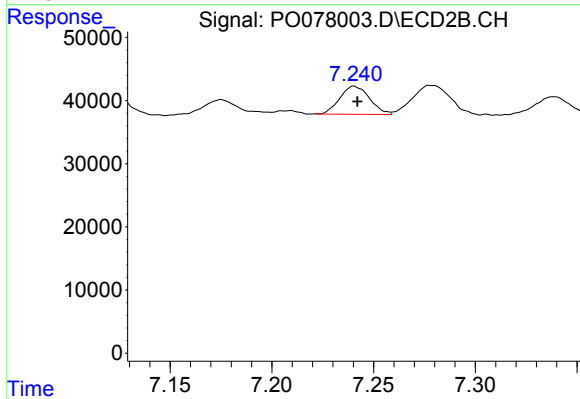

#34 AR-1260-4

R.T.: 7.240 min
Delta R.T.: -0.002 min
Response: 45478
Conc: 30.17 ng/ml

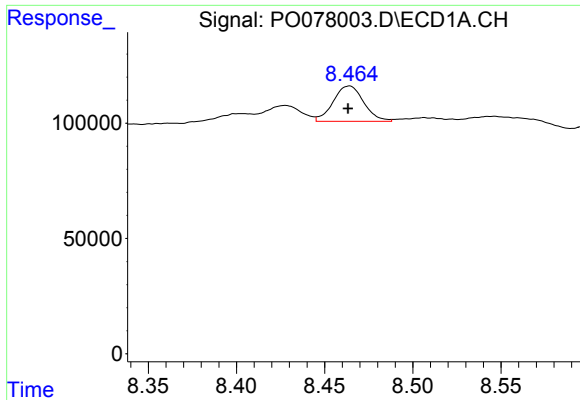


#35 AR-1260-5

R.T.: 8.464 min
Delta R.T.: 0.000 min
Response: 184525
Conc: 35.93 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-2

Manual Integrations
APPROVED

Ankita
5/20/2021 2:06:23 PM

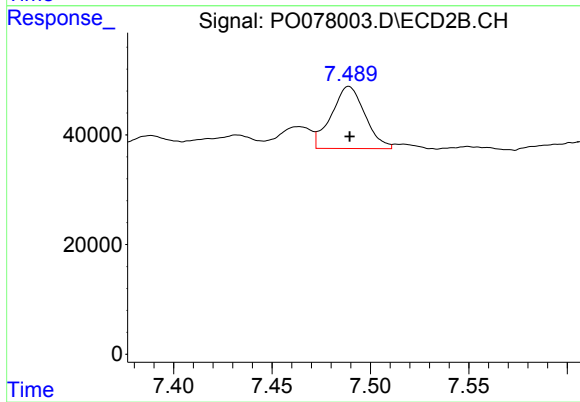

#35 AR-1260-5

R.T.: 7.489 min
Delta R.T.: 0.000 min
Response: 133520
Conc: 38.29 ng/ml m