

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051922\
 Data File : P0086213.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 May 2022 21:41
 Operator : YP\AJ
 Sample : N2902-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WASTE-WATER-5/16/22

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 02:54:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 19 09:06:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.480	3.678	1525775	575398	15.016	13.210
2) SA Decachlor...	10.335	8.737	287759	161571	5.300	4.643

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051922\
Data File : P0086213.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 May 2022 21:41
Operator : YP\AJ
Sample : N2902-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
WASTE-WATER-5/16/22

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 02:54:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 19 09:06:34 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

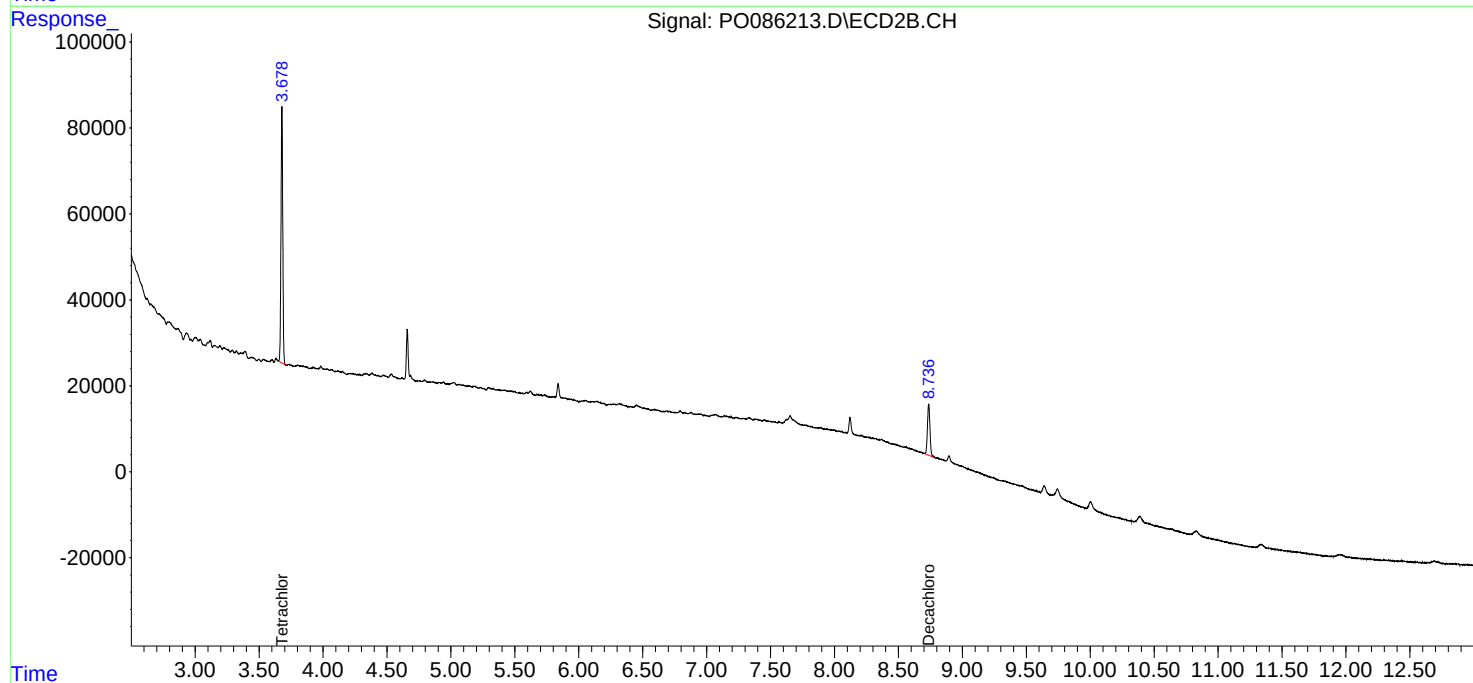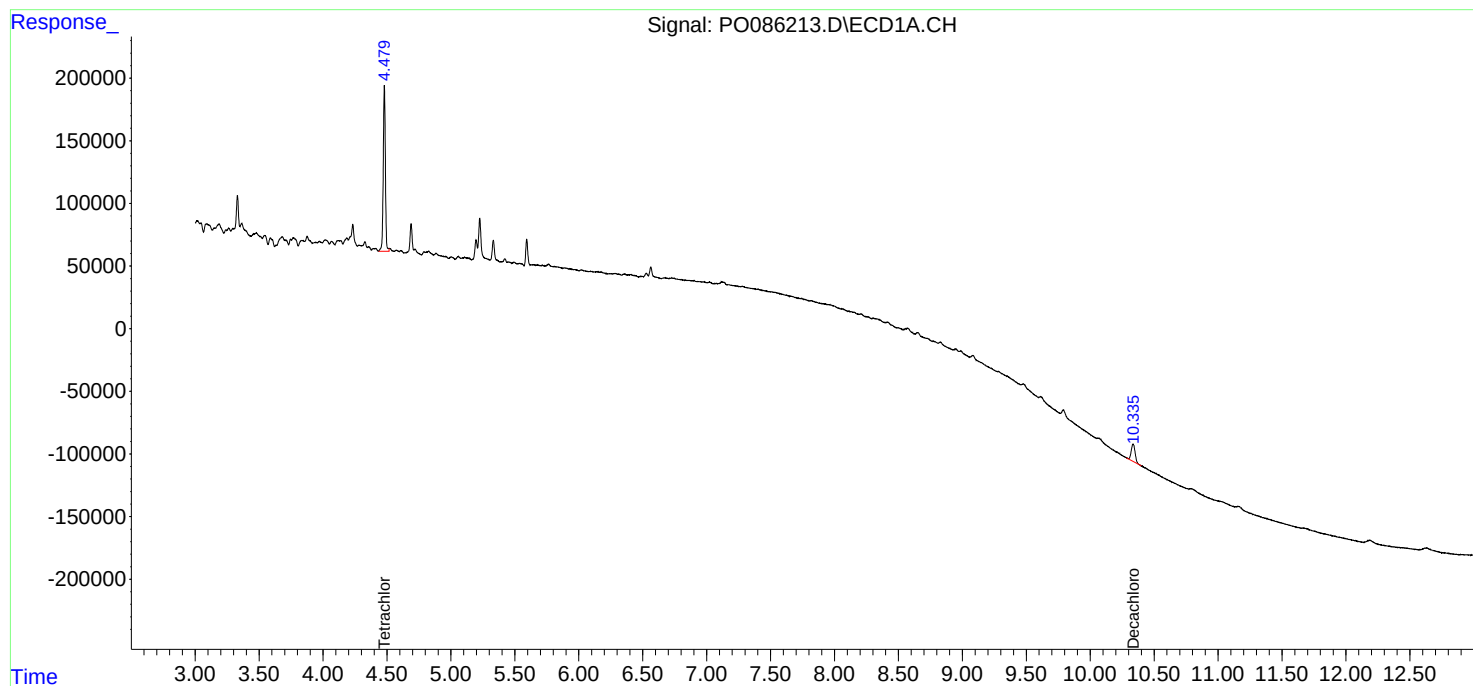


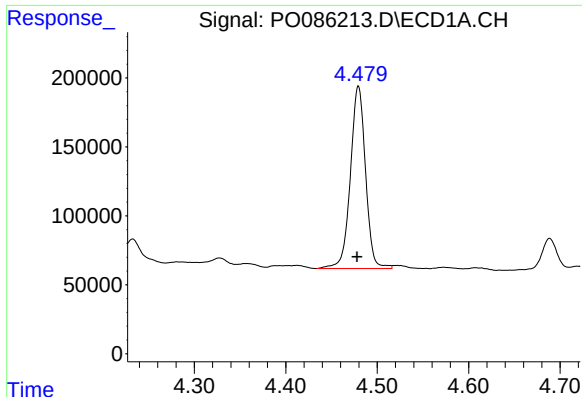

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: 0.002 min
Response: 1525775
Conc: 15.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
WASTE-WATER-5/16/22

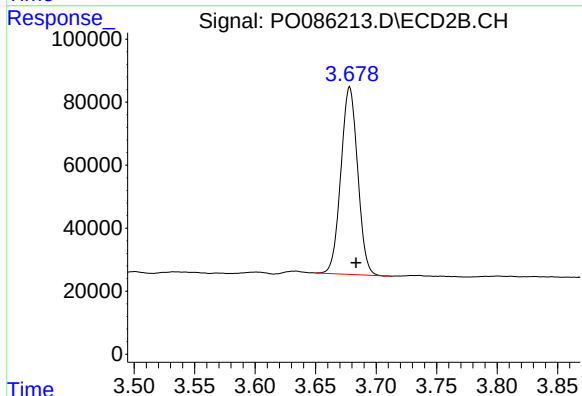


#1 Tetrachloro-m-xylene

R.T.: 3.678 min
Delta R.T.: -0.005 min
Response: 575398
Conc: 13.21 ng/ml

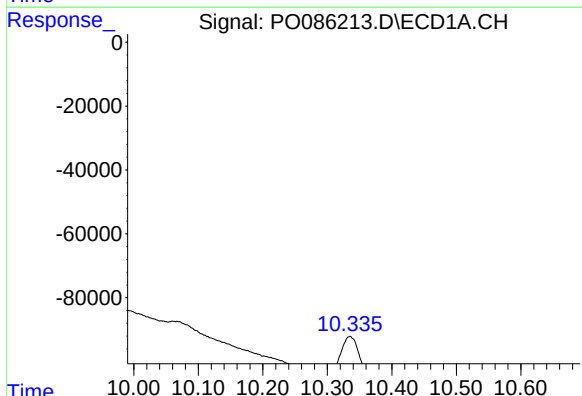

#2 Decachlorobiphenyl

R.T.: 10.335 min
Delta R.T.: 0.010 min
Response: 287759
Conc: 5.30 ng/ml

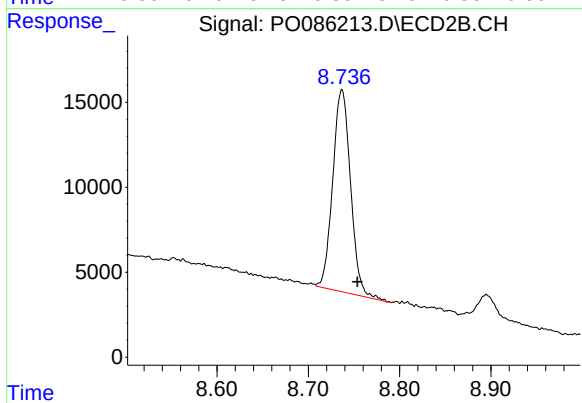

#2 Decachlorobiphenyl

R.T.: 8.737 min
Delta R.T.: -0.017 min
Response: 161571
Conc: 4.64 ng/ml