

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051922\
 Data File : P0086243.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 May 2022 8:29
 Operator : YP\AJ
 Sample : N2912-01
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 3/4-BLEND-RCA

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/23/2022
 Supervised By :Ankita Jodhani 05/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 09:18:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 19 09:06:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.479	3.677	2338206	932389	23.012	21.406
2) SA Decachlor...	10.335	8.735	1167021	739736	21.492m	21.256m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051922\
Data File : P0086243.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 May 2022 8:29
Operator : YP\AJ
Sample : N2912-01
Misc :
ALS Vial : 42 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
3/4-BLEND-RCA


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/23/2022
Supervised By :Ankita Jodhani 05/23/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 09:18:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 19 09:06:34 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

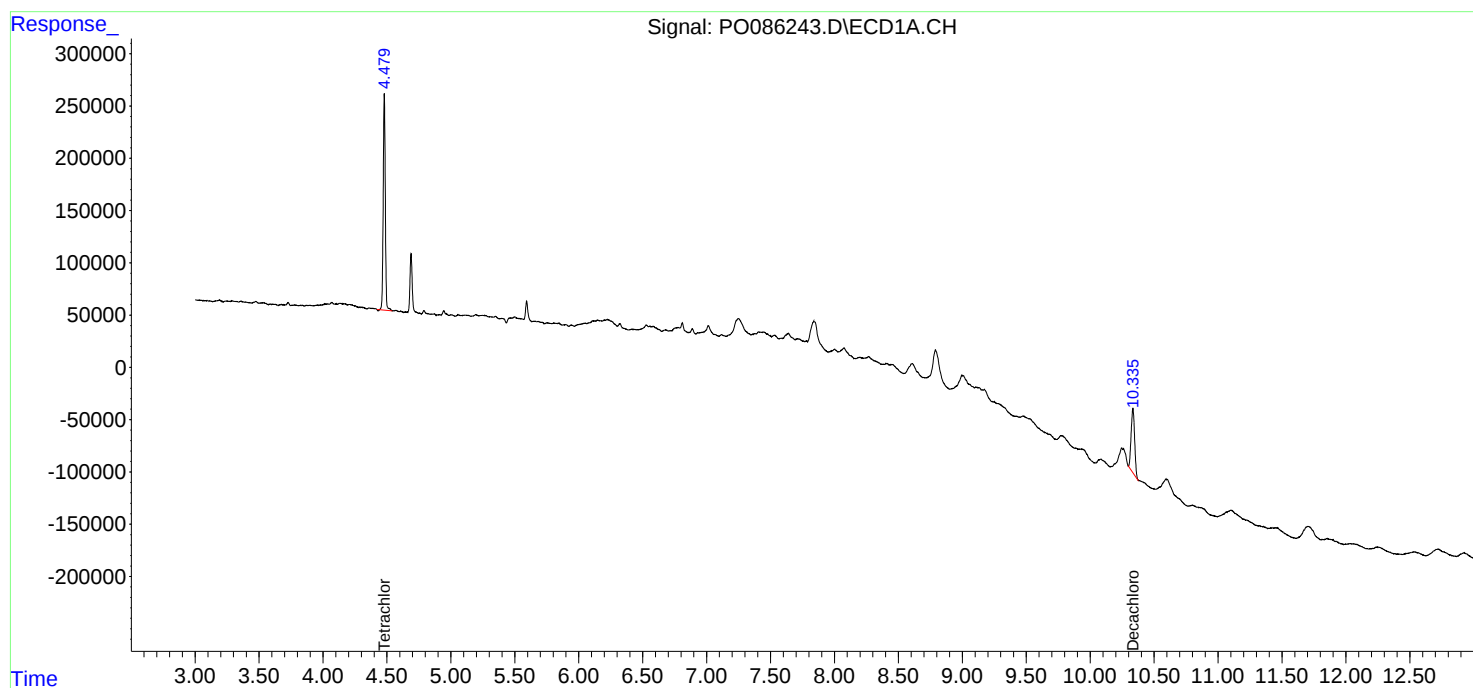

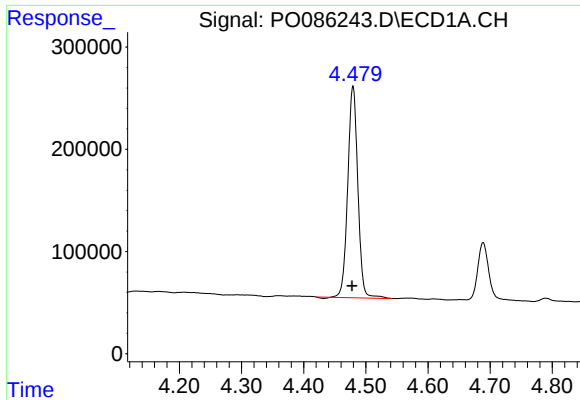


#1 Tetrachloro-m-xylene

R.T.: 4.479 min
Delta R.T.: 0.001 min
Response: 2338206
Conc: 23.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
3/4-BLEND-RCA


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/23/2022
Supervised By :Ankita Jodhani 05/23/2022

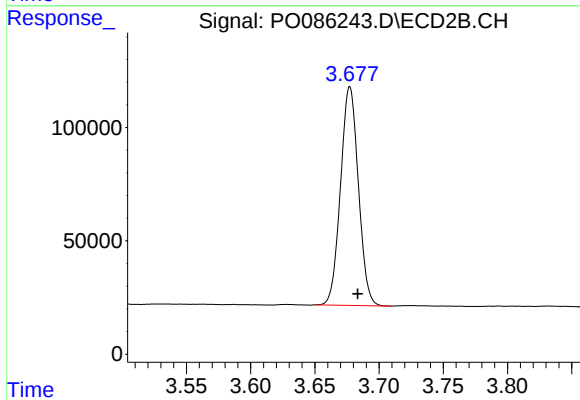


#1 Tetrachloro-m-xylene

R.T.: 3.677 min
Delta R.T.: -0.006 min
Response: 932389
Conc: 21.41 ng/ml

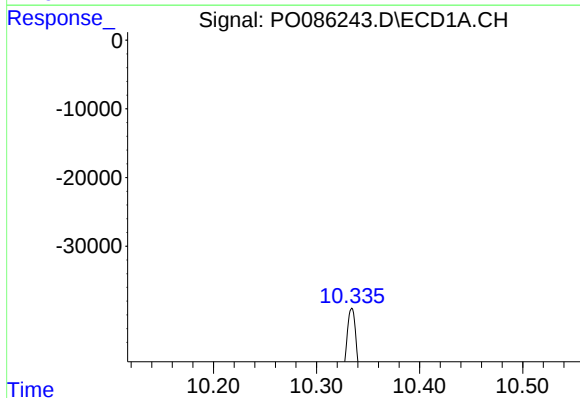

#2 Decachlorobiphenyl

R.T.: 10.335 min
Delta R.T.: 0.010 min
Response: 1167021
Conc: 21.49 ng/ml m

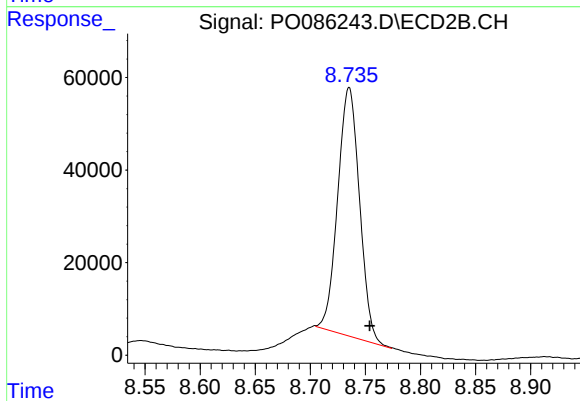

#2 Decachlorobiphenyl

R.T.: 8.735 min
Delta R.T.: -0.019 min
Response: 739736
Conc: 21.26 ng/ml m