

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051923\
 Data File : P0095207.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2023 20:24
 Operator : YP/AJ
 Sample : 02830-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SEMI-ANNUAL-CONDENSATE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/20/2023
 Supervised By :Ankita Jodhani 05/22/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 22:10:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 19 06:20:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.493	3.656	1638604	19407119	0.562m	17.091 #
2) SA Decachlor...	10.548	8.705	31537811	24015310	13.591	24.763 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051923\
Data File : PO095207.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2023 20:24
Operator : YP/AJ
Sample : 02830-01
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SEMI-ANNUAL-CONDENSATE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/20/2023
Supervised By :Ankita Jodhani 05/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 22:10:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051823.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 19 06:20:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

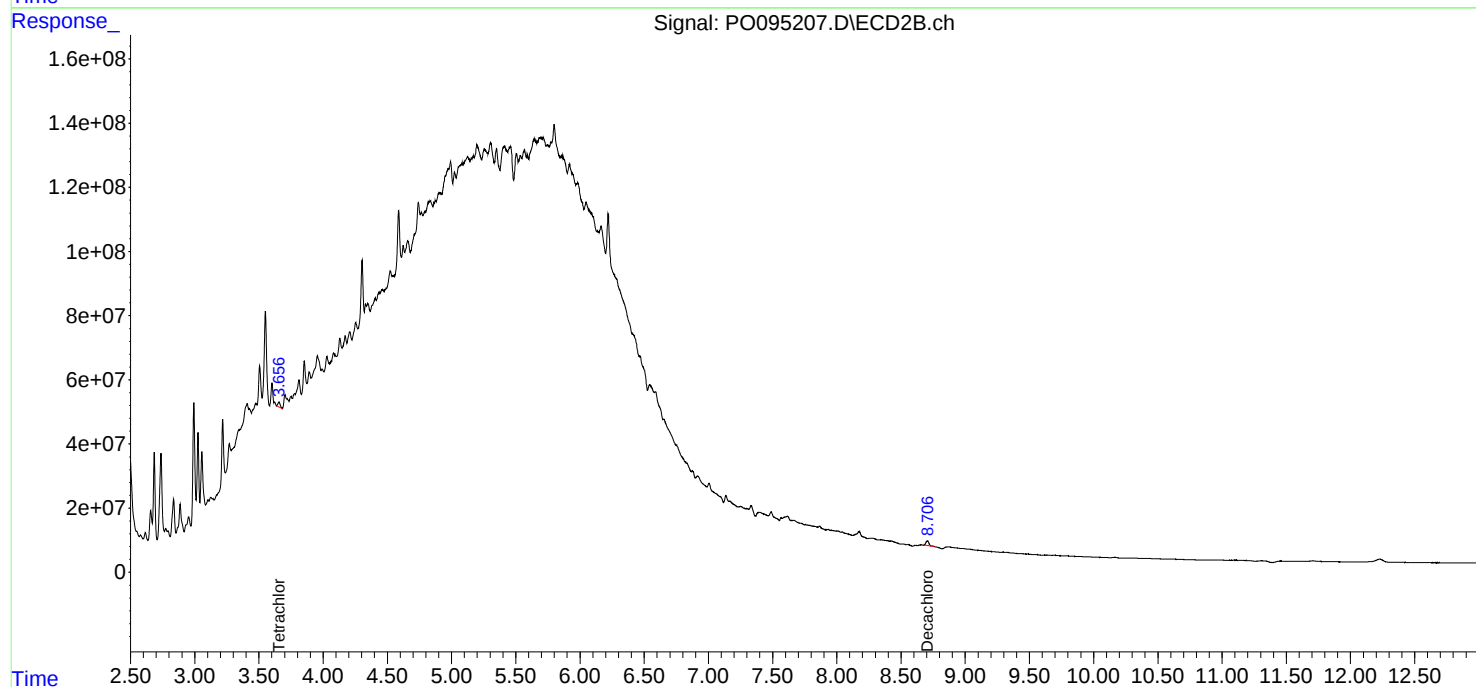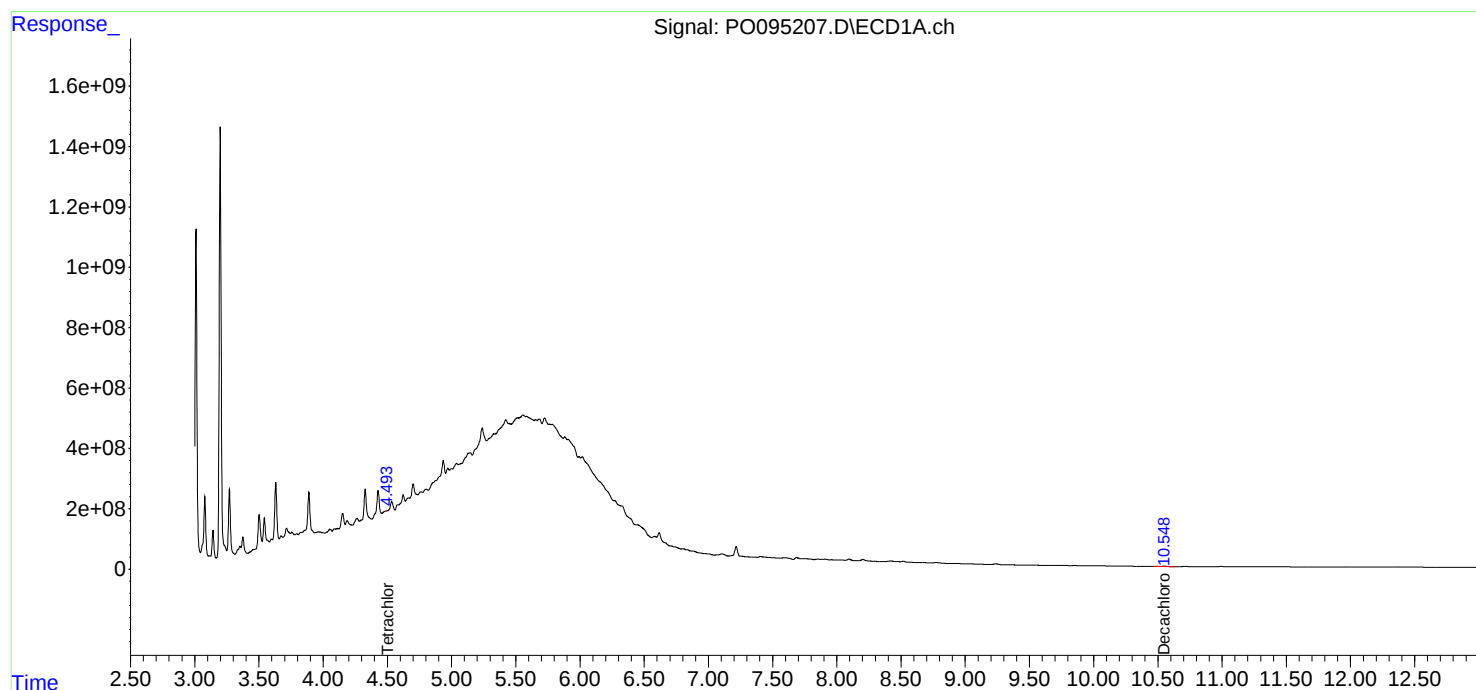

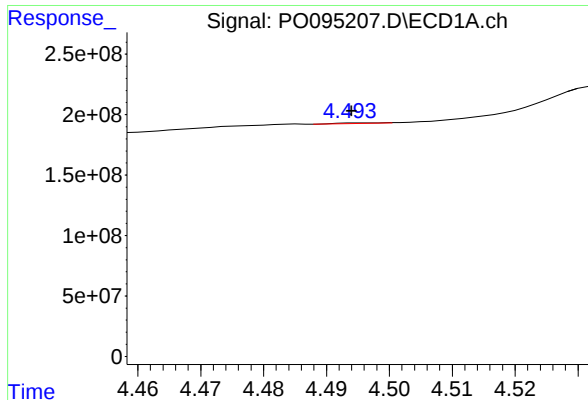


#1 Tetrachloro-m-xylene

R.T.: 4.493 min
Delta R.T.: 0.000 min
Response: 1638604
Conc: 0.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEMI-ANNUAL-CONDENSATE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/20/2023
Supervised By :Ankita Jodhani 05/22/2023

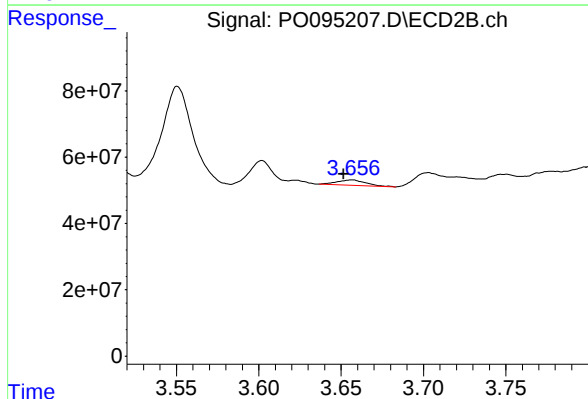


#1 Tetrachloro-m-xylene

R.T.: 3.656 min
Delta R.T.: 0.005 min
Response: 19407119
Conc: 17.09 ng/ml

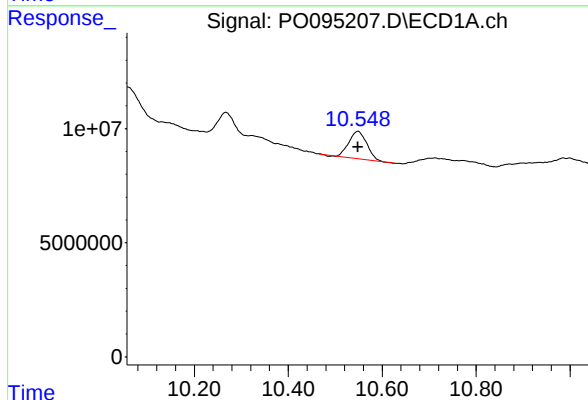

#2 Decachlorobiphenyl

R.T.: 10.548 min
Delta R.T.: 0.000 min
Response: 31537811
Conc: 13.59 ng/ml

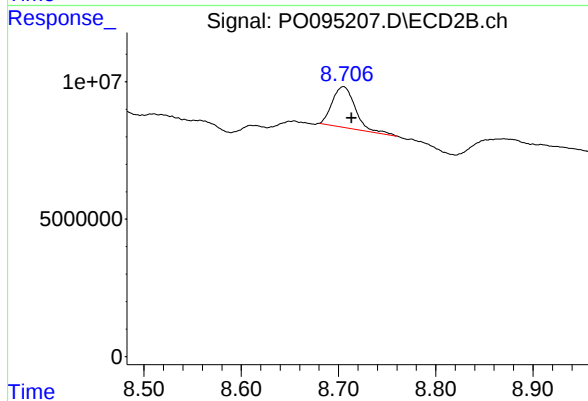

#2 Decachlorobiphenyl

R.T.: 8.705 min
Delta R.T.: -0.009 min
Response: 24015310
Conc: 24.76 ng/ml