

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052021\
 Data File : P0078056.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 May 2021 22:22
 Operator : DD\AJ
 Sample : M2466-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 02:35:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.342	3.622	1101974	493274	14.910	16.325
2) SA Decachlor...	9.957	8.820	775206	459857	15.680	15.815
Target Compounds						
29) L6 AR-1254-4	7.431	0.000	276928	0	101.973	N.D. #
30) L6 AR-1254-5	7.850	0.000	510748	0	174.646	N.D. #
31) L7 AR-1260-1	7.296	0.000	238029	0	84.821	N.D. #
32) L7 AR-1260-2	7.563	0.000	280908	0	83.502	N.D. #
35) L7 AR-1260-5	8.465	0.000	574452	0	111.851	N.D. #
37) L8 AR-1262-2	8.465	0.000	574452	0	95.431	N.D. #
39) L8 AR-1262-4	0.000	7.829	0	355130	N.D.	118.423 #
42) L9 AR-1268-2	0.000	7.829	0	355130	N.D.	85.832 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052021\
Data File : P0078056.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 May 2021 22:22
Operator : DD\AJ
Sample : M2466-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 02:35:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

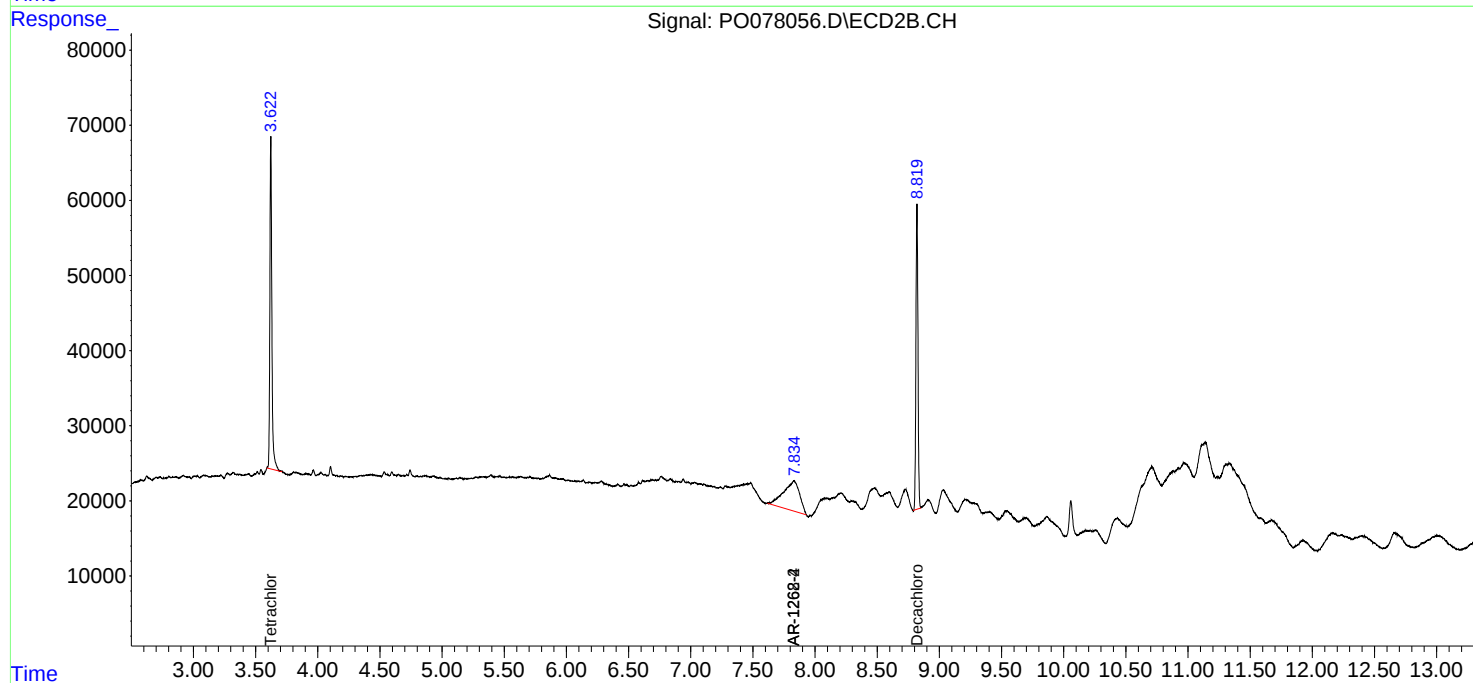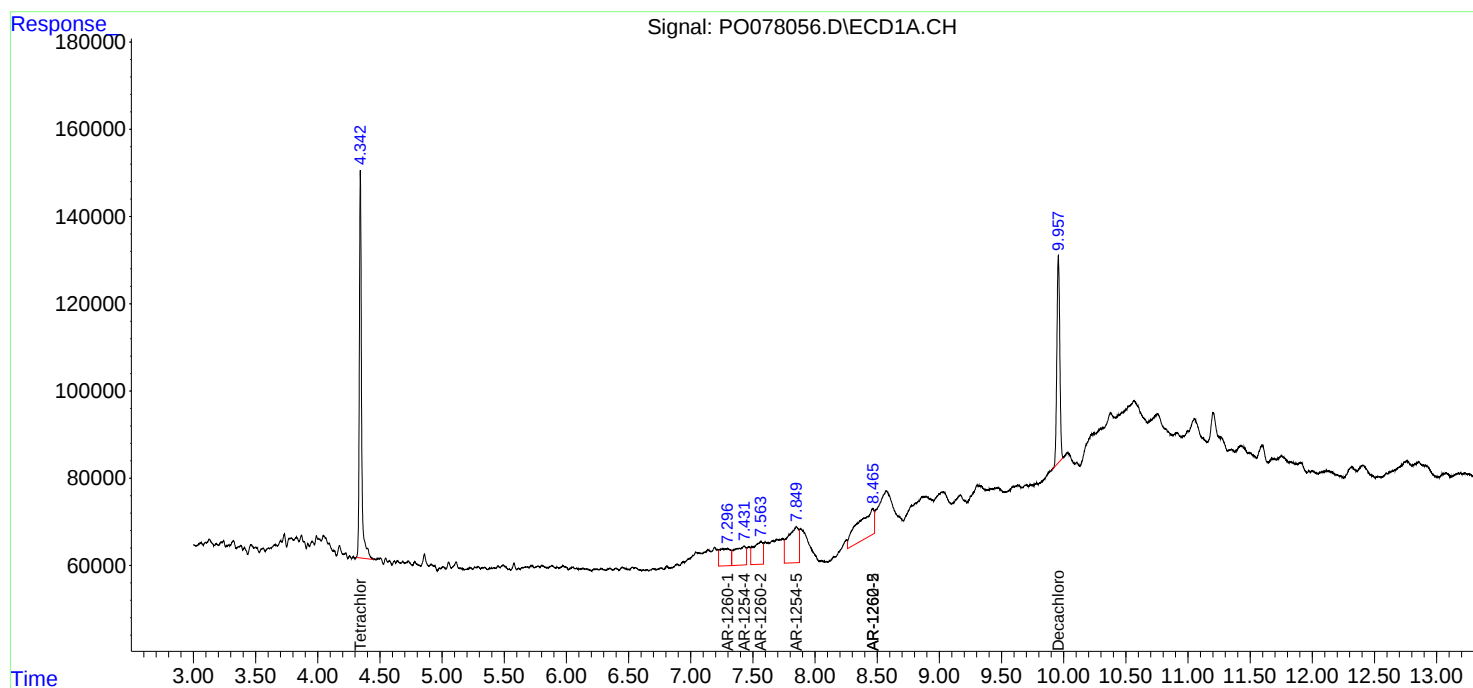


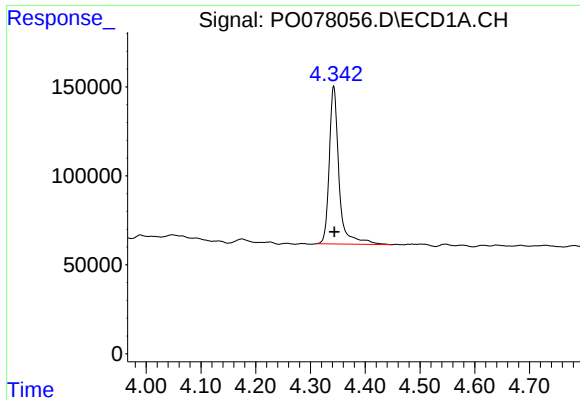

#1 Tetrachloro-m-xylene


R.T.: 4.342 min
Delta R.T.: -0.002 min
Response: 1101974
Conc: 14.91 ng/ml

Instrument :
ECD_O
ClientSampleId :

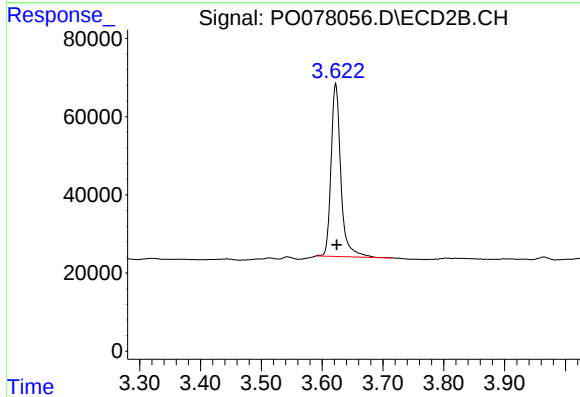


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.001 min
Response: 493274
Conc: 16.32 ng/ml

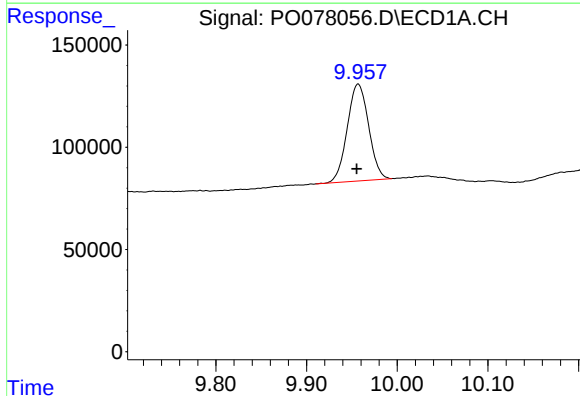


#2 Decachlorobiphenyl

R.T.: 9.957 min
Delta R.T.: 0.002 min
Response: 775206
Conc: 15.68 ng/ml

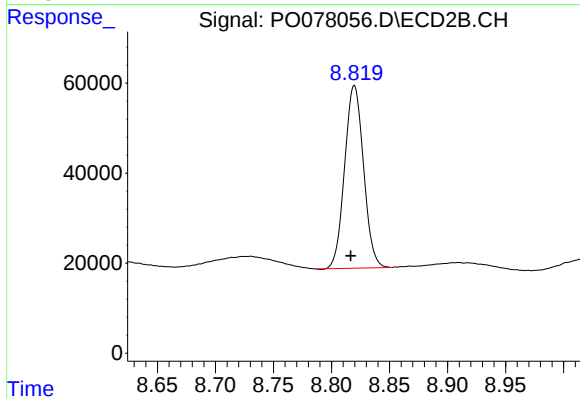

#2 Decachlorobiphenyl


R.T.: 8.820 min
Delta R.T.: 0.003 min
Response: 459857
Conc: 15.81 ng/ml

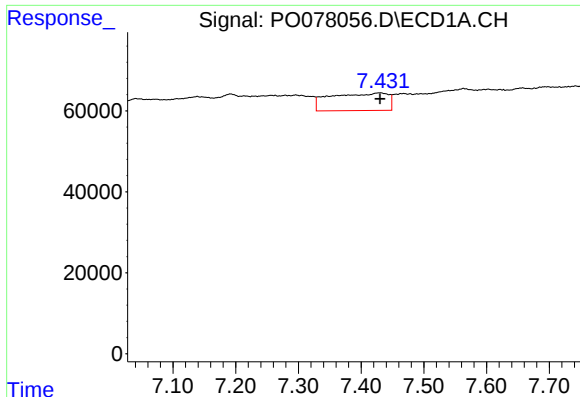

#29 AR-1254-4


R.T.: 7.431 min
Delta R.T.: 0.000 min
Response: 276928
Conc: 101.97 ng/ml

Instrument :
ECD_O
ClientSampleId :

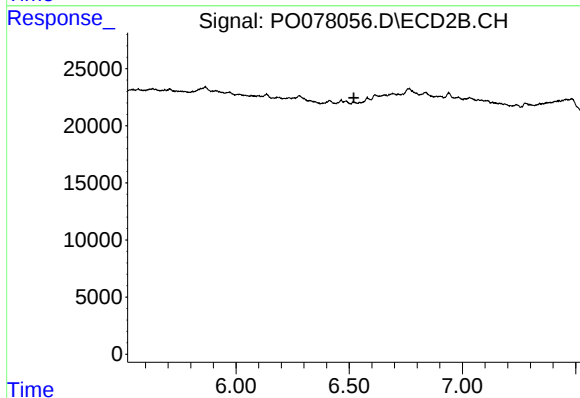


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.521 min
Response: 0
Conc: N.D.

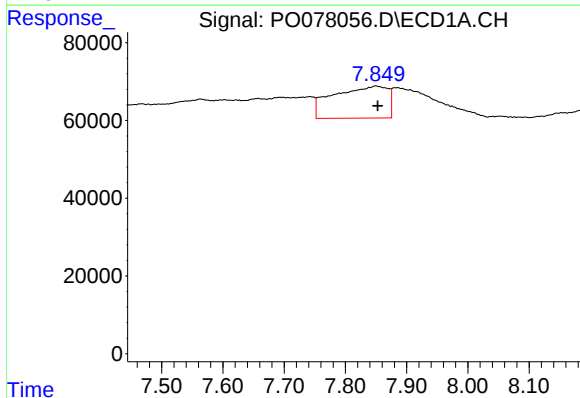


#30 AR-1254-5

R.T.: 7.850 min
Delta R.T.: -0.004 min
Response: 510748
Conc: 174.65 ng/ml

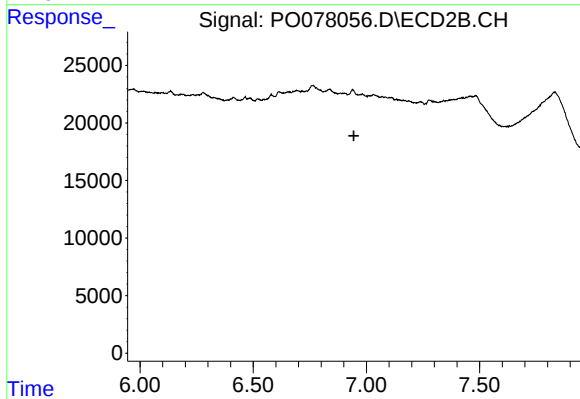

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 6.944 min
Response: 0
Conc: N.D.

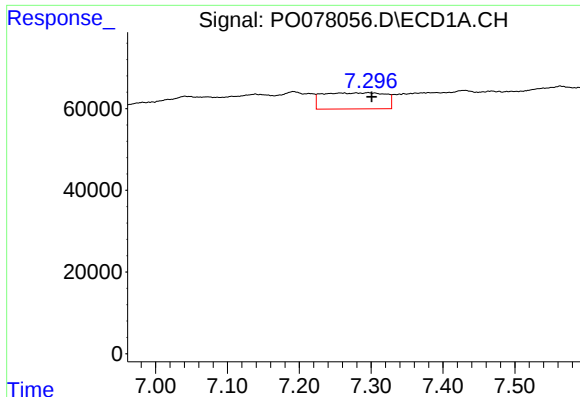

#31 AR-1260-1


R.T.: 7.296 min
Delta R.T.: -0.005 min
Response: 238029
Conc: 84.82 ng/ml

Instrument :
ECD_O
ClientSampleId :

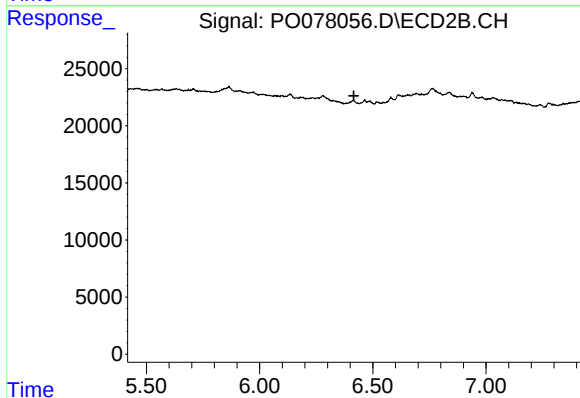


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.417 min
Response: 0
Conc: N.D.

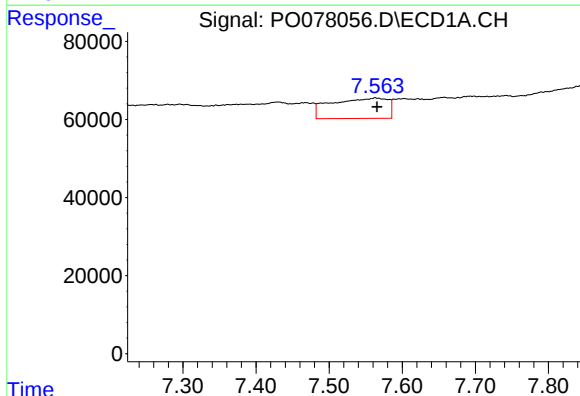


#32 AR-1260-2

R.T.: 7.563 min
Delta R.T.: -0.003 min
Response: 280908
Conc: 83.50 ng/ml

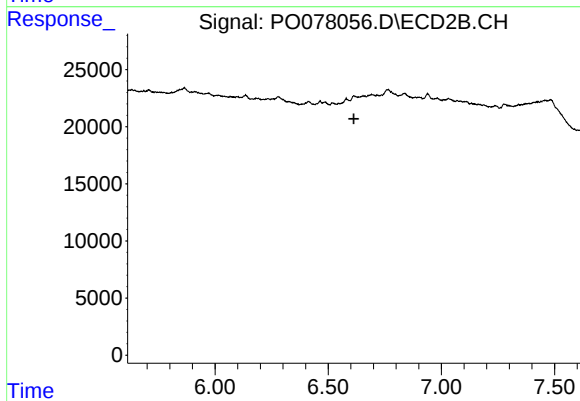

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.613 min
Response: 0
Conc: N.D.

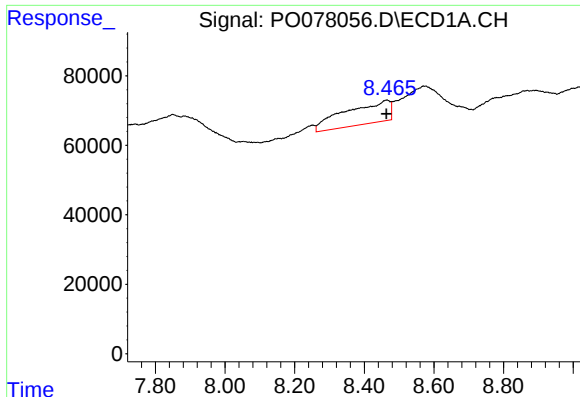

#35 AR-1260-5


R.T.: 8.465 min
Delta R.T.: 0.002 min
Response: 574452
Conc: 111.85 ng/ml

Instrument :
ECD_O
ClientSampleId :

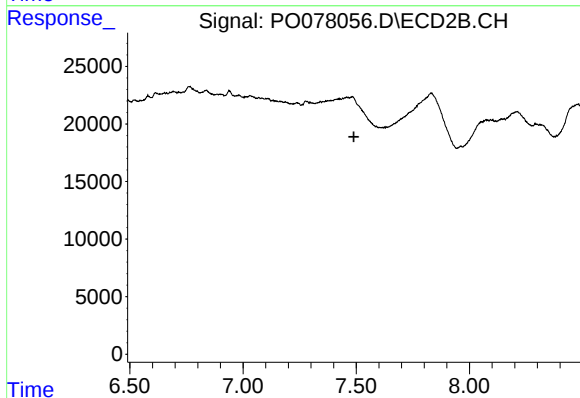


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.489 min
Response: 0
Conc: N.D.

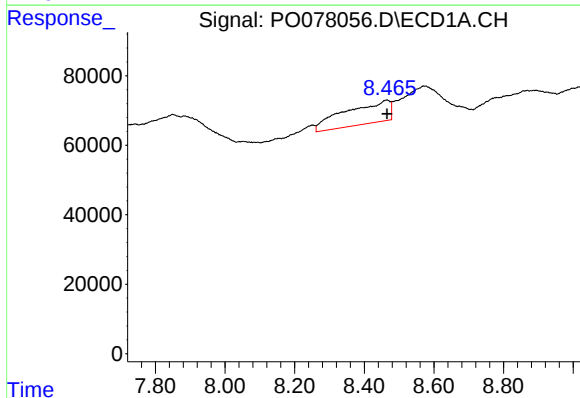


#37 AR-1262-2

R.T.: 8.465 min
Delta R.T.: 0.000 min
Response: 574452
Conc: 95.43 ng/ml

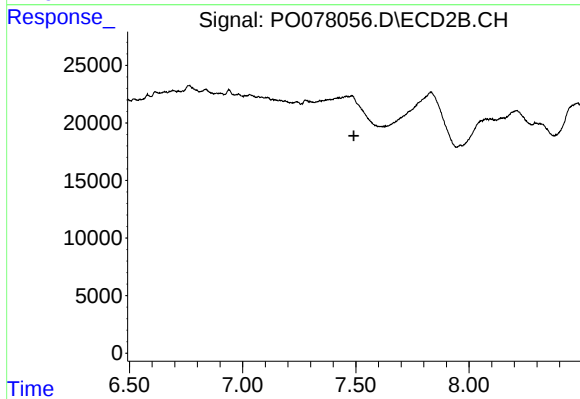

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.491 min
Response: 0
Conc: N.D.

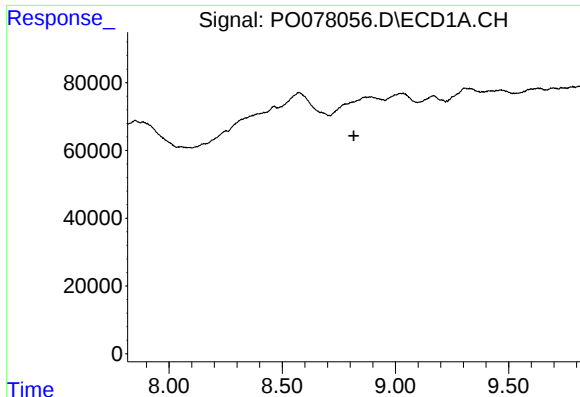

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.816 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

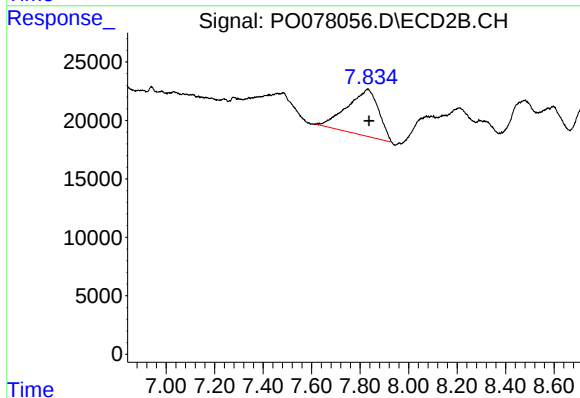


#39 AR-1262-4

R.T.: 7.829 min
Delta R.T.: -0.008 min
Response: 355130
Conc: 118.42 ng/ml

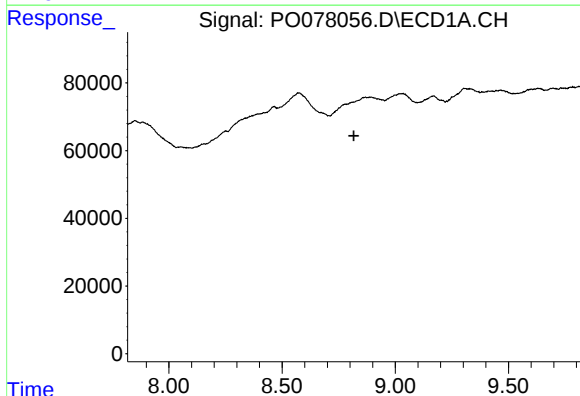

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.817 min
Response: 0
Conc: N.D.

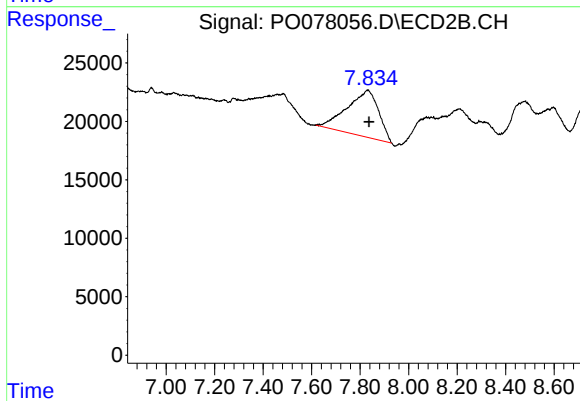

#42 AR-1268-2

R.T.: 7.829 min
Delta R.T.: -0.008 min
Response: 355130
Conc: 85.83 ng/ml