

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052022\
 Data File : P0086285.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 May 2022 2:07
 Operator : YP\AJ
 Sample : N2960-03
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BIN-4-SP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 04:51:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 19 09:06:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	3.676	2133502	894080	20.998	20.526
2)	SA Decachlor...	10.334	8.734	1027884	539509	18.930	15.503

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052022\
Data File : P0086285.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 May 2022 2:07
Operator : YP\AJ
Sample : N2960-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BIN-4-SP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 04:51:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 19 09:06:34 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

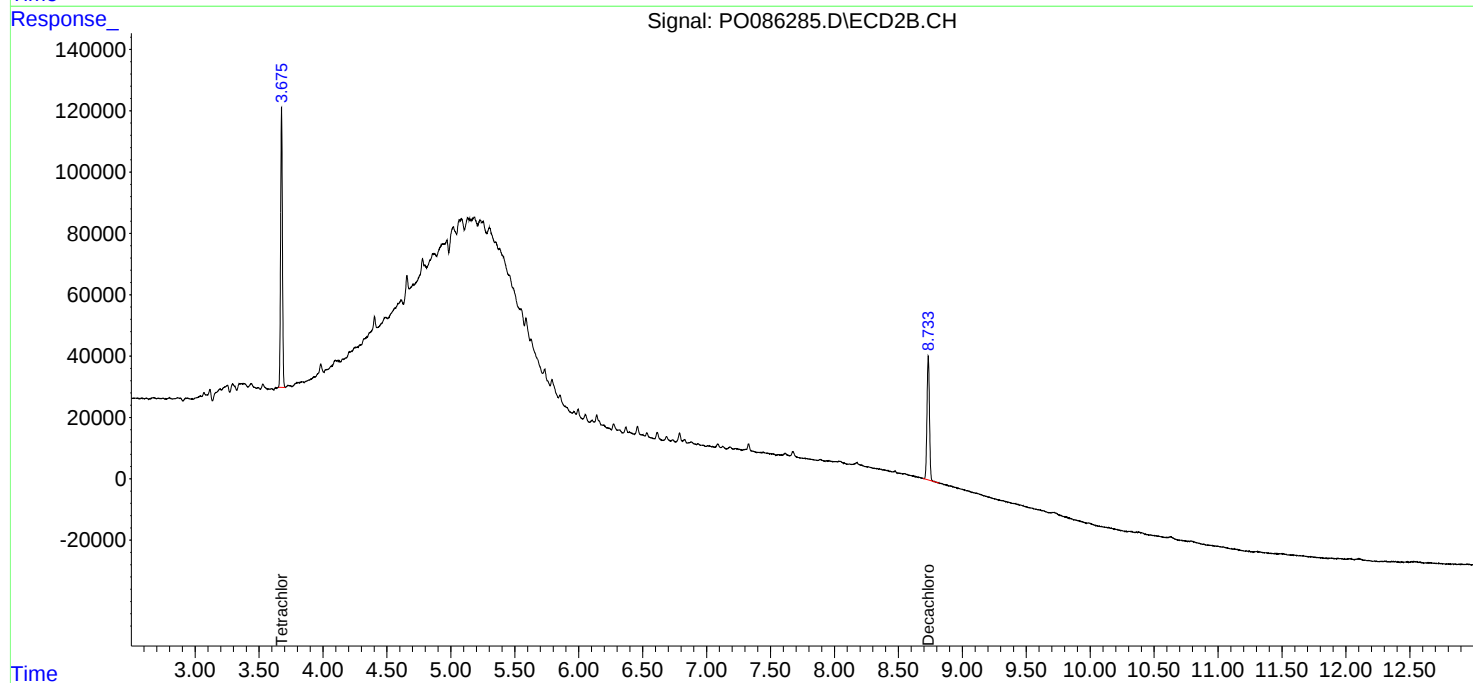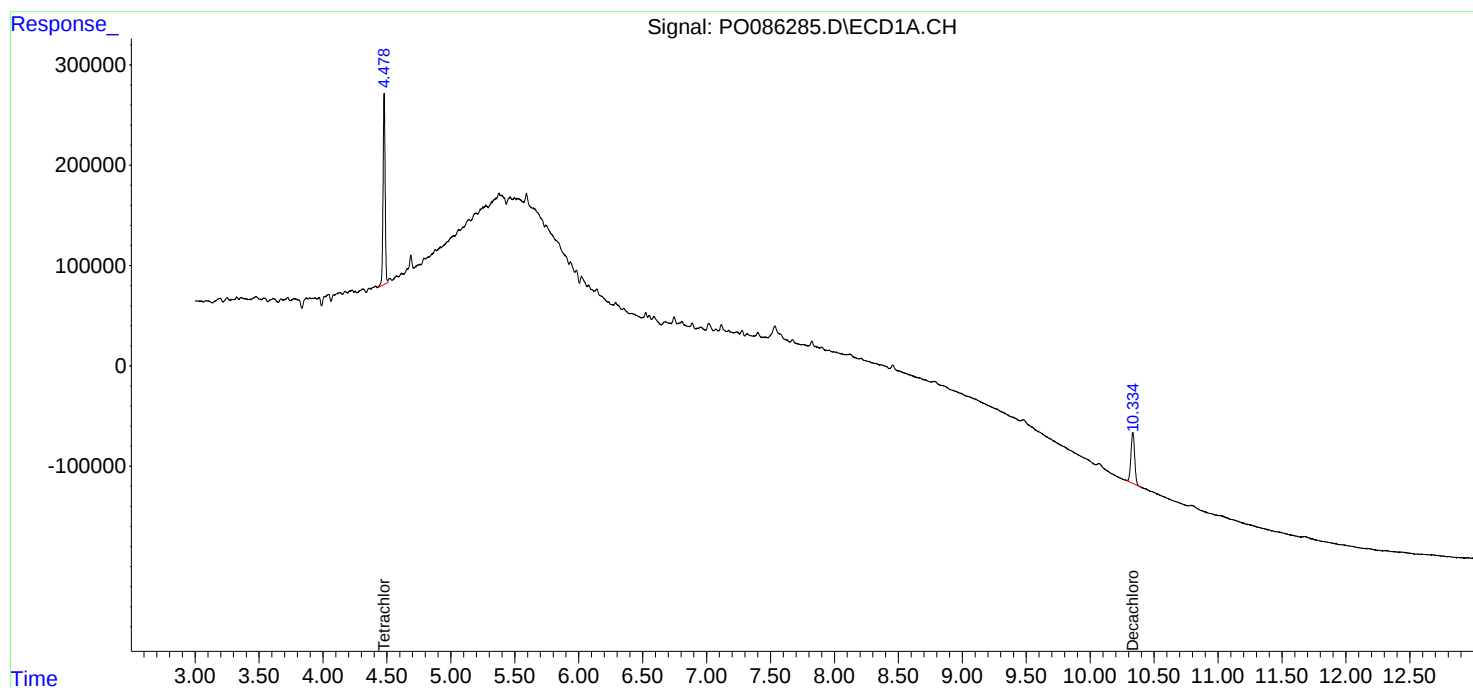


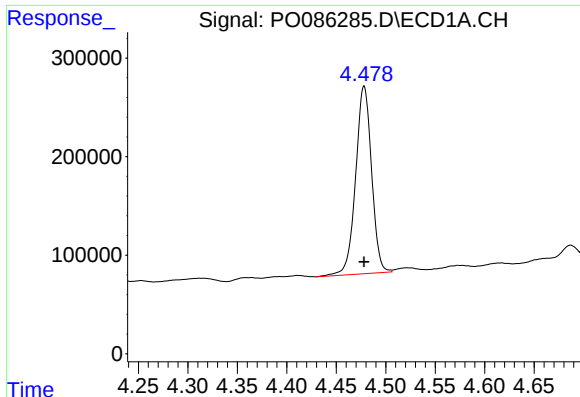

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: 0.000 min
Response: 2133502
Conc: 21.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
BIN-4-SP-2

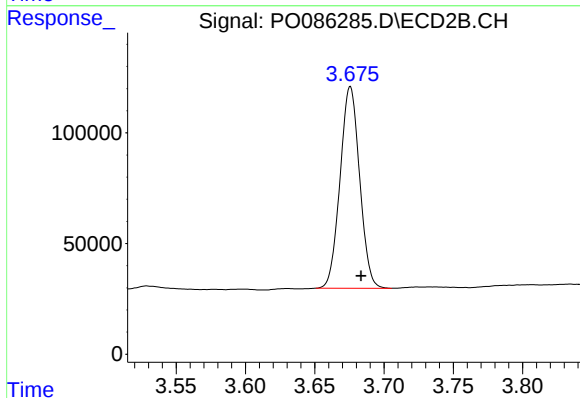


#1 Tetrachloro-m-xylene

R.T.: 3.676 min
Delta R.T.: -0.008 min
Response: 894080
Conc: 20.53 ng/ml

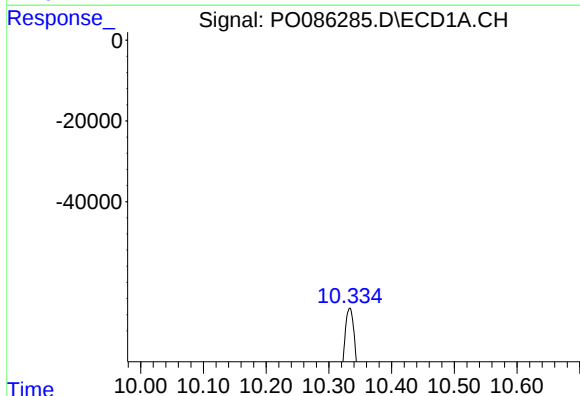

#2 Decachlorobiphenyl

R.T.: 10.334 min
Delta R.T.: 0.008 min
Response: 1027884
Conc: 18.93 ng/ml

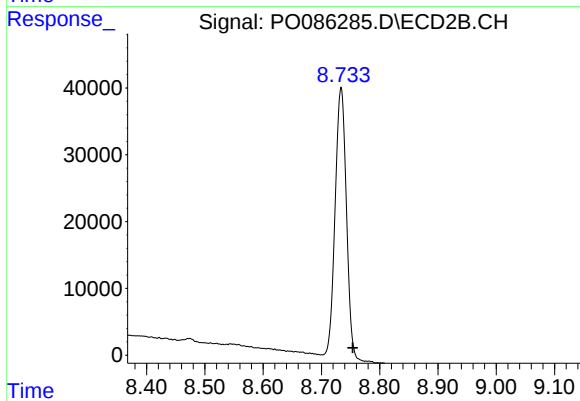

#2 Decachlorobiphenyl

R.T.: 8.734 min
Delta R.T.: -0.020 min
Response: 539509
Conc: 15.50 ng/ml