

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052024\
 Data File : P0103985.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2024 19:10
 Operator : YP/AJ
 Sample : P2511-07RE
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 510-ABRE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/21/2024
 Supervised By :Ankita Jodhani 05/21/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 22:39:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 16 04:14:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.449	3.583	122.8E6	44509682	15.957m	17.668
2) SA Decachlor...	10.205	8.535	26647343	6386117	5.622m	4.909

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052024\
Data File : P0103985.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2024 19:10
Operator : YP/AJ
Sample : P2511-07RE
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
510-ABRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/21/2024
Supervised By :Ankita Jodhani 05/21/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 22:39:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050624.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 16 04:14:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

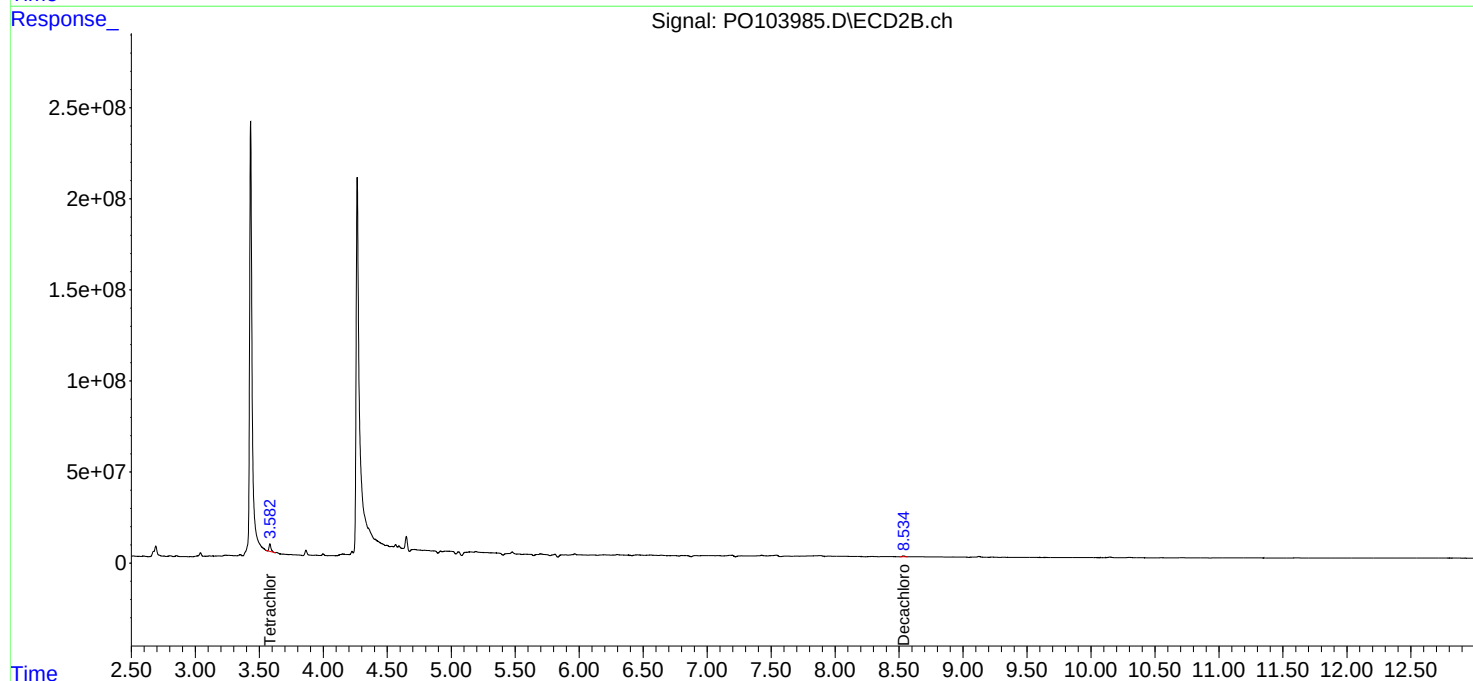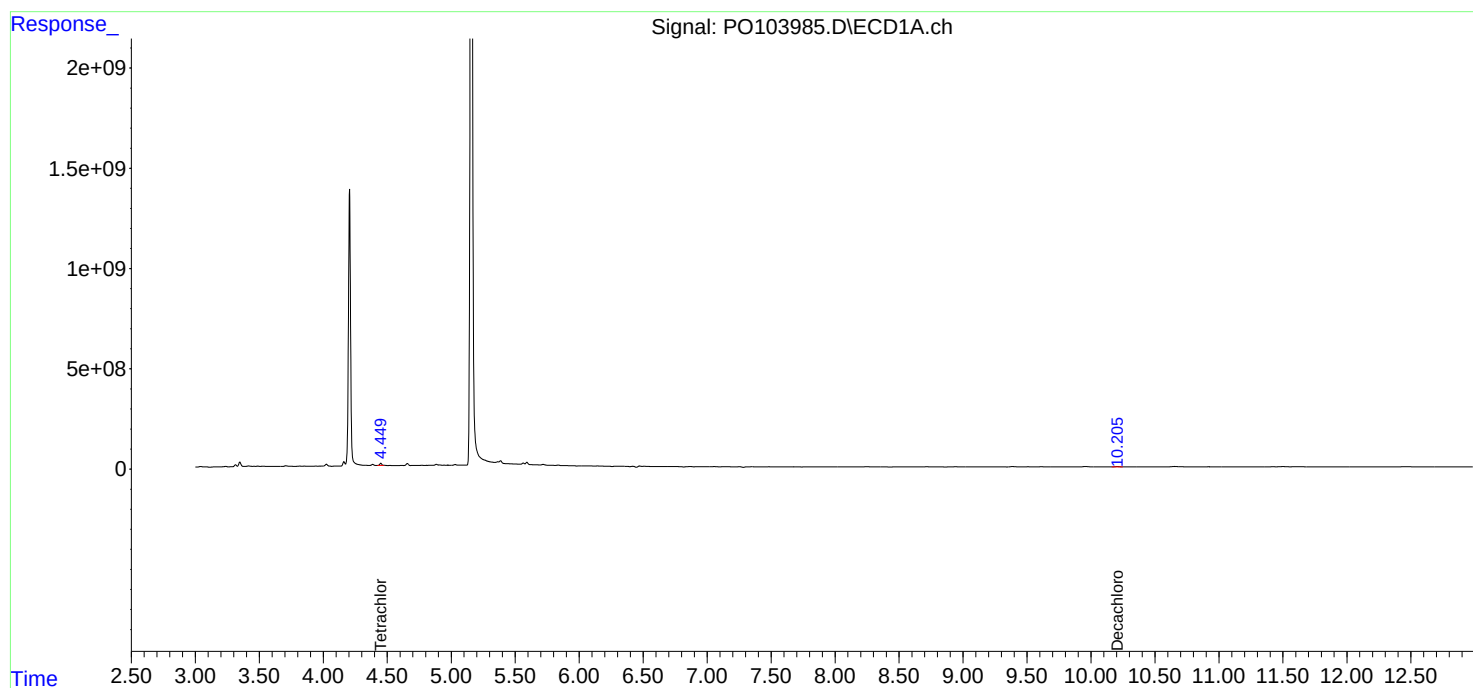

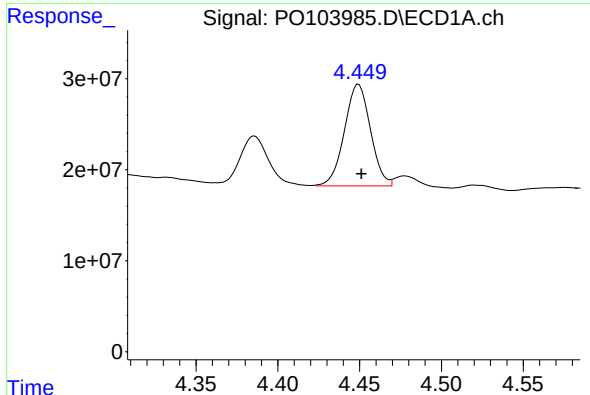


#1 Tetrachloro-m-xylene

R.T.: 4.449 min
Delta R.T.: -0.002 min
Response: 122802484
Conc: 15.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
510-ABRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/21/2024
Supervised By :Ankita Jodhani 05/21/2024

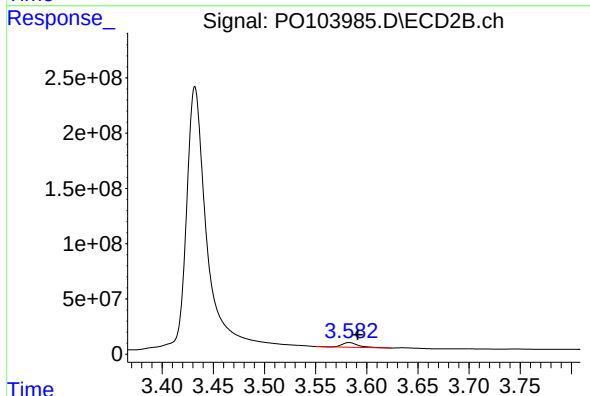


#1 Tetrachloro-m-xylene

R.T.: 3.583 min
Delta R.T.: -0.009 min
Response: 44509682
Conc: 17.67 ng/ml

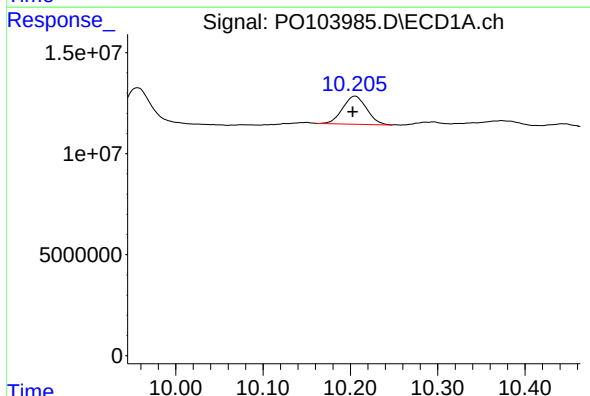

#2 Decachlorobiphenyl

R.T.: 10.205 min
Delta R.T.: 0.003 min
Response: 26647343
Conc: 5.62 ng/ml m

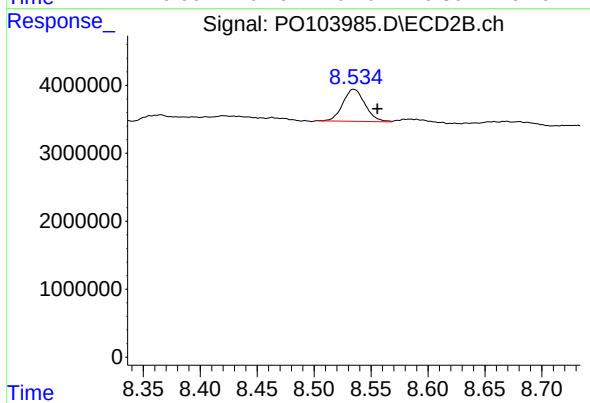

#2 Decachlorobiphenyl

R.T.: 8.535 min
Delta R.T.: -0.021 min
Response: 6386117
Conc: 4.91 ng/ml