

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052119\
 Data File : P0056447.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 May 2019 20:26
 Operator : SM/SJ
 Sample : K2241-09
 Misc : AR1242 MDL 25PPB
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 02:07:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 21 03:48:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.257	3.574	556443	484347	19.321	17.959
2)	SA Decachlor...	9.838	8.512	996752	813521	19.534	18.518
Target Compounds							
12)	L3 AR-1232-2	5.187	0.000	155997	0	235.863	N.D. #
20)	L4 AR-1242-5	6.266	0.000	22921	0	20.120	N.D. #
24)	L5 AR-1248-4	6.266	0.000	22921	0	12.570	N.D. #
26)	L6 AR-1254-1	6.266	0.000	22921	0	9.800	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052119\
Data File : P0056447.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 May 2019 20:26
Operator : SM/SJ
Sample : K2241-09
Misc : AR1242 MDL 25PPB
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 02:07:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052019.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 21 03:48:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

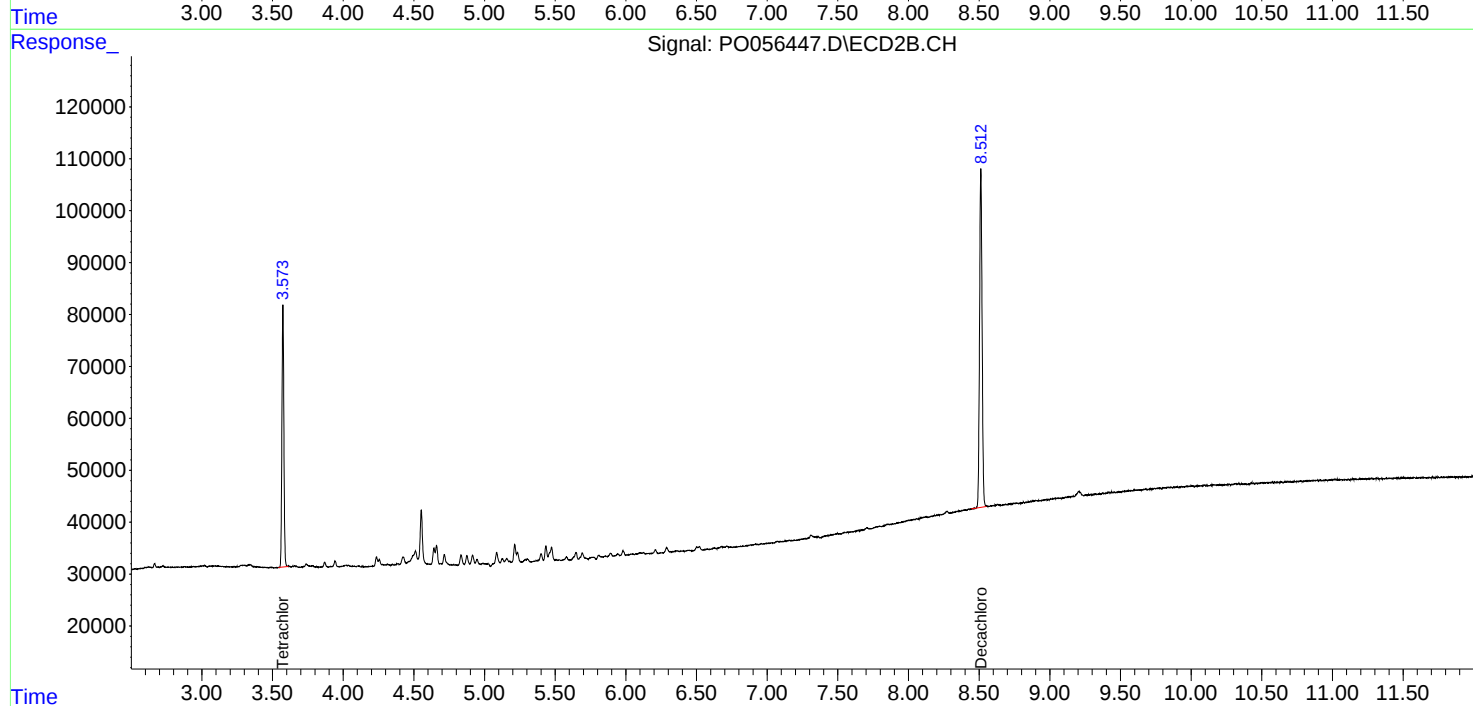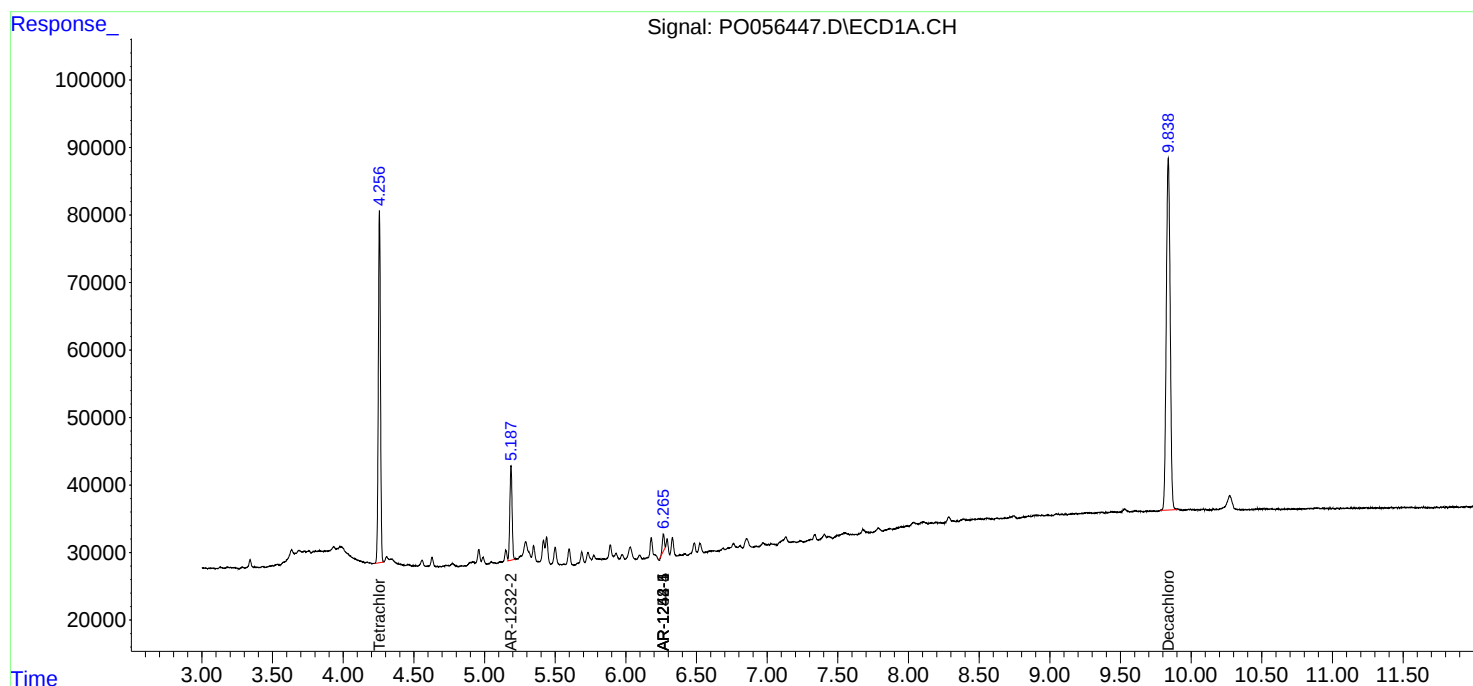


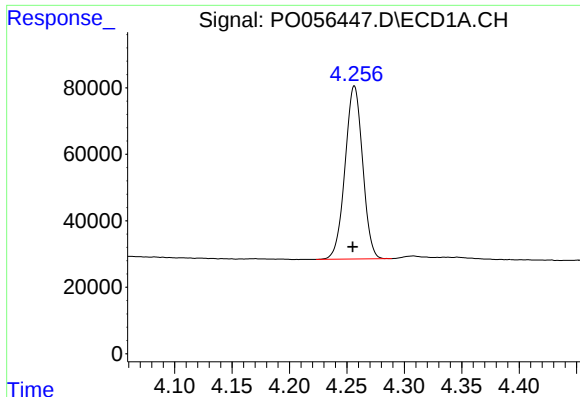

#1 Tetrachloro-m-xylene


R.T.: 4.257 min
Delta R.T.: 0.002 min
Response: 556443
Conc: 19.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

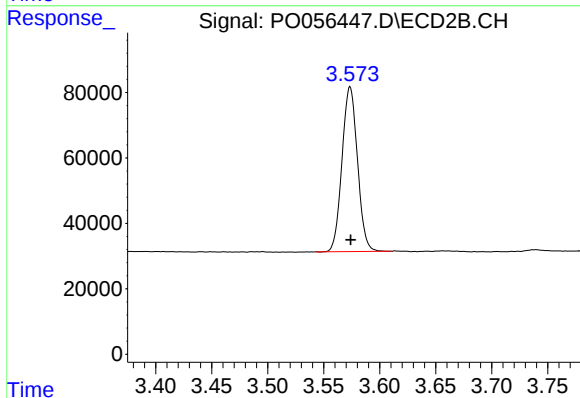


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: 0.000 min
Response: 484347
Conc: 17.96 ng/ml

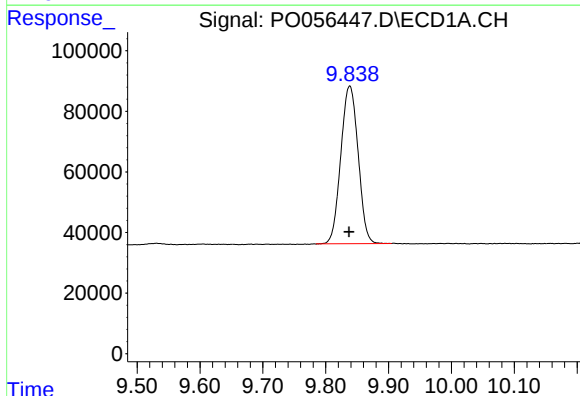


#2 Decachlorobiphenyl

R.T.: 9.838 min
Delta R.T.: 0.001 min
Response: 996752
Conc: 19.53 ng/ml

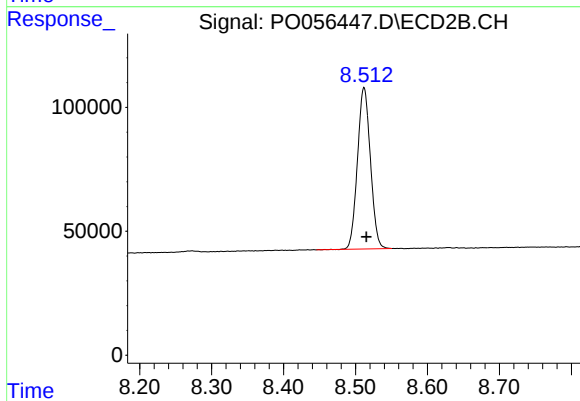

#2 Decachlorobiphenyl


R.T.: 8.512 min
Delta R.T.: -0.003 min
Response: 813521
Conc: 18.52 ng/ml

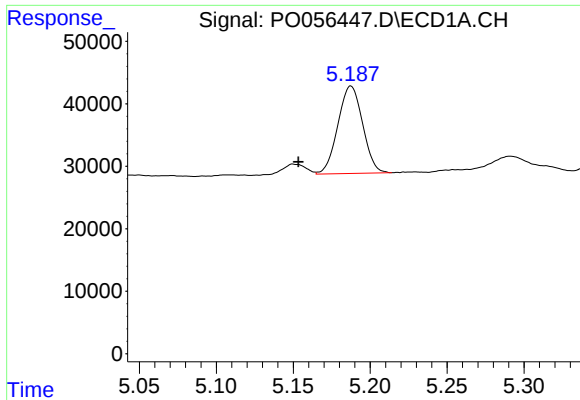

#12 AR-1232-2


R.T.: 5.187 min
Delta R.T.: 0.034 min
Response: 155997
Conc: 235.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

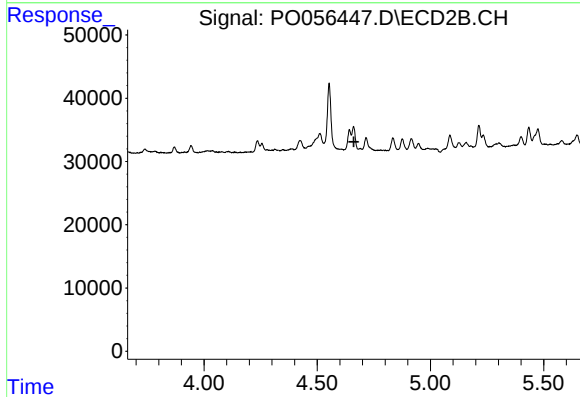


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 4.662 min
Response: 0
Conc: N.D.

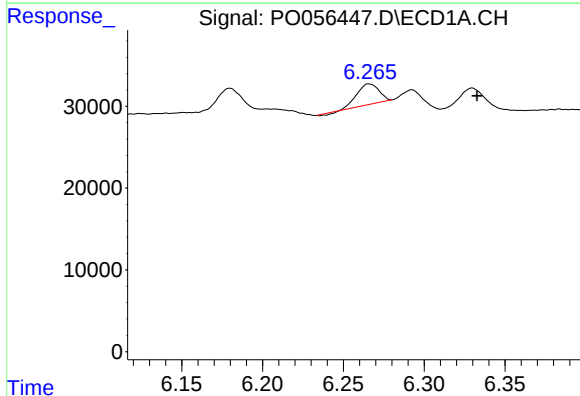


#20 AR-1242-5

R.T.: 6.266 min
Delta R.T.: -0.067 min
Response: 22921
Conc: 20.12 ng/ml

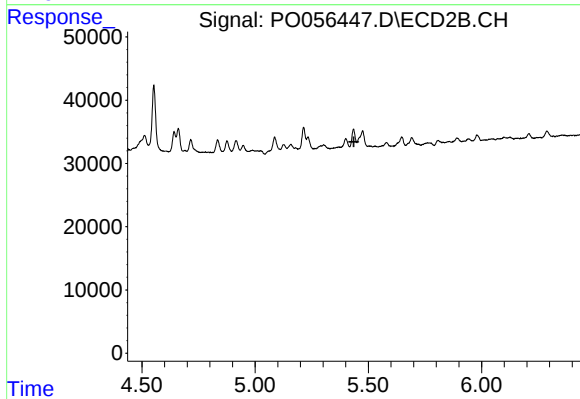

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 5.436 min
Response: 0
Conc: N.D.

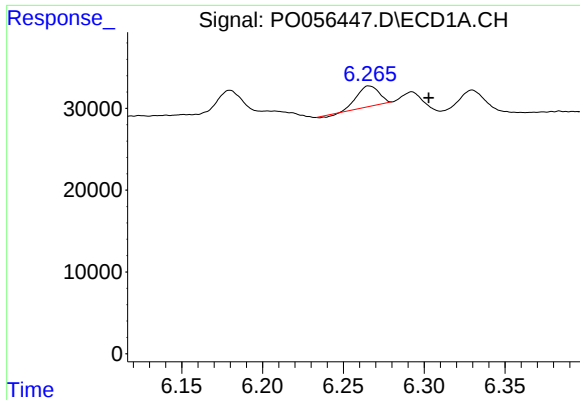

#24 AR-1248-4


R.T.: 6.266 min
Delta R.T.: -0.037 min
Response: 22921
Conc: 12.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

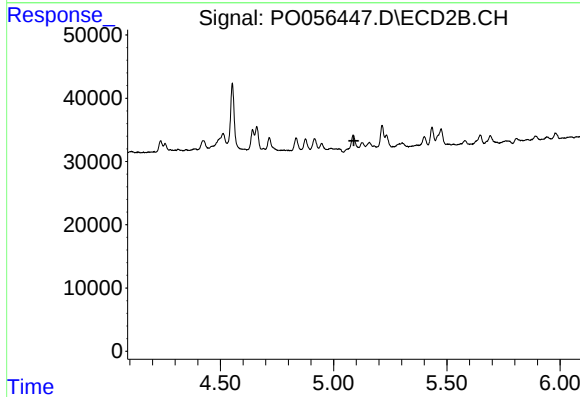


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.089 min
Response: 0
Conc: N.D.

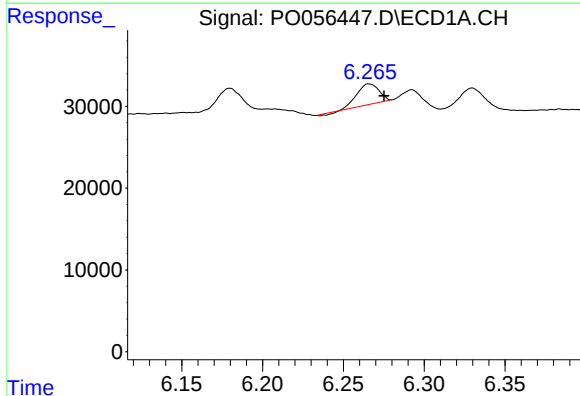

#26 AR-1254-1

R.T.: 6.266 min
Delta R.T.: -0.009 min
Response: 22921
Conc: 9.80 ng/ml

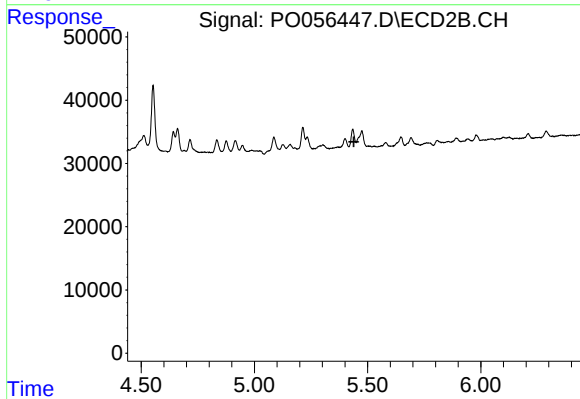

#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.439 min
Response: 0
Conc: N.D.