

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052119\
 Data File : P0056429.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 May 2019 14:23
 Operator : SM/SJ
 Sample : K2967-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TRAIN-2C

Manual Integrations
 APPROVED

Ankita
 5/22/2019 4:01:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 14:38:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 21 03:48:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.264	3.574	485819	541837	16.868m	20.091m
2) SA Decachlor...	9.850	8.517	673237	637233	13.194m	14.506

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO052119\
Data File : PO056429.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 May 2019 14:23
Operator : SM/SJ
Sample : K2967-05
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TRAIN-2C


Manual Integrations
APPROVED

Ankita
5/22/2019 4:01:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 14:38:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052019.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 21 03:48:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

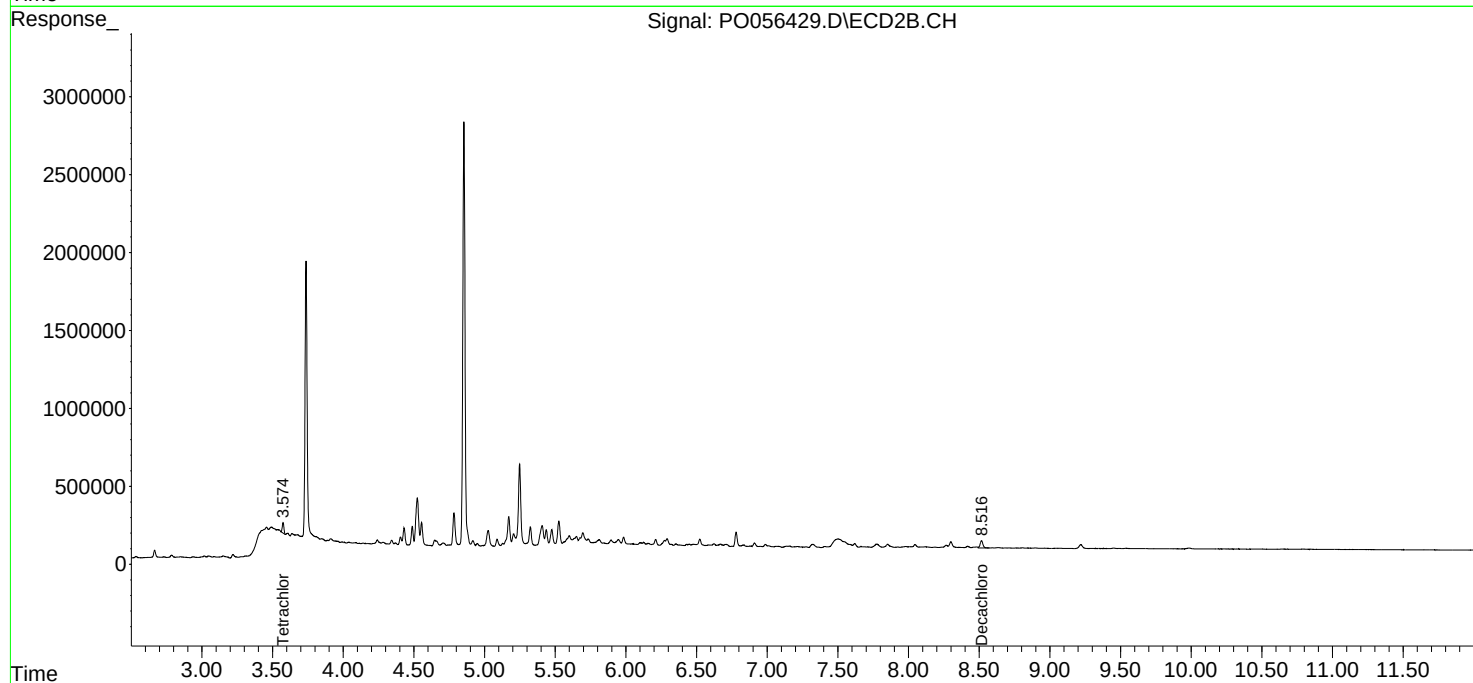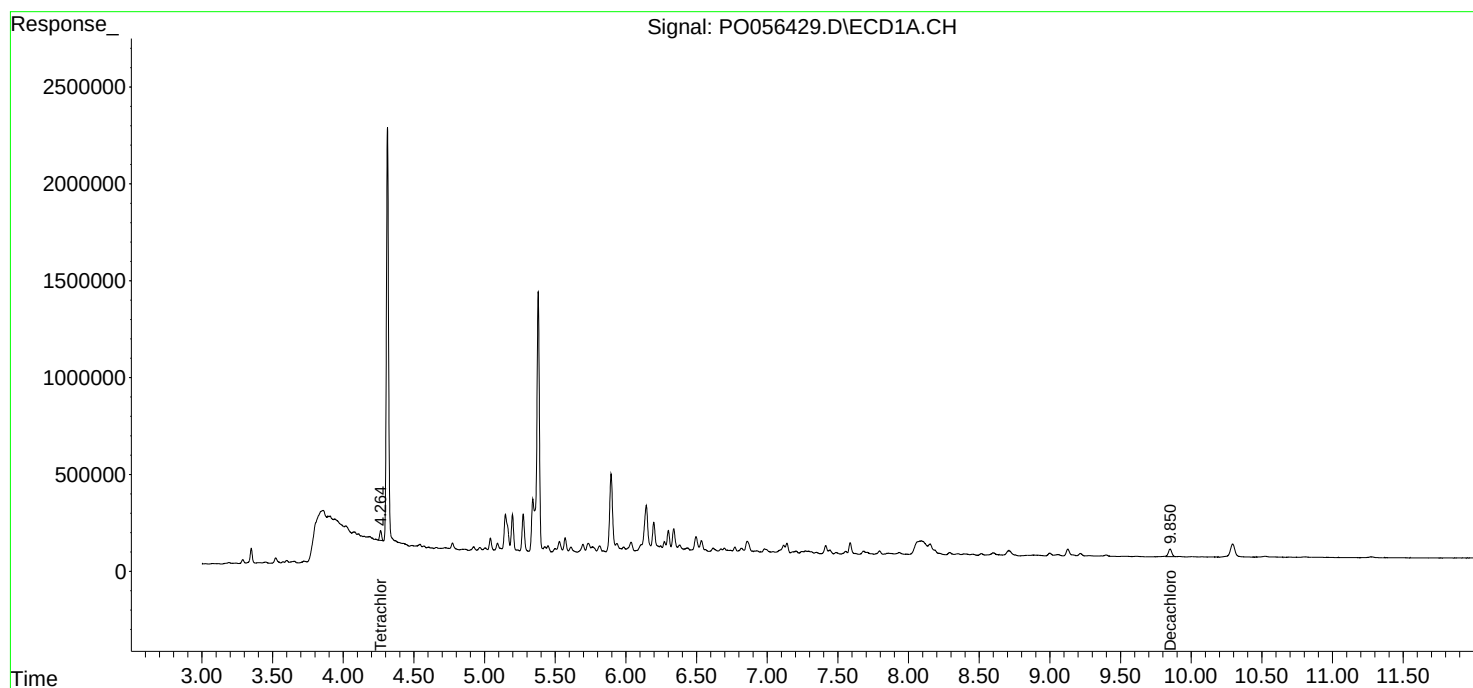

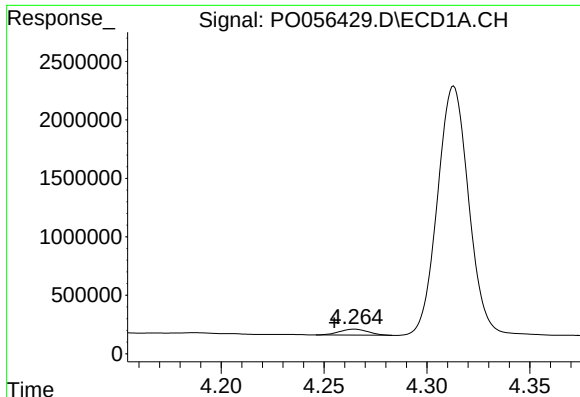


#1 Tetrachloro-m-xylene

R.T.: 4.264 min
Delta R.T.: 0.009 min
Response: 485819
Conc: 16.87 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TRAIN-2C


Manual Integrations
APPROVED

Ankita
5/22/2019 4:01:43 PM

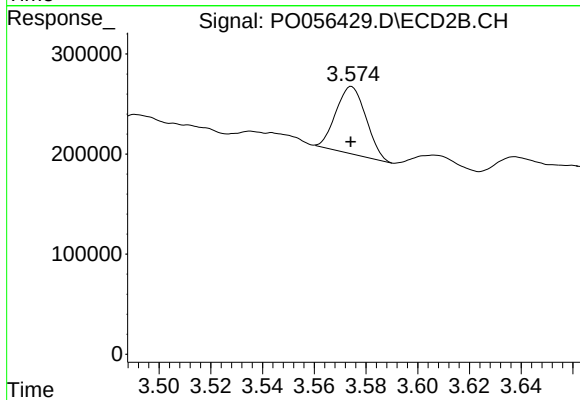


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: 0.000 min
Response: 541837
Conc: 20.09 ng/ml m

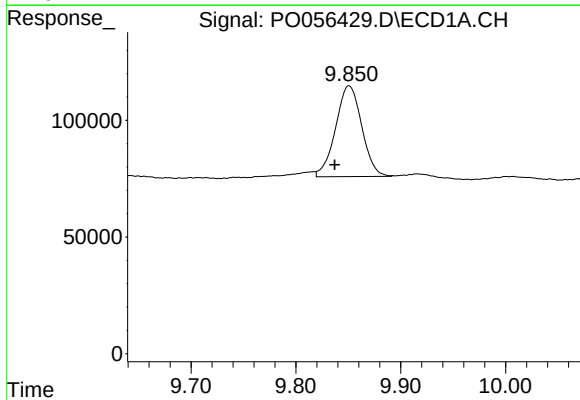

#2 Decachlorobiphenyl

R.T.: 9.850 min
Delta R.T.: 0.013 min
Response: 673237
Conc: 13.19 ng/ml m

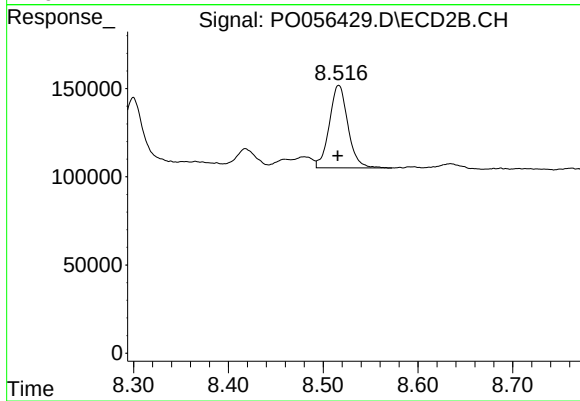

#2 Decachlorobiphenyl

R.T.: 8.517 min
Delta R.T.: 0.001 min
Response: 637233
Conc: 14.51 ng/ml