

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0052119\
 Data File : P0056447.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 May 2019 20:26
 Operator : SM/SJ
 Sample : K2241-09
 Misc : AR1242 MDL 25PPB
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 MDL-MDL-WATER-03-QT2-2019

Manual Integrations
 APPROVED

Ankita
 5/22/2019 4:02:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 05:08:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0052019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 21 03:48:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.257	3.574	556443	484347	19.321	17.959
2)	SA Decachlor...	9.838	8.512	996752	813521	19.534	18.518
Target Compounds							
16)	L4 AR-1242-1	5.417	4.641	34558	29461	29.511m	28.253m
17)	L4 AR-1242-2	5.439	4.660	44097	34976	27.002m	24.627m
18)	L4 AR-1242-3	5.500	4.833	30268	21662	28.169m	26.173m
19)	L4 AR-1242-4	5.598	4.915	26062	18439	29.327m	22.967m
20)	L4 AR-1242-5	6.329	5.434	30738	27202	26.981m	24.569m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO052119\
Data File : PO056447.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 May 2019 20:26
Operator : SM/SJ
Sample : K2241-09
Misc : AR1242 MDL 25PPB
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019


Manual Integrations
APPROVED

Ankita
5/22/2019 4:02:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 05:08:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052019.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 21 03:48:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

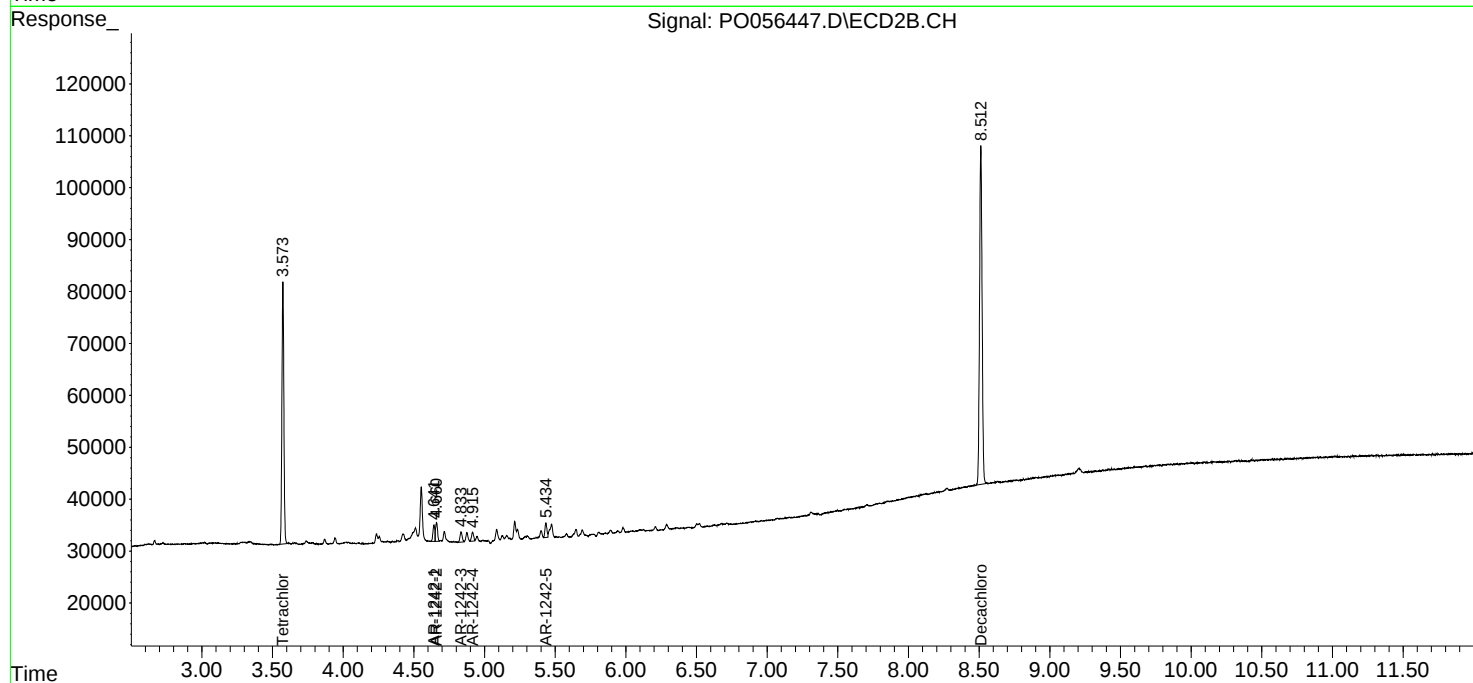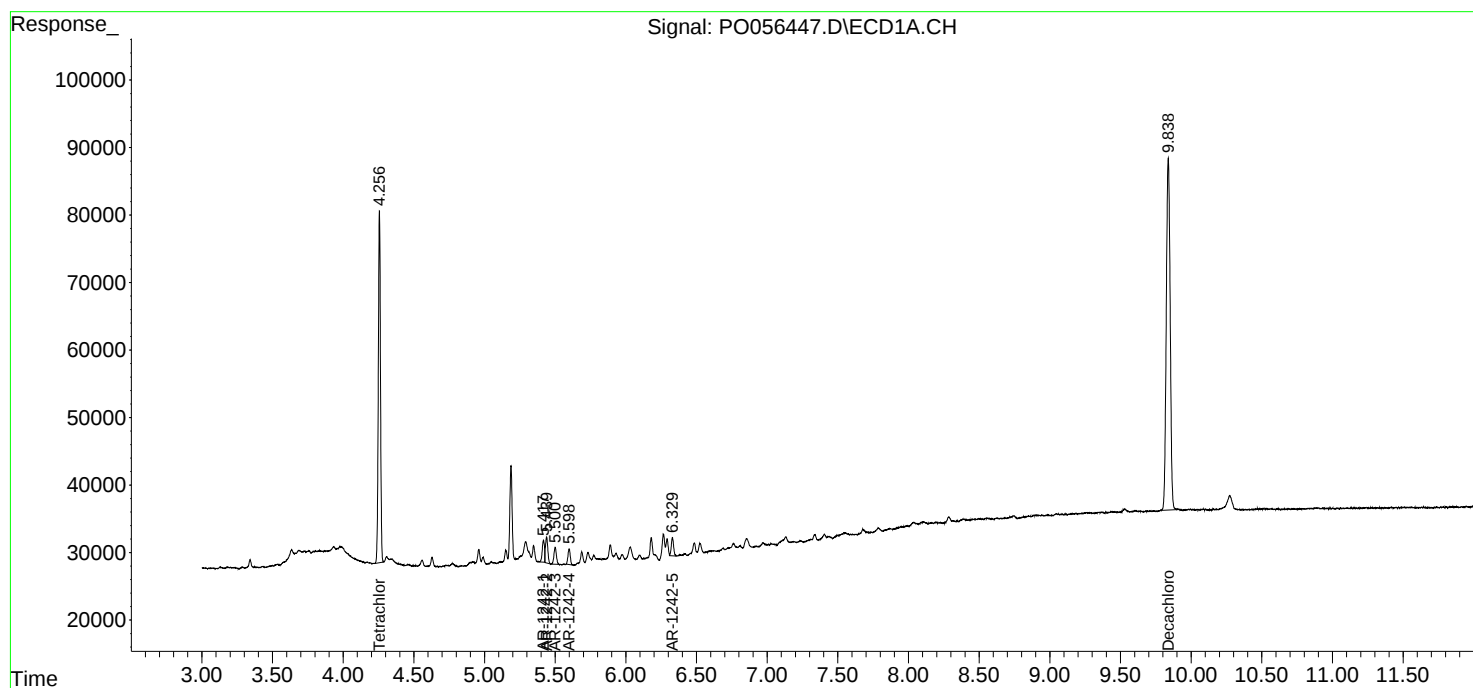

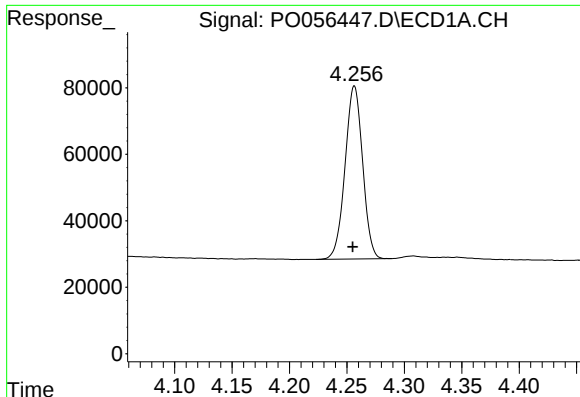


#1 Tetrachloro-m-xylene

R.T.: 4.257 min
Delta R.T.: 0.002 min
Response: 556443
Conc: 19.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019


Manual Integrations
APPROVED

Ankita
5/22/2019 4:02:52 PM

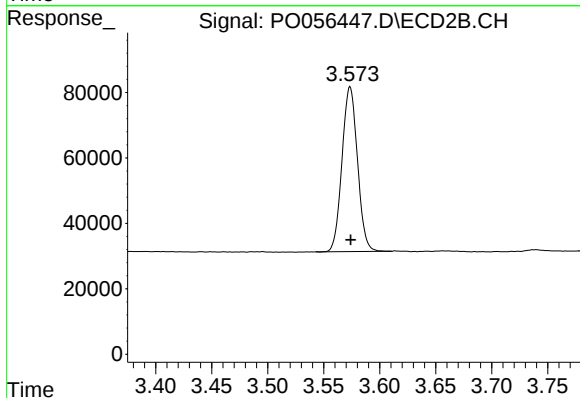


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: 0.000 min
Response: 484347
Conc: 17.96 ng/ml

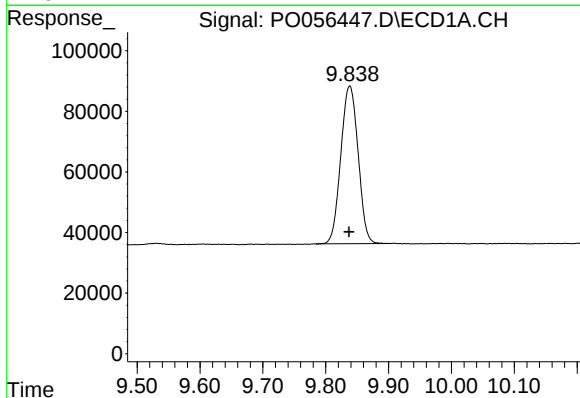


#2 Decachlorobiphenyl

R.T.: 9.838 min
Delta R.T.: 0.001 min
Response: 996752
Conc: 19.53 ng/ml

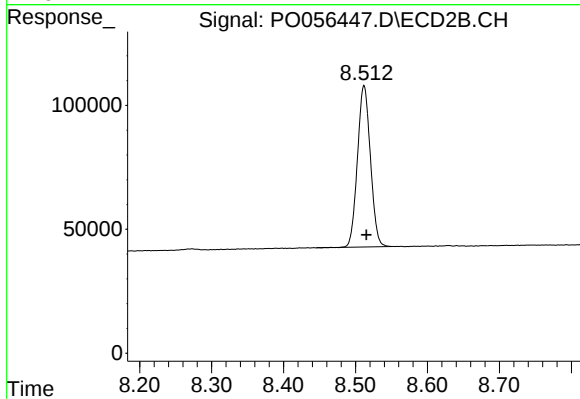

#2 Decachlorobiphenyl

R.T.: 8.512 min
Delta R.T.: -0.003 min
Response: 813521
Conc: 18.52 ng/ml

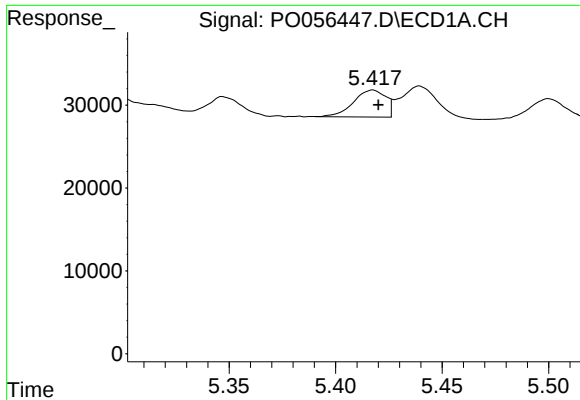


#16 AR-1242-1

R.T.: 5.417 min
Delta R.T.: -0.003 min
Response: 34558
Conc: 29.51 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019


Manual Integrations
APPROVED

Ankita
5/22/2019 4:02:52 PM

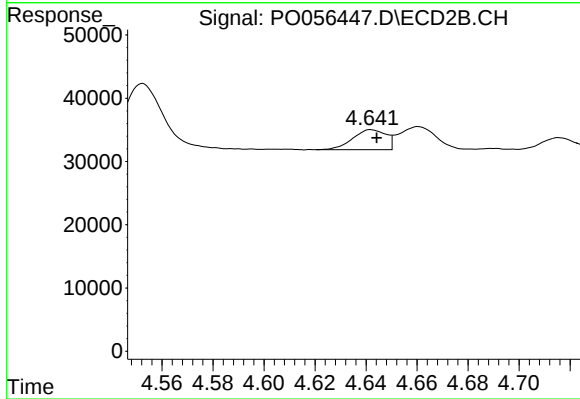


#16 AR-1242-1

R.T.: 4.641 min
Delta R.T.: -0.003 min
Response: 29461
Conc: 28.25 ng/ml m

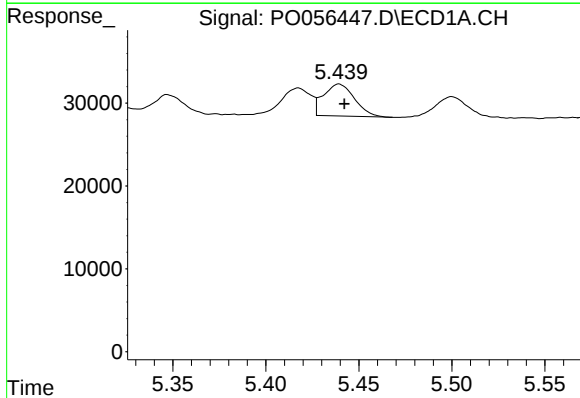


#17 AR-1242-2

R.T.: 5.439 min
Delta R.T.: -0.003 min
Response: 44097
Conc: 27.00 ng/ml m

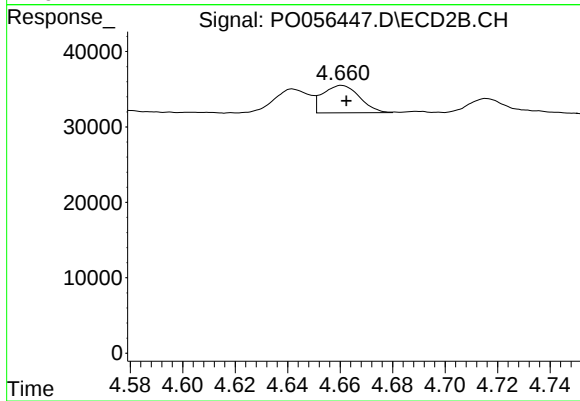

#17 AR-1242-2

R.T.: 4.660 min
Delta R.T.: -0.002 min
Response: 34976
Conc: 24.63 ng/ml m

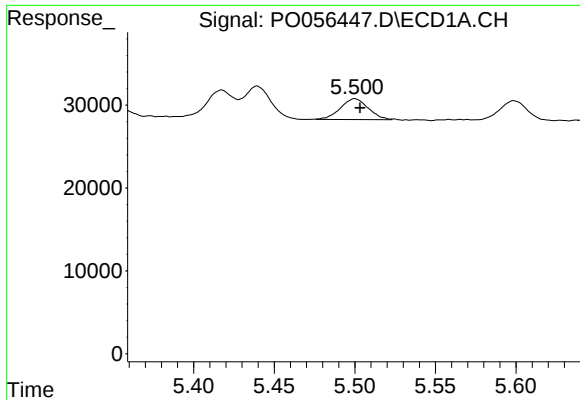


#18 AR-1242-3

R.T.: 5.500 min
Delta R.T.: -0.004 min
Response: 30268
Conc: 28.17 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019


Manual Integrations
APPROVED

Ankita
5/22/2019 4:02:52 PM

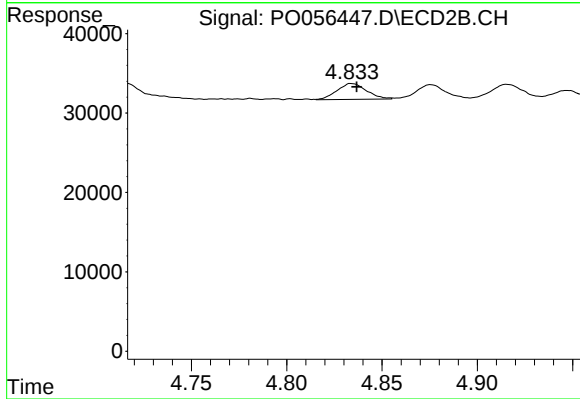


#18 AR-1242-3

R.T.: 4.833 min
Delta R.T.: -0.004 min
Response: 21662
Conc: 26.17 ng/ml m

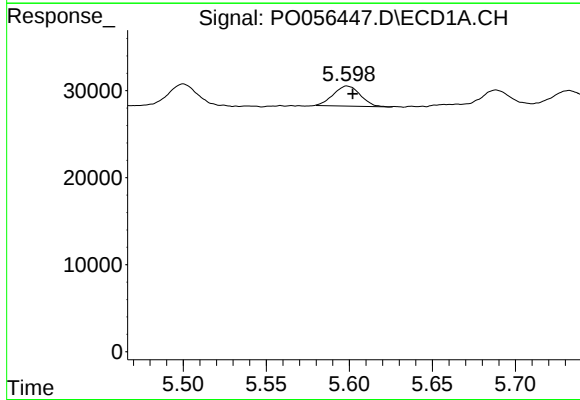


#19 AR-1242-4

R.T.: 5.598 min
Delta R.T.: -0.004 min
Response: 26062
Conc: 29.33 ng/ml m

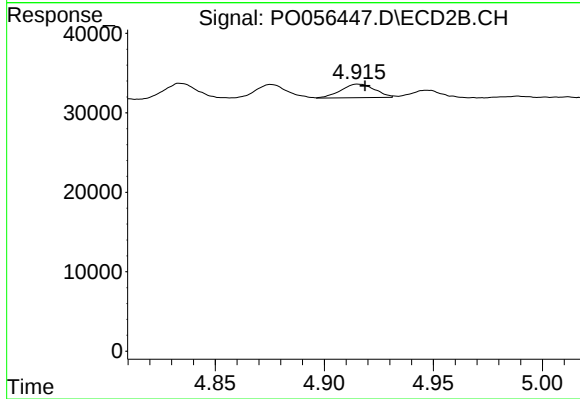

#19 AR-1242-4

R.T.: 4.915 min
Delta R.T.: -0.004 min
Response: 18439
Conc: 22.97 ng/ml m

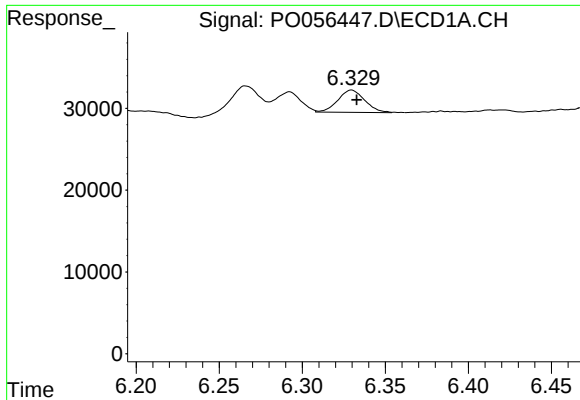


#20 AR-1242-5

R.T.: 6.329 min
Delta R.T.: -0.003 min
Response: 30738
Conc: 26.98 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

Manual Integrations
APPROVED

Ankita
5/22/2019 4:02:52 PM

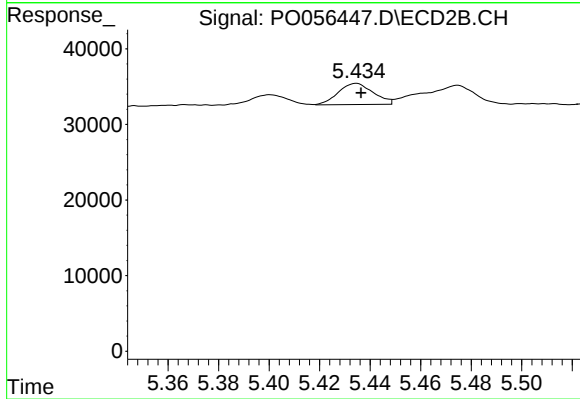

#20 AR-1242-5

R.T.: 5.434 min
Delta R.T.: -0.002 min
Response: 27202
Conc: 24.57 ng/ml m