

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0052119\
 Data File : P0056448.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 May 2019 20:42
 Operator : SM/SJ
 Sample : K2241-09
 Misc : AR1248 MDL 25PPB
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT2-2019

Manual Integrations
 APPROVED

Ankita
 5/22/2019 4:02:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 05:11:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0052019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 21 03:48:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.257	3.574	623847	549891	21.661	20.390
2) SA Decachlor...	9.840	8.513	1098384	903365	21.526	20.564
Target Compounds						
21) L5 AR-1248-1	5.418	4.642	24586	24324	27.154m	30.360m
22) L5 AR-1248-2	5.688	4.875	36162	31754	27.455m	29.369m
23) L5 AR-1248-3	5.890	4.917	36561	26389	24.582	23.447m
24) L5 AR-1248-4	6.291	5.086	35663	40047	19.557m	28.129m#
25) L5 AR-1248-5	6.329	5.474	40711	20599	23.188m	13.451m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO052119\
Data File : PO056448.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 May 2019 20:42
Operator : SM/SJ
Sample : K2241-09
Misc : AR1248 MDL 25PPB
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019


Manual Integrations
APPROVED

Ankita
5/22/2019 4:02:59 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 05:11:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052019.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 21 03:48:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

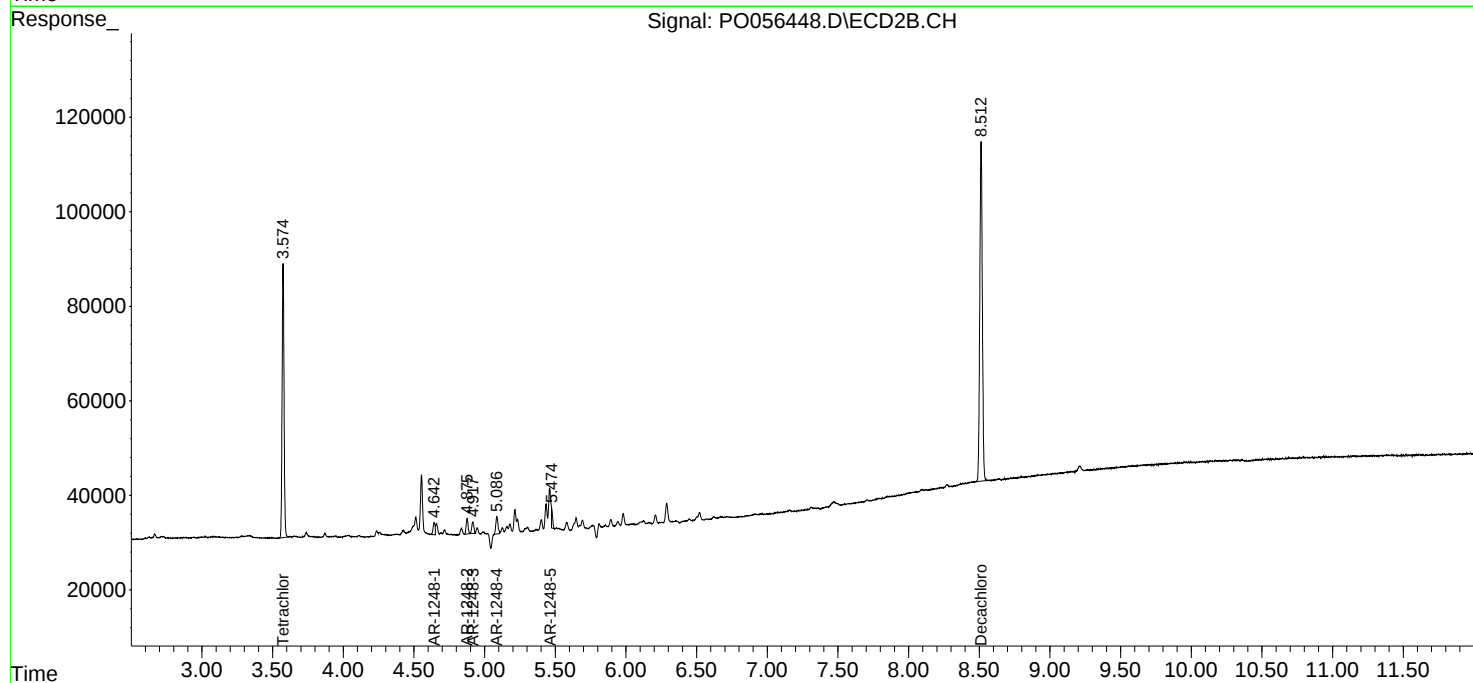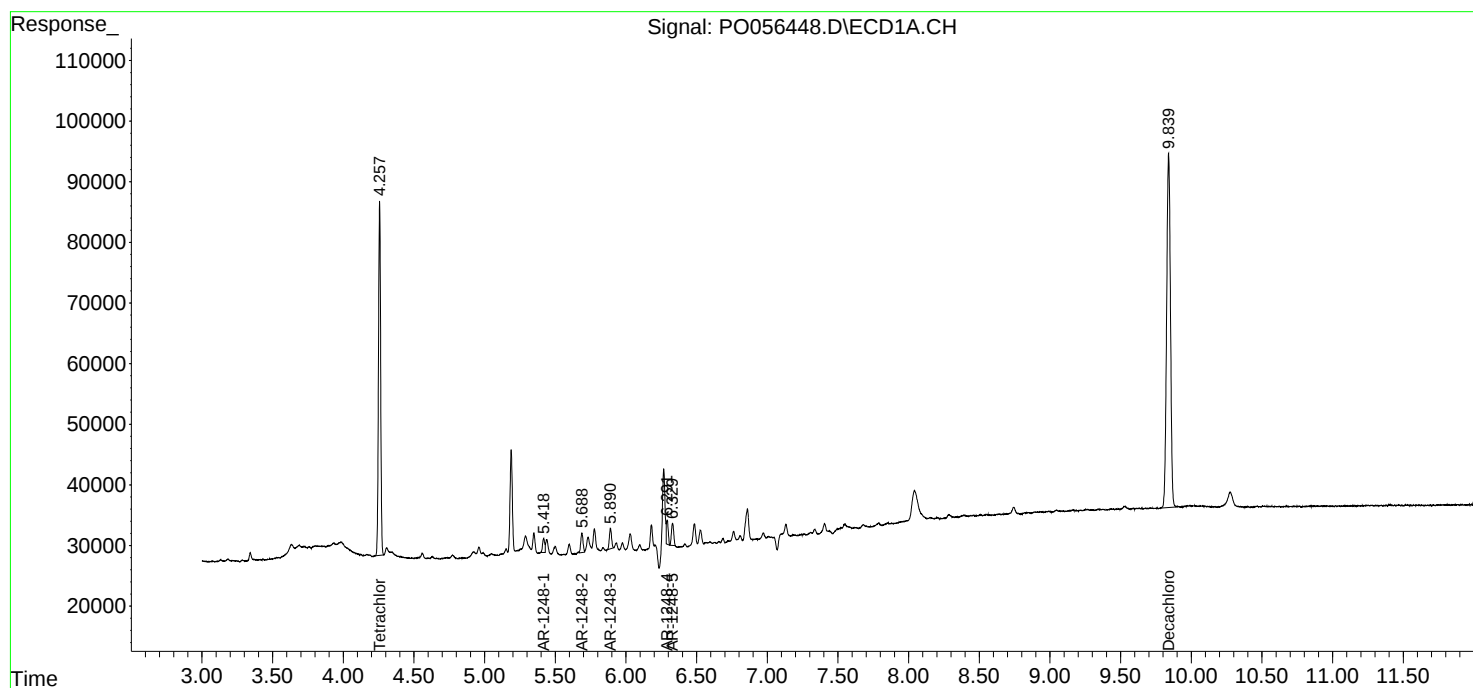

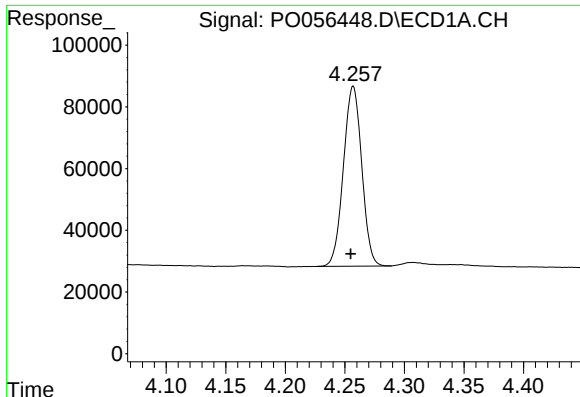


#1 Tetrachloro-m-xylene

R.T.: 4.257 min
Delta R.T.: 0.002 min
Response: 623847
Conc: 21.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019


Manual Integrations
APPROVED

Ankita
5/22/2019 4:02:59 PM

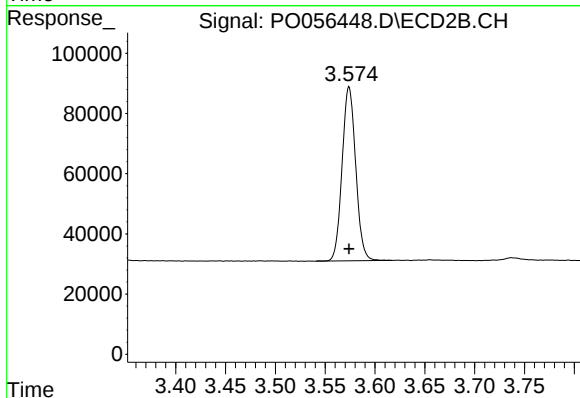


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: 0.000 min
Response: 549891
Conc: 20.39 ng/ml

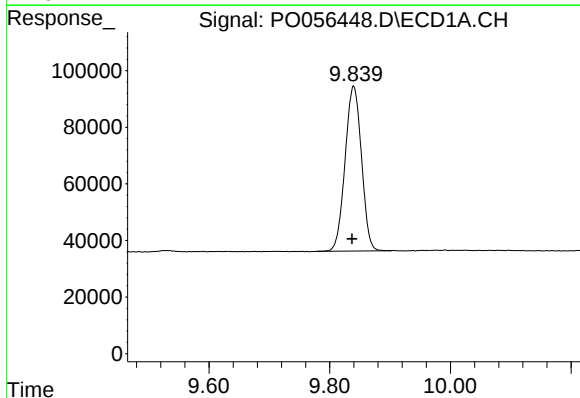


#2 Decachlorobiphenyl

R.T.: 9.840 min
Delta R.T.: 0.003 min
Response: 1098384
Conc: 21.53 ng/ml

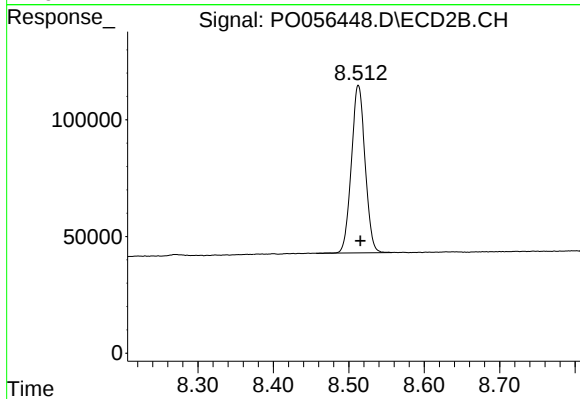

#2 Decachlorobiphenyl

R.T.: 8.513 min
Delta R.T.: -0.003 min
Response: 903365
Conc: 20.56 ng/ml

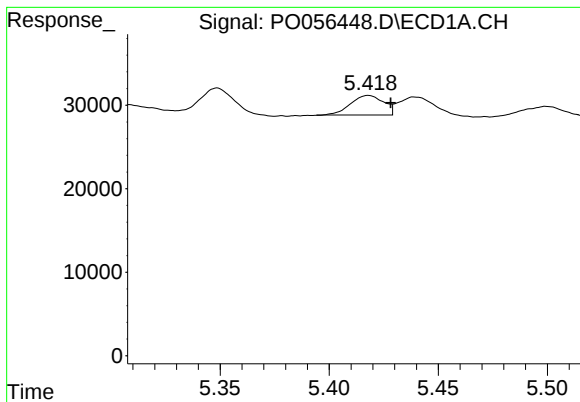


#21 AR-1248-1

R.T.: 5.418 min
Delta R.T.: -0.011 min
Response: 24586
Conc: 27.15 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019


Manual Integrations
APPROVED

Ankita
5/22/2019 4:02:59 PM

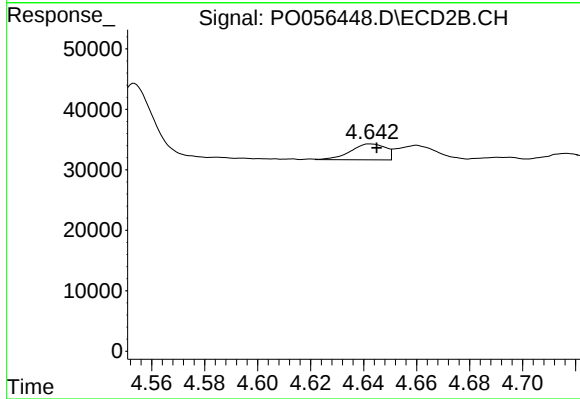


#21 AR-1248-1

R.T.: 4.642 min
Delta R.T.: -0.003 min
Response: 24324
Conc: 30.36 ng/ml m

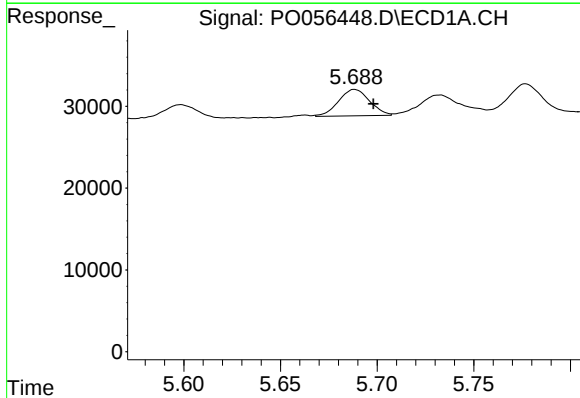


#22 AR-1248-2

R.T.: 5.688 min
Delta R.T.: -0.010 min
Response: 36162
Conc: 27.46 ng/ml m

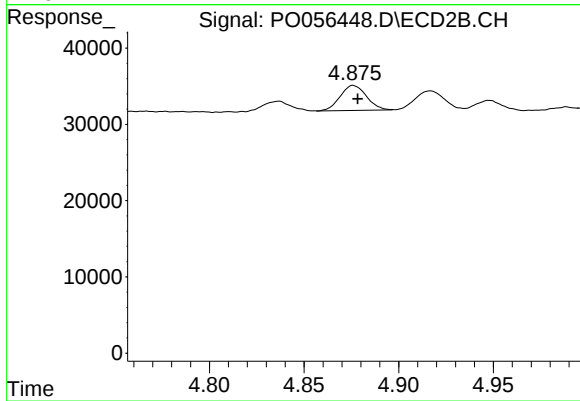

#22 AR-1248-2

R.T.: 4.875 min
Delta R.T.: -0.003 min
Response: 31754
Conc: 29.37 ng/ml m

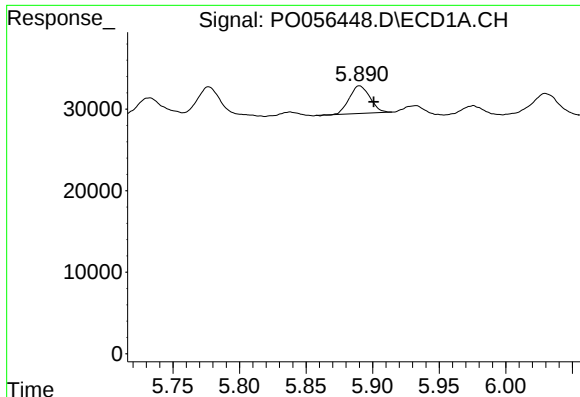


#23 AR-1248-3

R.T.: 5.890 min
Delta R.T.: -0.011 min
Response: 36561
Conc: 24.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019


Manual Integrations
APPROVED

Ankita
5/22/2019 4:02:59 PM

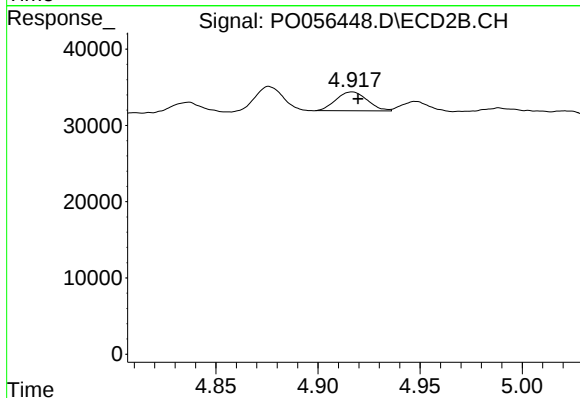


#23 AR-1248-3

R.T.: 4.917 min
Delta R.T.: -0.003 min
Response: 26389
Conc: 23.45 ng/ml m

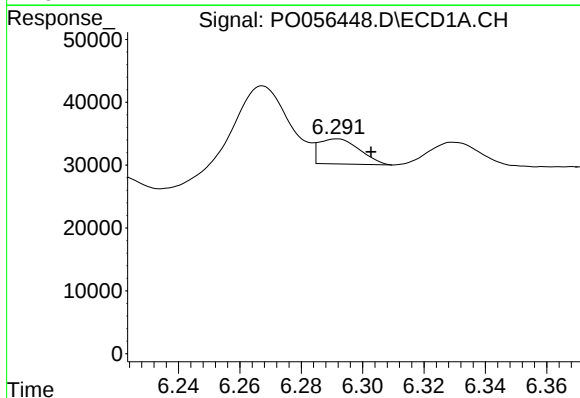


#24 AR-1248-4

R.T.: 6.291 min
Delta R.T.: -0.012 min
Response: 35663
Conc: 19.56 ng/ml m

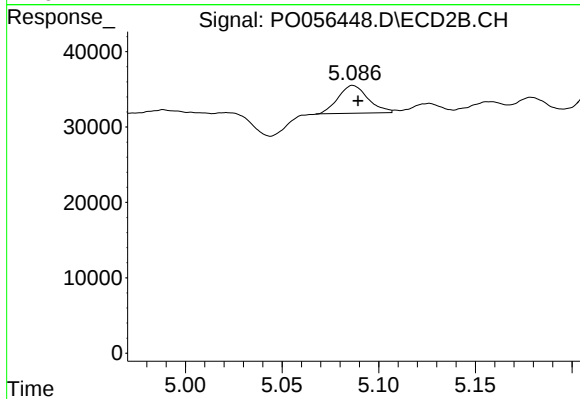

#24 AR-1248-4

R.T.: 5.086 min
Delta R.T.: -0.003 min
Response: 40047
Conc: 28.13 ng/ml m

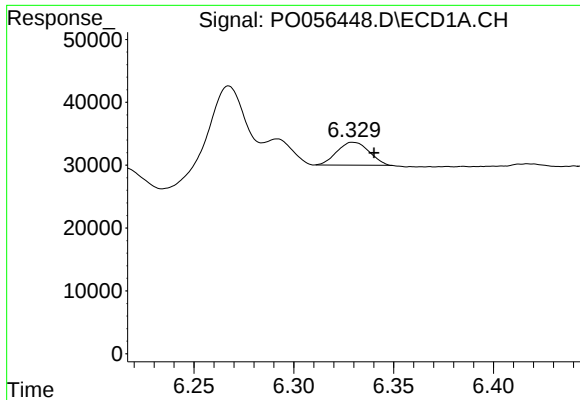


#25 AR-1248-5

R.T.: 6.329 min
Delta R.T.: -0.011 min
Response: 40711
Conc: 23.19 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

Manual Integrations
APPROVED

Ankita
5/22/2019 4:02:59 PM

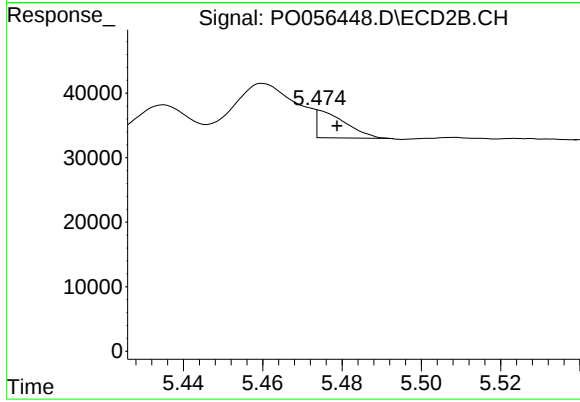

#25 AR-1248-5

R.T.: 5.474 min
Delta R.T.: -0.005 min
Response: 20599
Conc: 13.45 ng/ml m