

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052121\
 Data File : P0078063.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 May 2021 8:59
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 12:54:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.341	0.000	18519	0	0.251	N.D. #
2)	SA Decachlor...	9.954	8.812	31931	22684	0.646	0.780
Target Compounds							
20)	L4 AR-1242-5	6.599	5.732f	9129	24594	6.822	29.992 #
24)	L5 AR-1248-4	6.543f	0.000	74067	0	31.820	N.D. #
25)	L5 AR-1248-5	6.599	5.732f	9129	24594	4.035	23.471 #
26)	L6 AR-1254-1	6.543	5.732f	74067	24594	29.842	14.261 #
28)	L6 AR-1254-3	7.149	0.000	49099	0	12.515	N.D. #
29)	L6 AR-1254-4	7.428	0.000	26962	0	9.928	N.D. #
35)	L7 AR-1260-5	8.469	0.000	202640	0	39.456	N.D. #
37)	L8 AR-1262-2	8.469	0.000	202640	0	33.664	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052121\
Data File : P0078063.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 May 2021 8:59
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 12:54:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

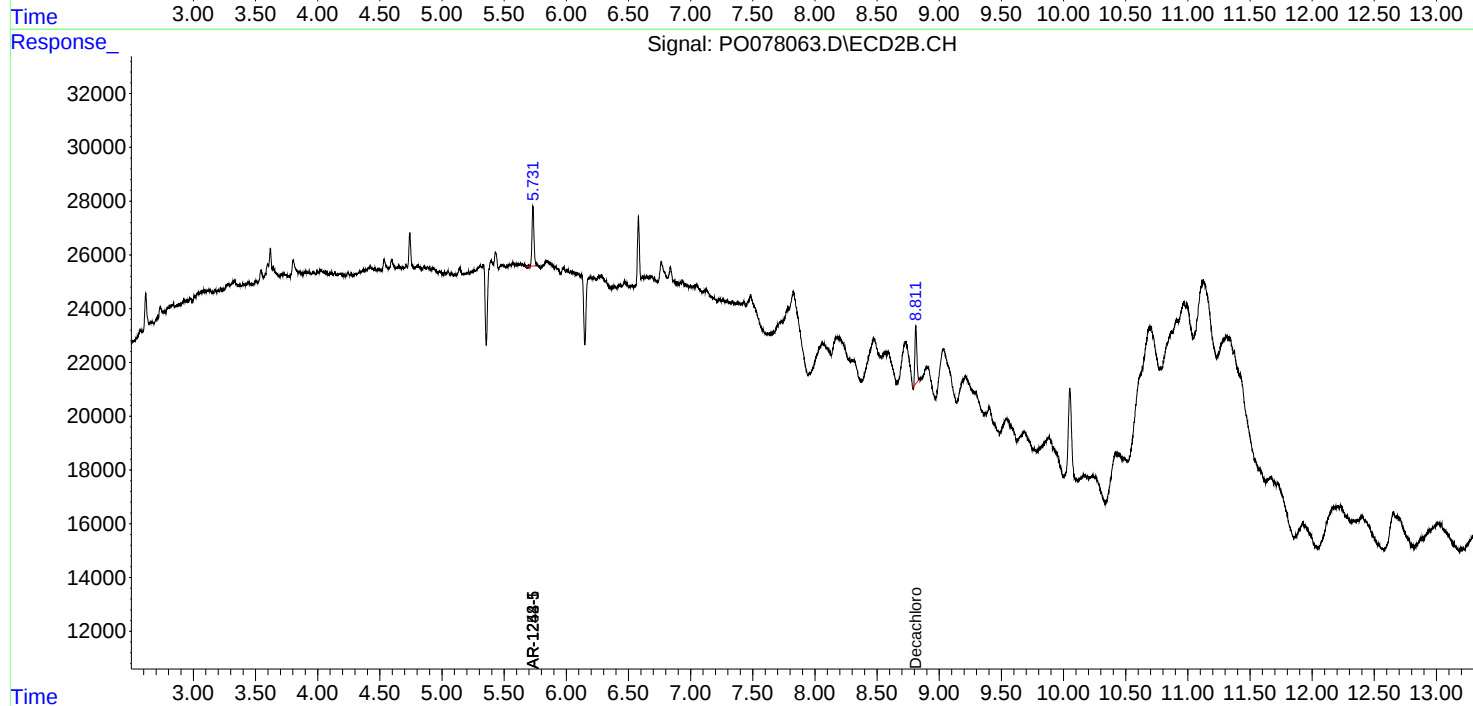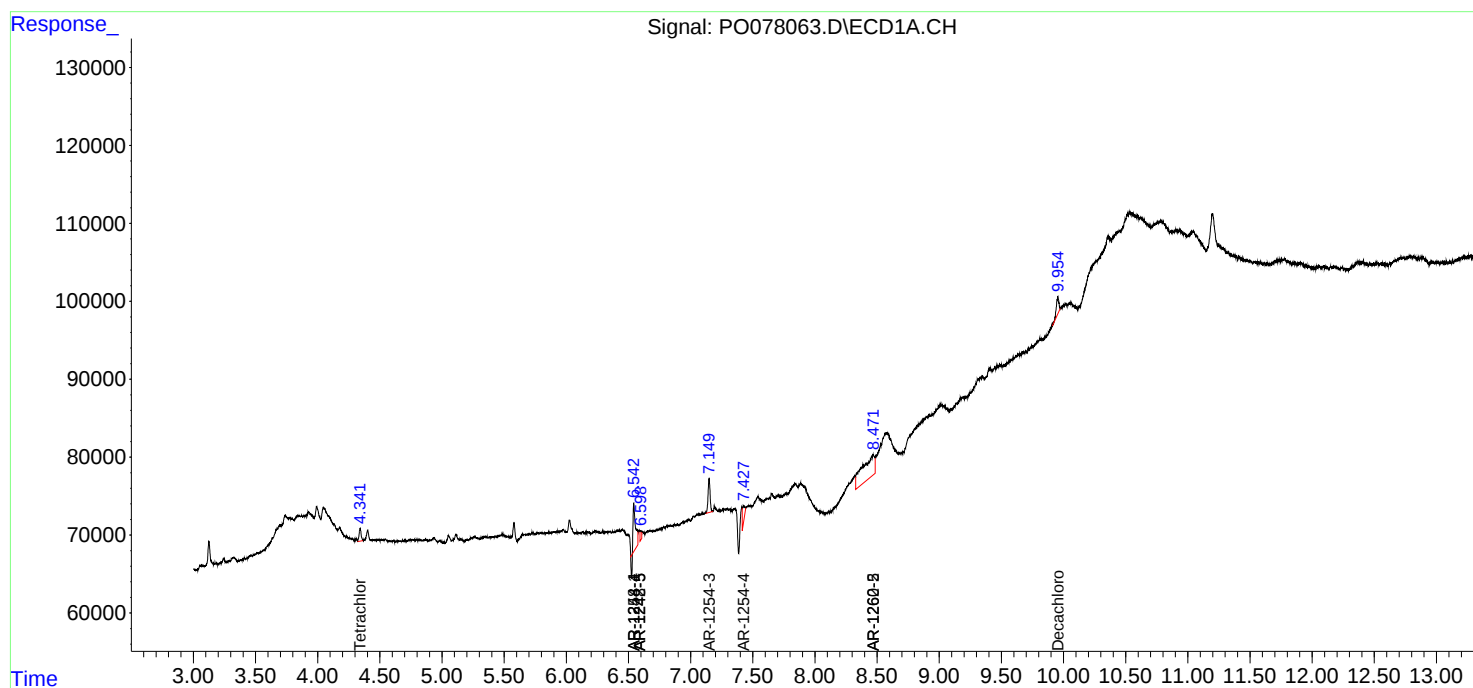


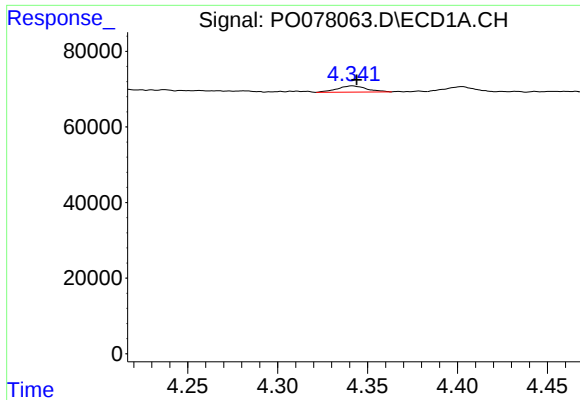

#1 Tetrachloro-m-xylene


R.T.: 4.341 min
Delta R.T.: -0.003 min
Response: 18519
Conc: 0.25 ng/ml

Instrument :
ECD_O
ClientSampleId :

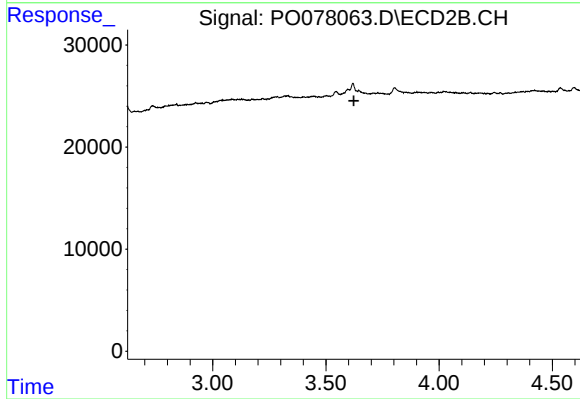


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.624 min
Response: 0
Conc: N.D.

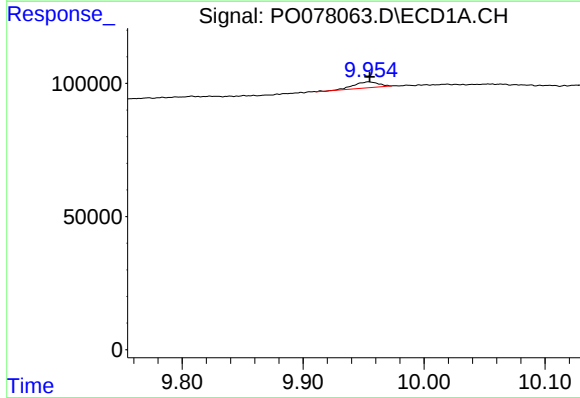


#2 Decachlorobiphenyl

R.T.: 9.954 min
Delta R.T.: 0.000 min
Response: 31931
Conc: 0.65 ng/ml

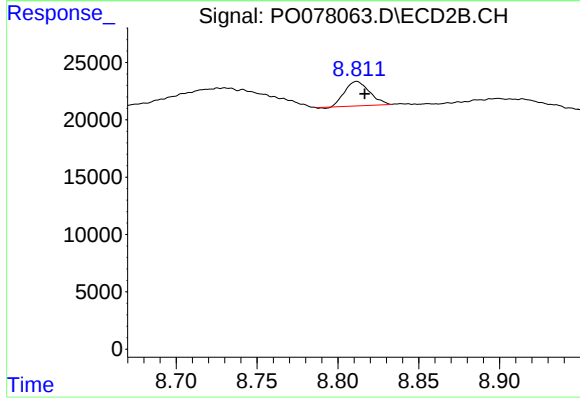

#2 Decachlorobiphenyl


R.T.: 8.812 min
Delta R.T.: -0.005 min
Response: 22684
Conc: 0.78 ng/ml

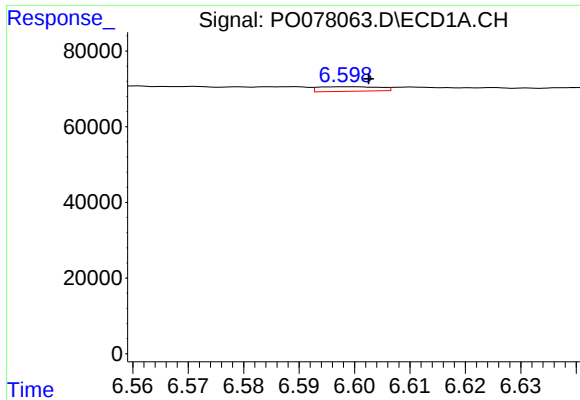

#20 AR-1242-5


R.T.: 6.599 min
Delta R.T.: -0.004 min
Response: 9129
Conc: 6.82 ng/ml

Instrument :
ECD_O
ClientSampleId :

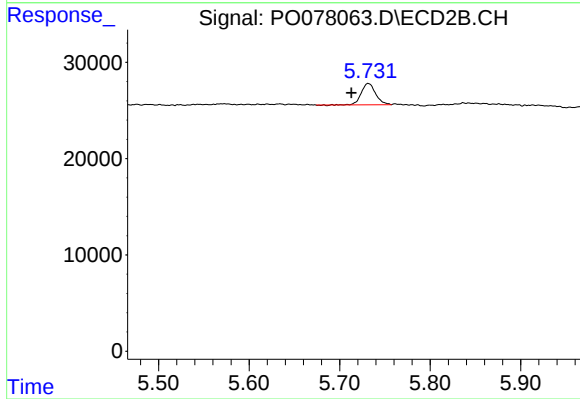


#20 AR-1242-5

R.T.: 5.732 min
Delta R.T.: 0.018 min
Response: 24594
Conc: 29.99 ng/ml

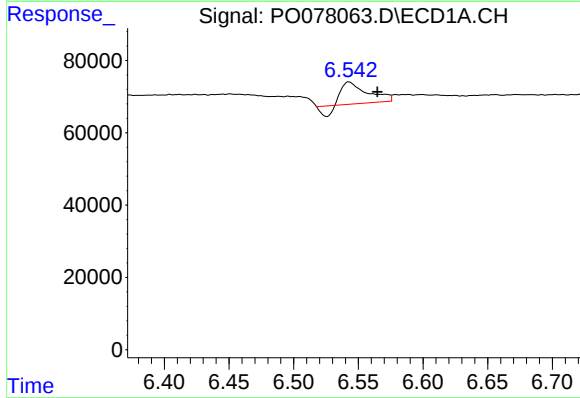


#24 AR-1248-4

R.T.: 6.543 min
Delta R.T.: -0.022 min
Response: 74067
Conc: 31.82 ng/ml

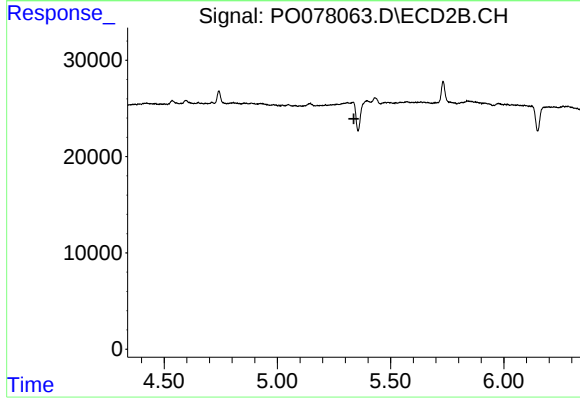

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.338 min
Response: 0
Conc: N.D.

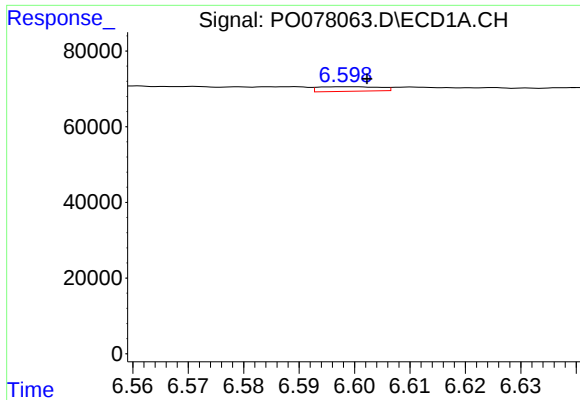

#25 AR-1248-5


R.T.: 6.599 min
Delta R.T.: -0.004 min
Response: 9129
Conc: 4.03 ng/ml

Instrument :
ECD_O
ClientSampleId :

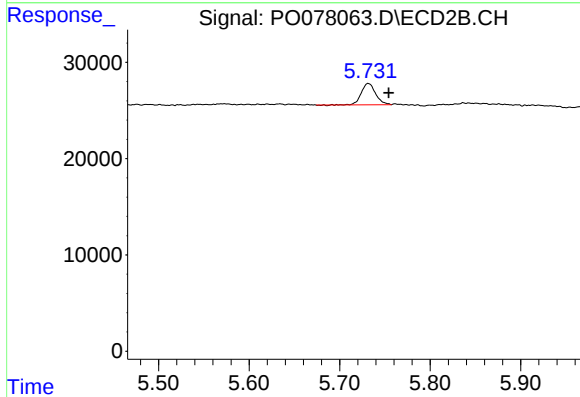


#25 AR-1248-5

R.T.: 5.732 min
Delta R.T.: -0.023 min
Response: 24594
Conc: 23.47 ng/ml

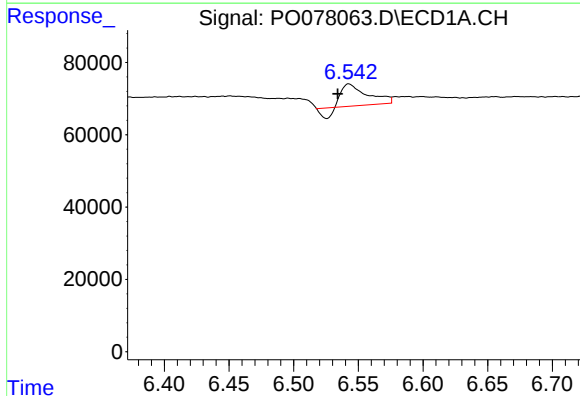


#26 AR-1254-1

R.T.: 6.543 min
Delta R.T.: 0.009 min
Response: 74067
Conc: 29.84 ng/ml

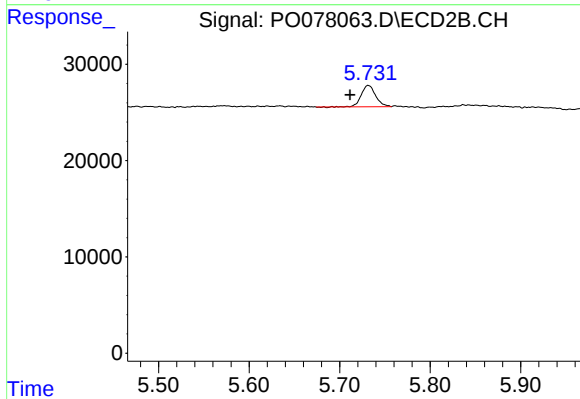

#26 AR-1254-1


R.T.: 5.732 min
Delta R.T.: 0.020 min
Response: 24594
Conc: 14.26 ng/ml

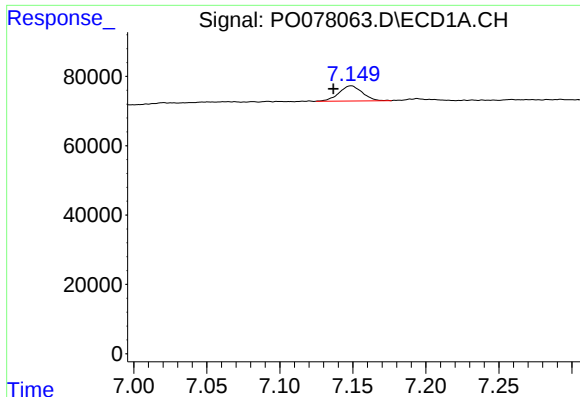

#28 AR-1254-3


R.T.: 7.149 min
Delta R.T.: 0.012 min
Response: 49099
Conc: 12.51 ng/ml

Instrument :
ECD_O
ClientSampleId :

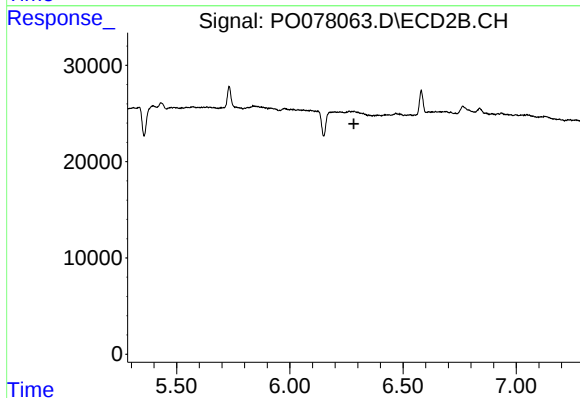


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.283 min
Response: 0
Conc: N.D.

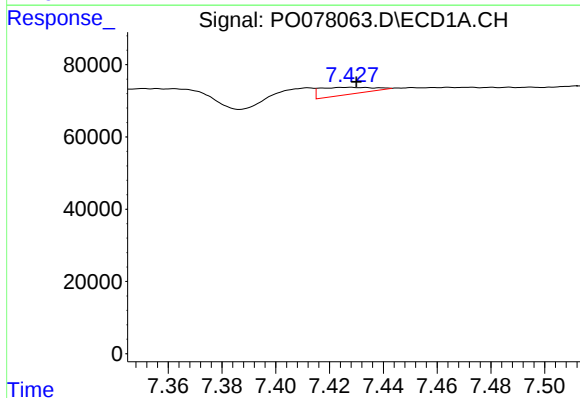


#29 AR-1254-4

R.T.: 7.428 min
Delta R.T.: -0.002 min
Response: 26962
Conc: 9.93 ng/ml

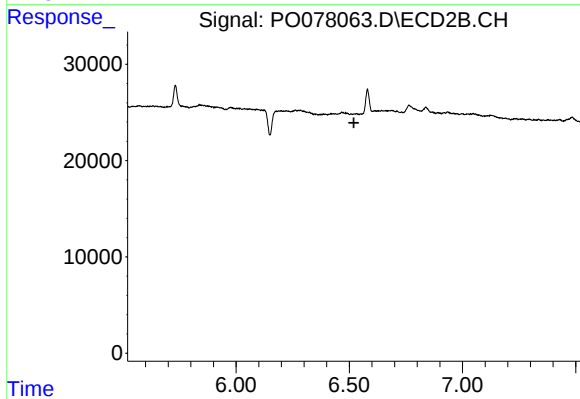

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.521 min
Response: 0
Conc: N.D.

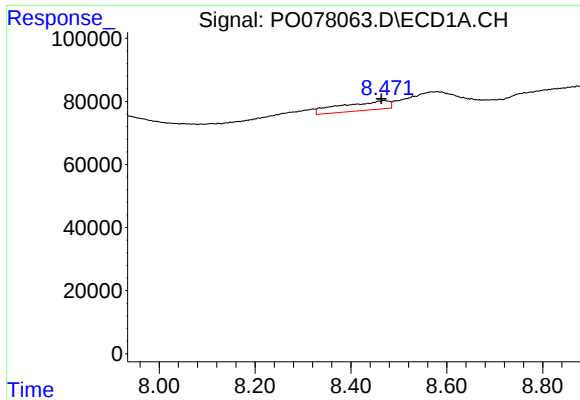

#35 AR-1260-5


R.T.: 8.469 min
Delta R.T.: 0.006 min
Response: 202640
Conc: 39.46 ng/ml

Instrument :
ECD_O
ClientSampleId :

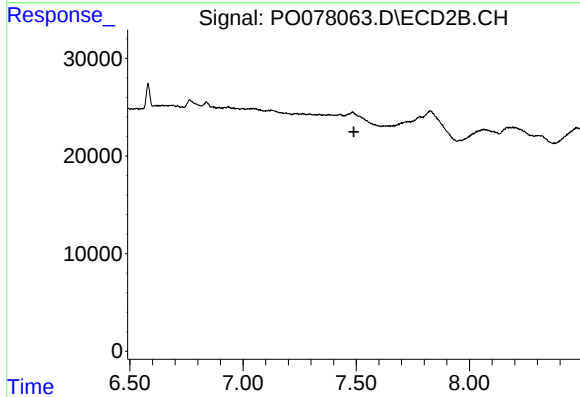


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.489 min
Response: 0
Conc: N.D.

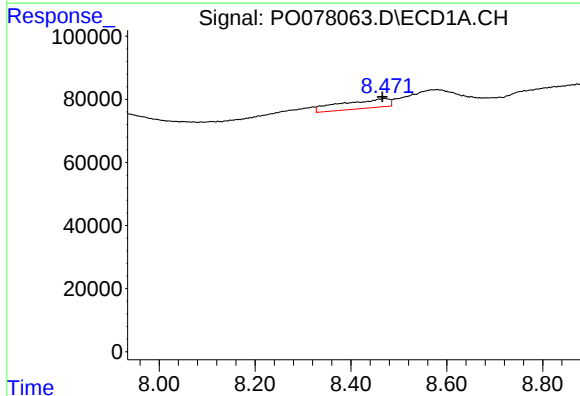

#37 AR-1262-2

R.T.: 8.469 min
Delta R.T.: 0.004 min
Response: 202640
Conc: 33.66 ng/ml

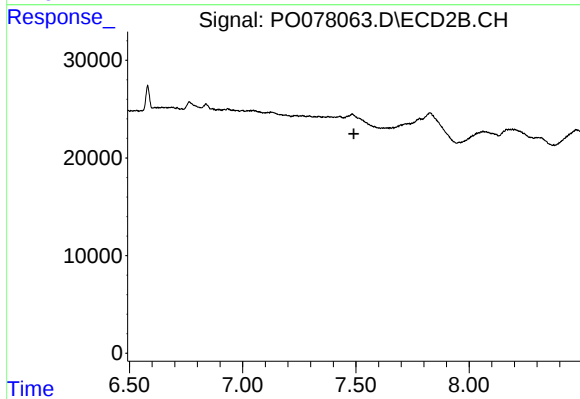

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.491 min
Response: 0
Conc: N.D.