

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052121\
 Data File : P0078096.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 May 2021 23:19
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 03:30:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.343	3.622	1422895	634855	19.252	21.010
2)	SA Decachlor...	9.952	8.810	975714	592668	19.735	20.382
Target Compounds							
24)	L5 AR-1248-4	6.545f	0.000	2381	0	1.023	N.D. #
26)	L6 AR-1254-1	6.545	0.000	2381	0	0.959	N.D. #
28)	L6 AR-1254-3	7.147	0.000	28141	0	7.173	N.D. #
38)	L8 AR-1262-3	8.752	0.000	11101	0	2.749	N.D. #
39)	L8 AR-1262-4	8.814	0.000	8574	0	2.749	N.D. #
41)	L9 AR-1268-1	8.752f	0.000	11101	0	1.566	N.D. #
42)	L9 AR-1268-2	8.814	0.000	8574	0	1.325	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO052121\
Data File : PO078096.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 May 2021 23:19
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 03:30:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

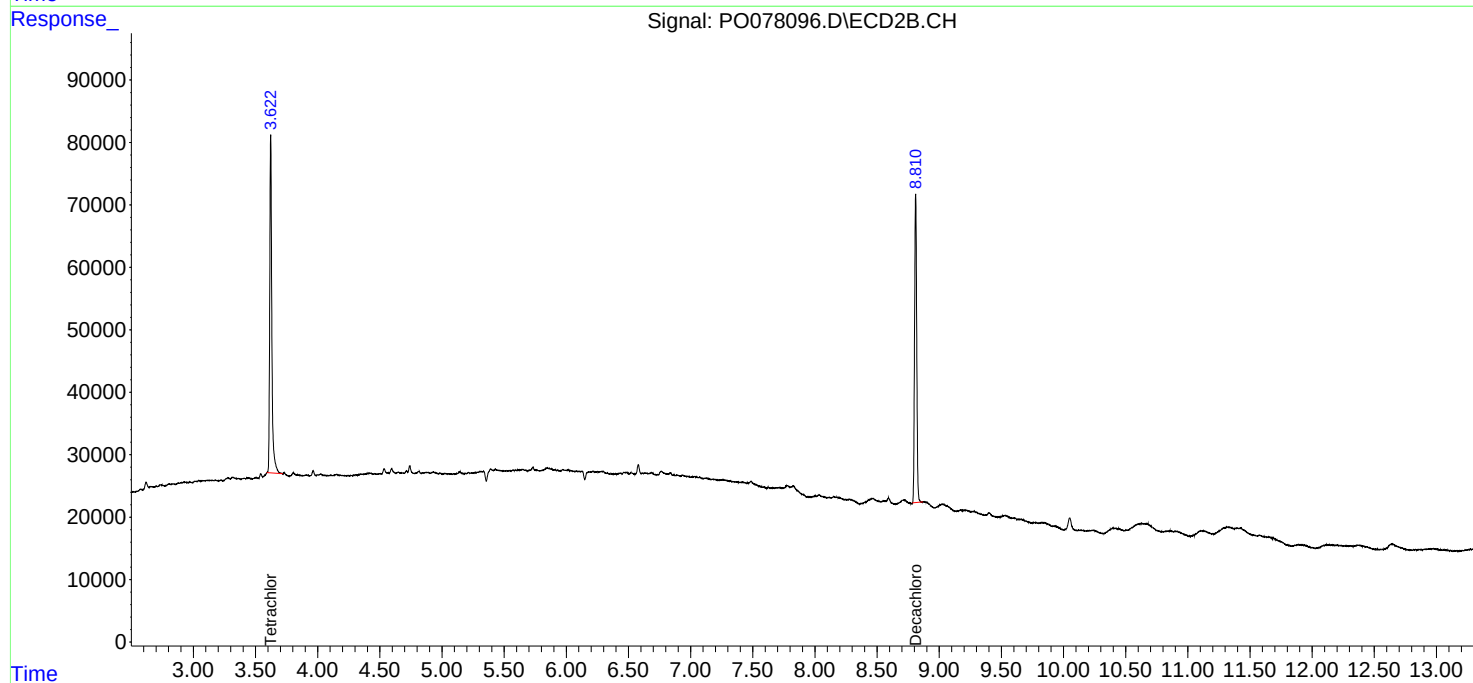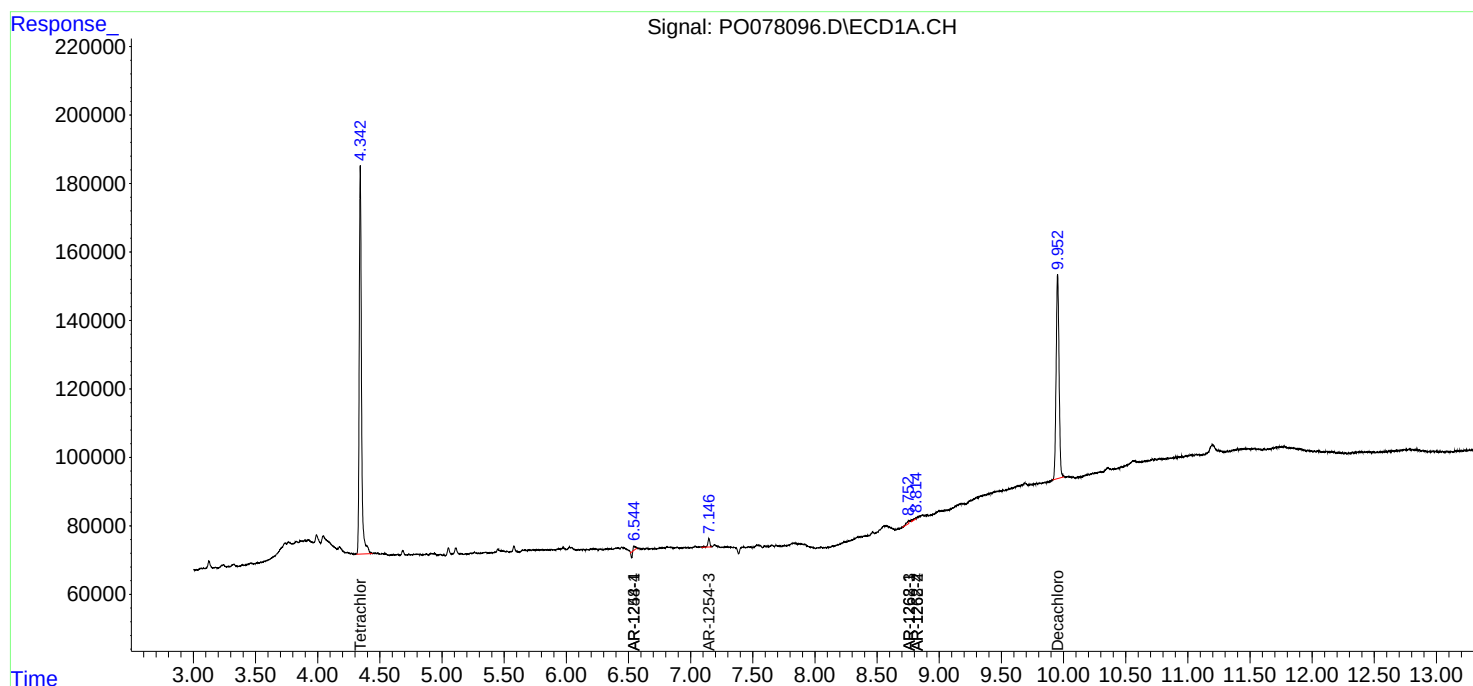


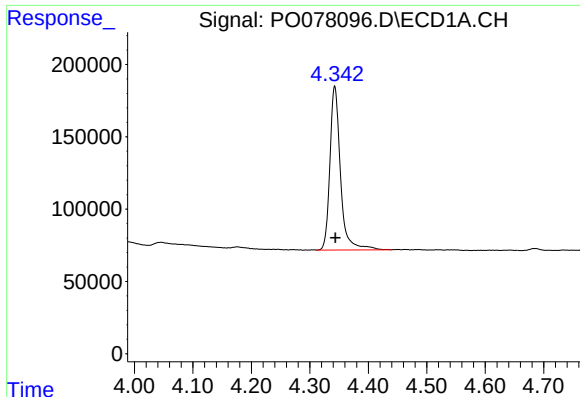

#1 Tetrachloro-m-xylene


R.T.: 4.343 min
Delta R.T.: -0.001 min
Response: 1422895
Conc: 19.25 ng/ml

Instrument :
ECD_O
ClientSampleId :

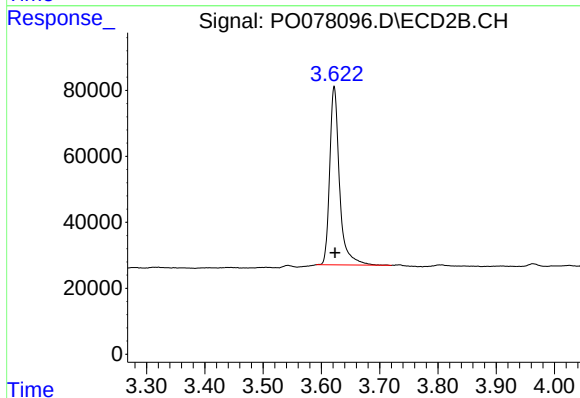


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.002 min
Response: 634855
Conc: 21.01 ng/ml

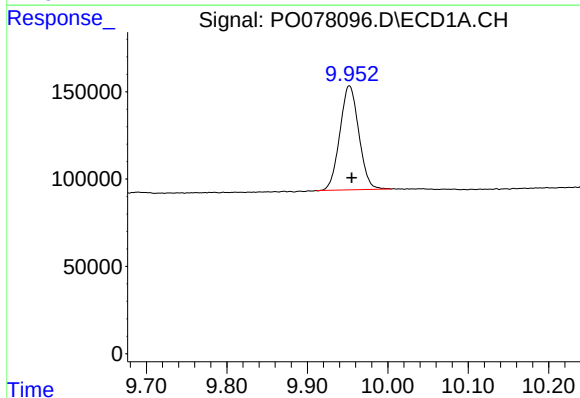


#2 Decachlorobiphenyl

R.T.: 9.952 min
Delta R.T.: -0.003 min
Response: 975714
Conc: 19.74 ng/ml

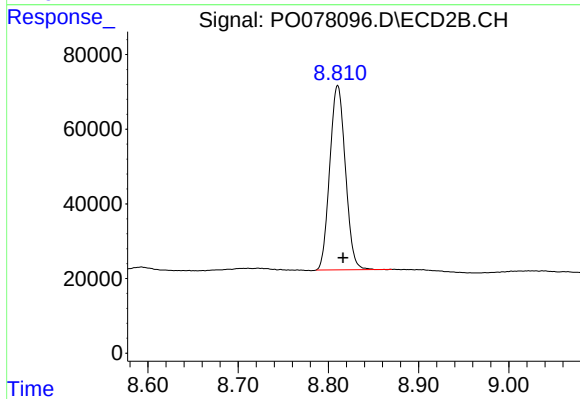

#2 Decachlorobiphenyl


R.T.: 8.810 min
Delta R.T.: -0.006 min
Response: 592668
Conc: 20.38 ng/ml

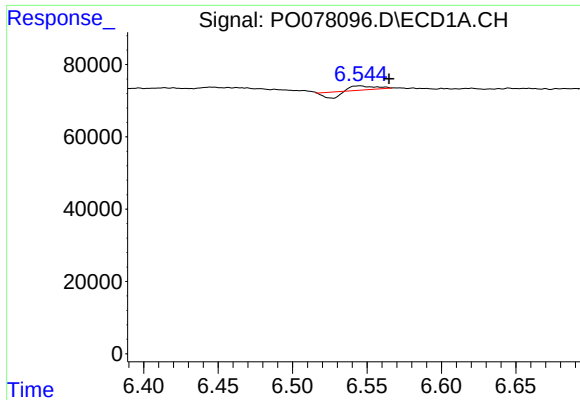

#24 AR-1248-4


R.T.: 6.545 min
Delta R.T.: -0.020 min
Response: 2381
Conc: 1.02 ng/ml

Instrument :
ECD_O
ClientSampleId :

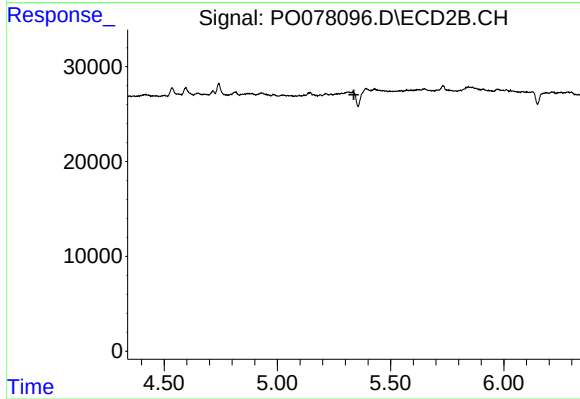


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.338 min
Response: 0
Conc: N.D.

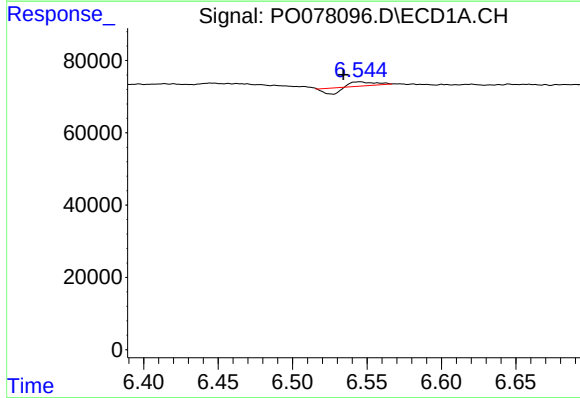


#26 AR-1254-1

R.T.: 6.545 min
Delta R.T.: 0.011 min
Response: 2381
Conc: 0.96 ng/ml

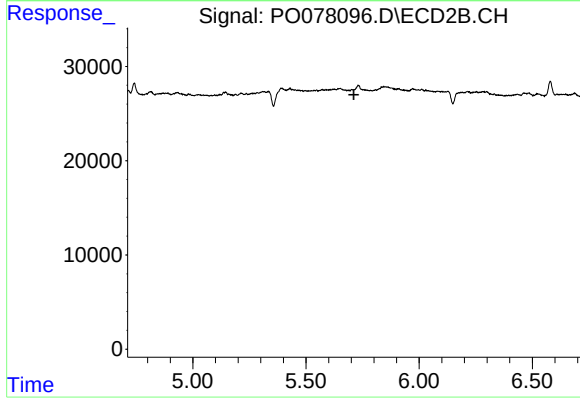

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.712 min
Response: 0
Conc: N.D.

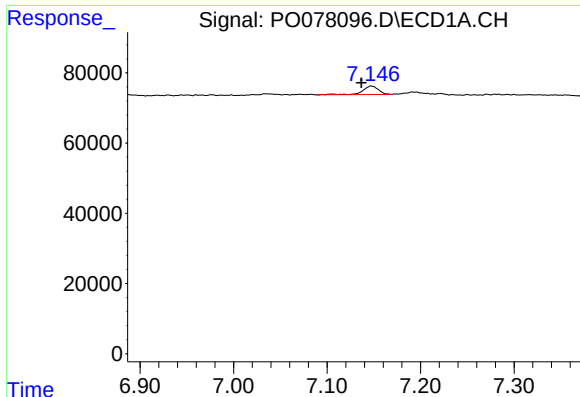

#28 AR-1254-3


R.T.: 7.147 min
Delta R.T.: 0.010 min
Response: 28141
Conc: 7.17 ng/ml

Instrument :
ECD_O
ClientSampleId :

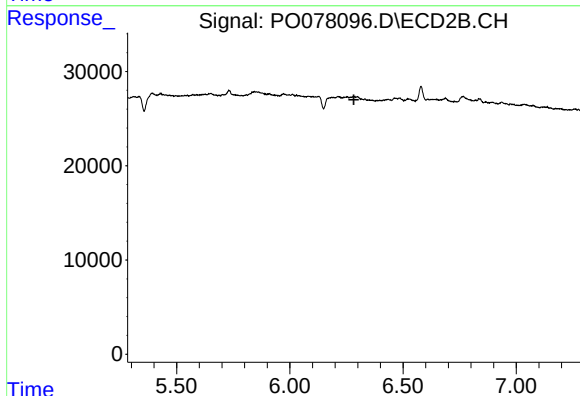


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.283 min
Response: 0
Conc: N.D.

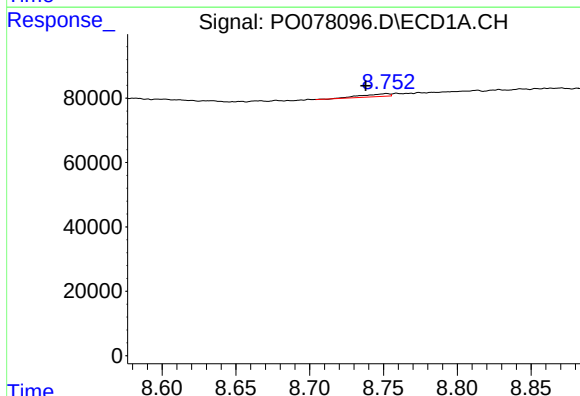


#38 AR-1262-3

R.T.: 8.752 min
Delta R.T.: 0.014 min
Response: 11101
Conc: 2.75 ng/ml

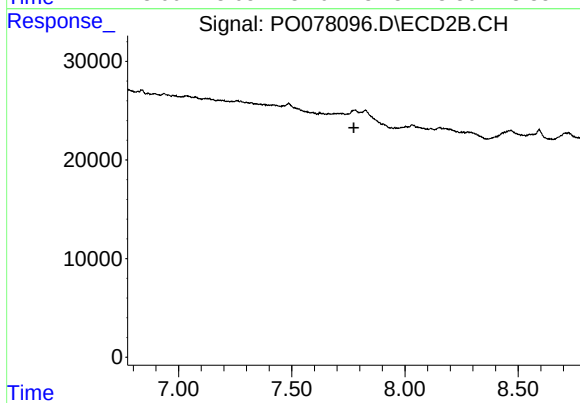

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 7.774 min
Response: 0
Conc: N.D.

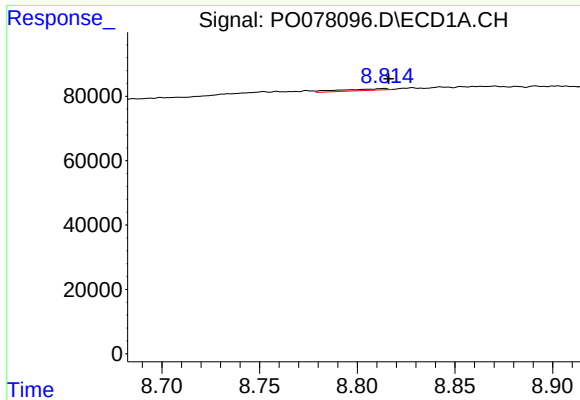

#39 AR-1262-4


R.T.: 8.814 min
Delta R.T.: -0.002 min
Response: 8574
Conc: 2.75 ng/ml

Instrument :
ECD_O
ClientSampleId :

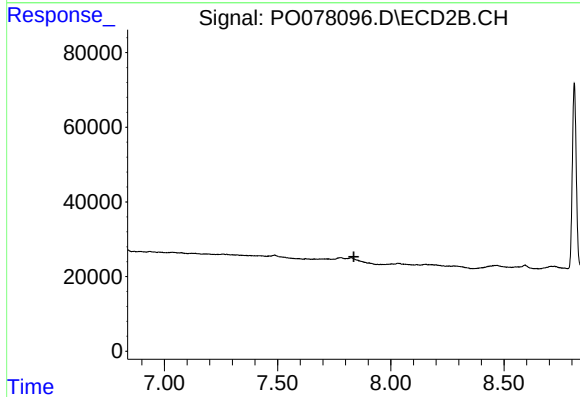


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.837 min
Response: 0
Conc: N.D.

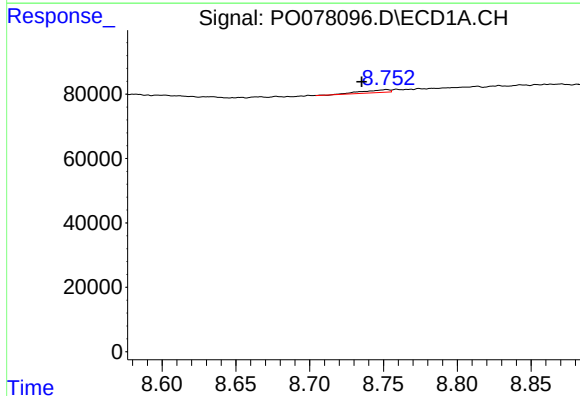


#41 AR-1268-1

R.T.: 8.752 min
Delta R.T.: 0.017 min
Response: 11101
Conc: 1.57 ng/ml

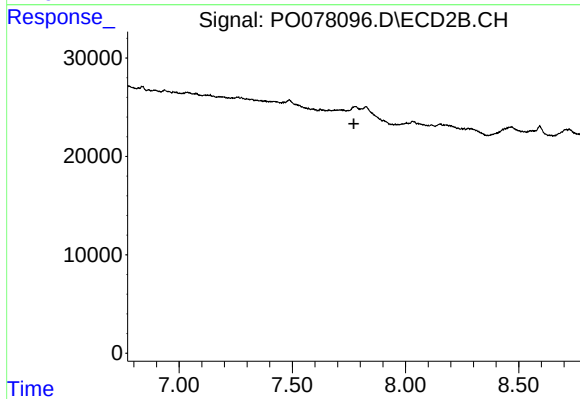

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 7.772 min
Response: 0
Conc: N.D.

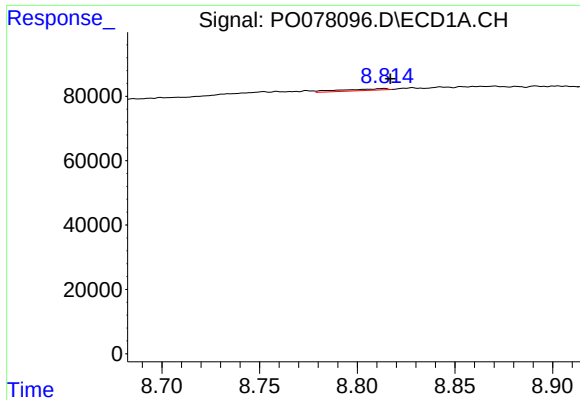

#42 AR-1268-2

R.T.: 8.814 min
Delta R.T.: -0.003 min
Response: 8574
Conc: 1.33 ng/ml

Instrument :
ECD_O
ClientSampleId :

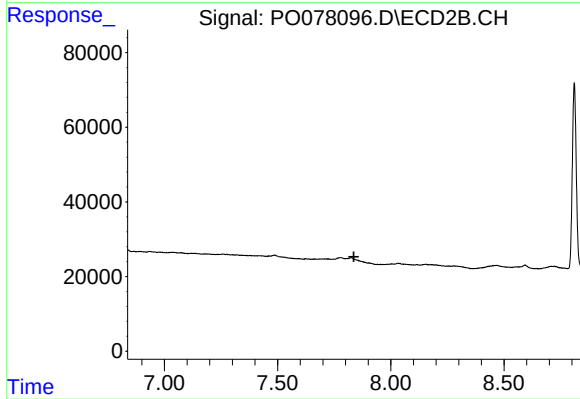

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.837 min
Response: 0
Conc: N.D.