

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052122\
Data File : P0086356.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 May 2022 3:43
Operator : YP\AJ
Sample : N2960-03
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BIN-4-SP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 13:29:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 19 09:06:34 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.479	3.675	2392948	995076	23.551	22.845
2)	SA Decachlor...	10.336	8.732	1015967	522688	18.711	15.019

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0052122\
Data File : P0086356.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 May 2022 3:43
Operator : YP\AJ
Sample : N2960-03
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BIN-4-SP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 13:29:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 19 09:06:34 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

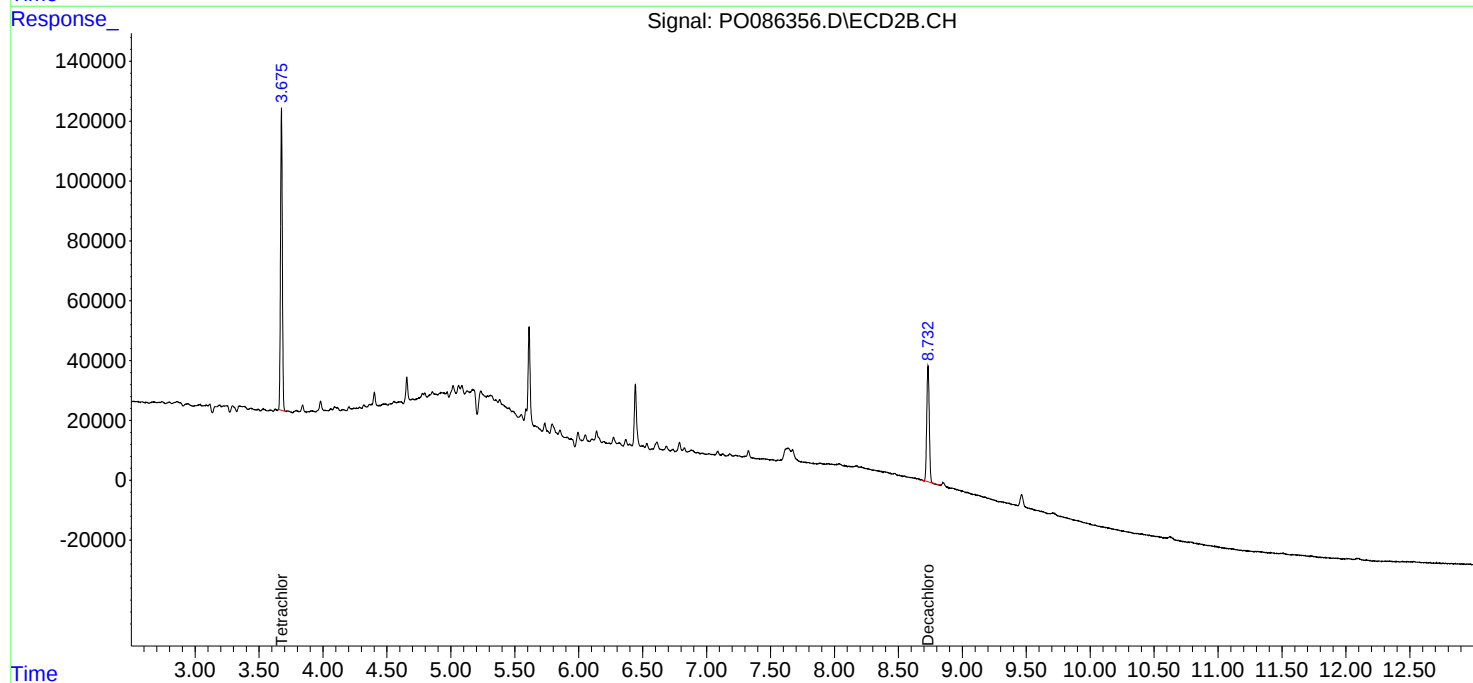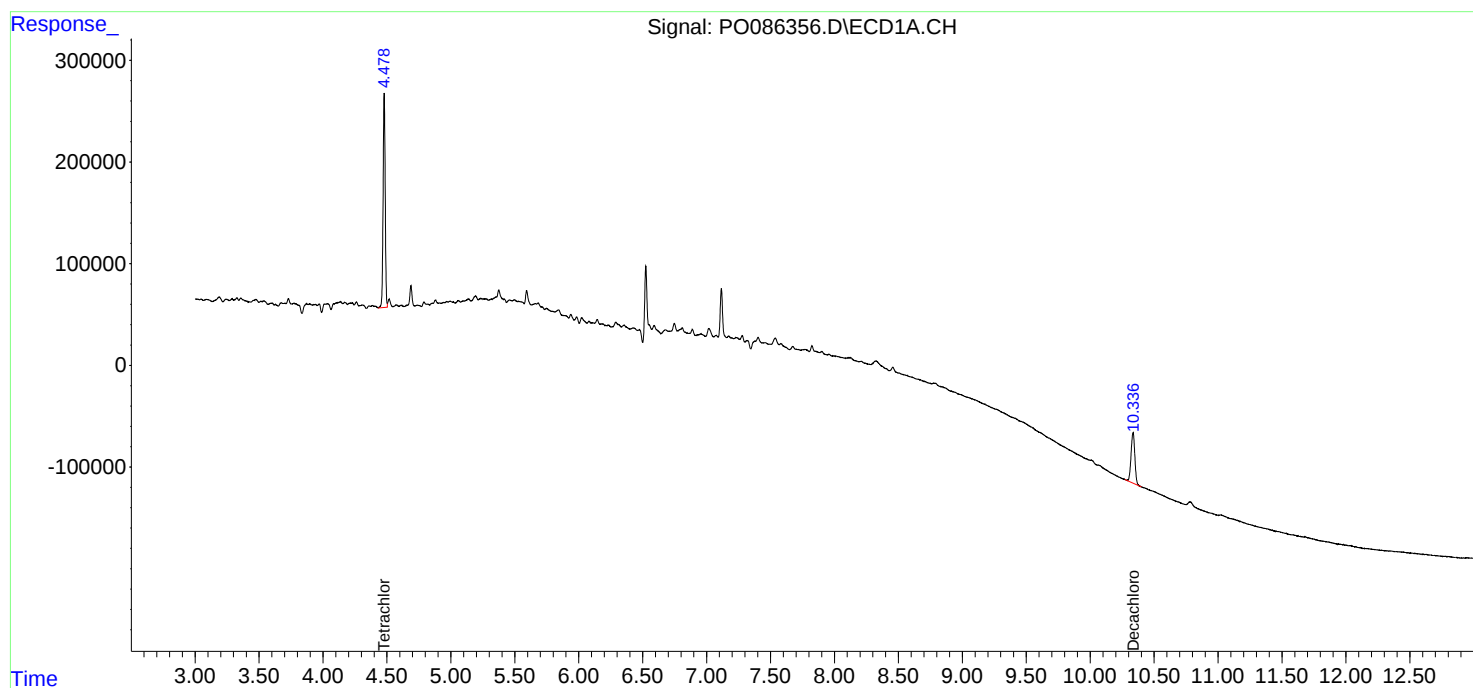


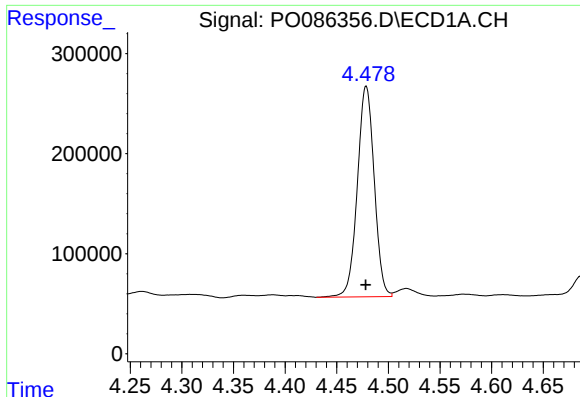

#1 Tetrachloro-m-xylene


R.T.: 4.479 min
Delta R.T.: 0.000 min
Response: 2392948
Conc: 23.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
BIN-4-SP-2

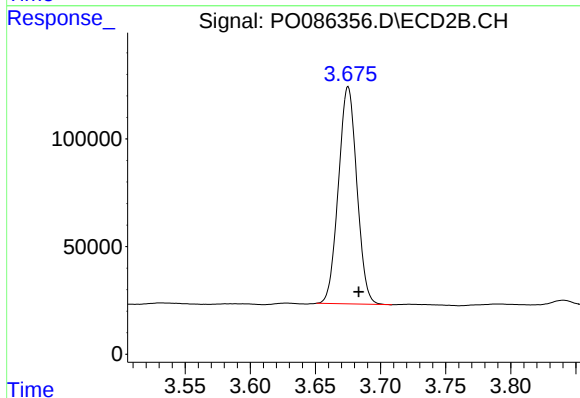


#1 Tetrachloro-m-xylene

R.T.: 3.675 min
Delta R.T.: -0.008 min
Response: 995076
Conc: 22.84 ng/ml

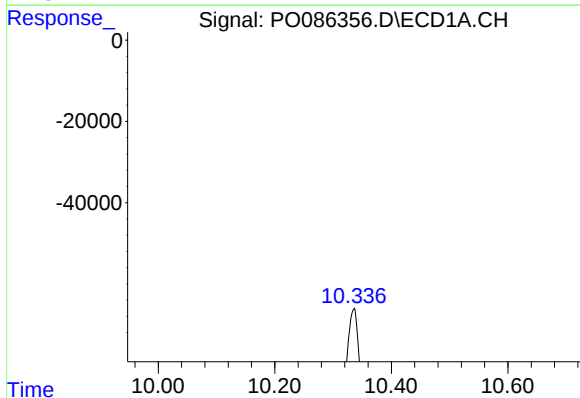

#2 Decachlorobiphenyl

R.T.: 10.336 min
Delta R.T.: 0.011 min
Response: 1015967
Conc: 18.71 ng/ml

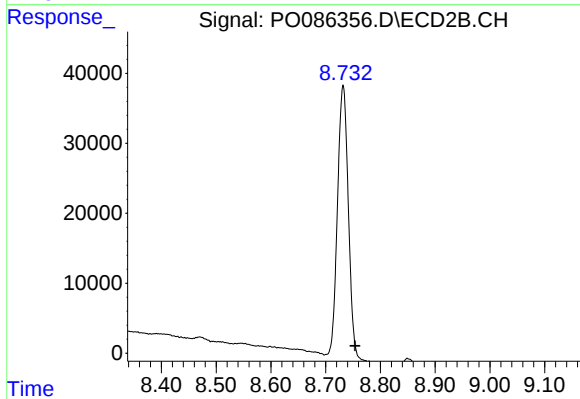

#2 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: -0.022 min
Response: 522688
Conc: 15.02 ng/ml