

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052122\
Data File : P0086376.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 May 2022 10:12
Operator : YP\AJ
Sample : N2982-02
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
P-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 13:36:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 19 09:06:34 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.479	3.675	2452291	1000392	24.135	22.967
2) SA Decachlor...	10.330	8.729	1091711	589304	20.106	16.934

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052122\
Data File : P0086376.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 May 2022 10:12
Operator : YP\AJ
Sample : N2982-02
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
P-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 13:36:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 19 09:06:34 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

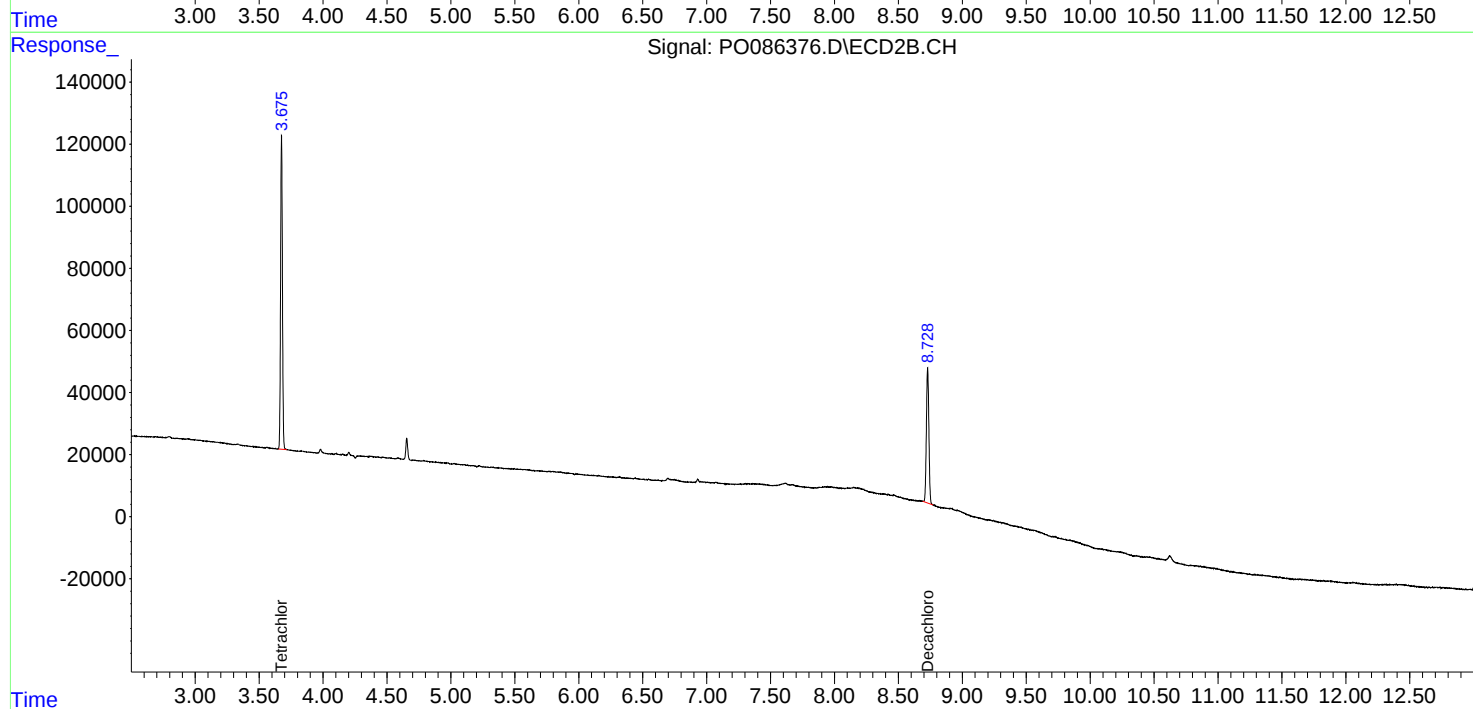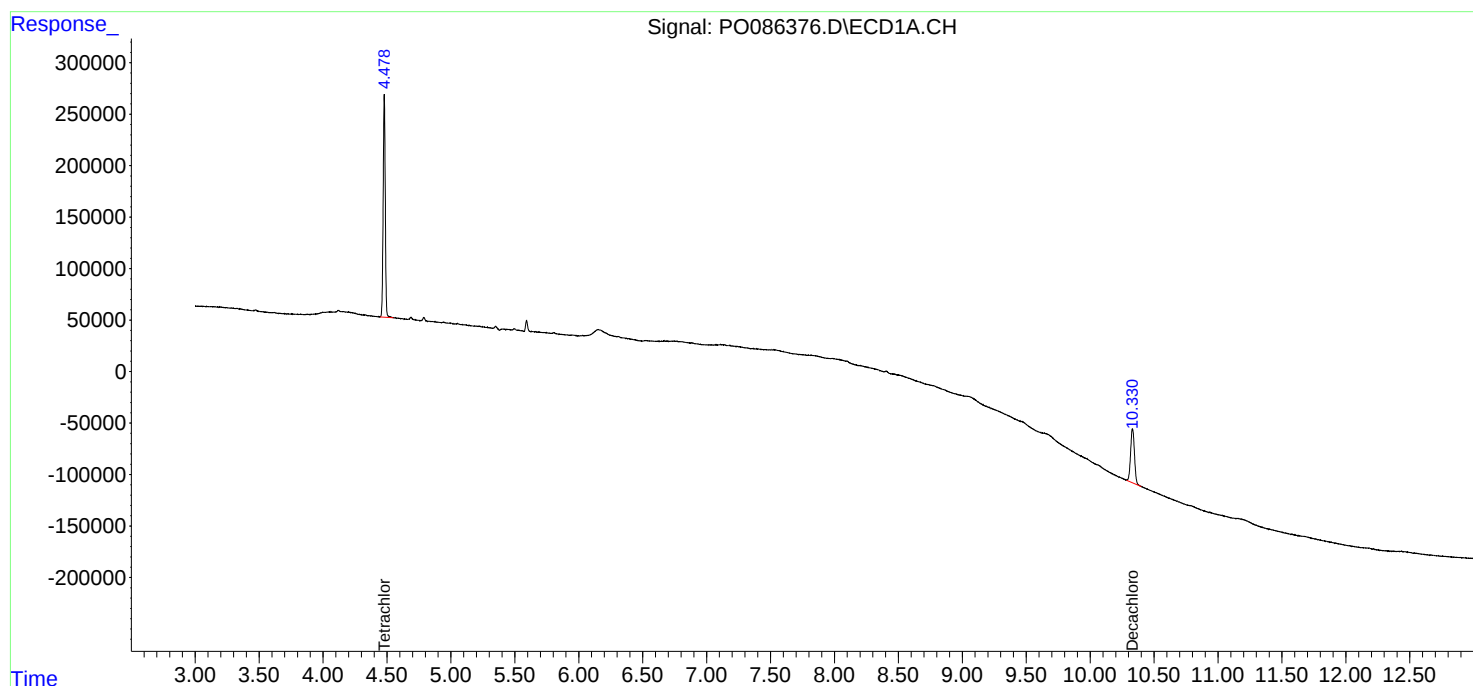


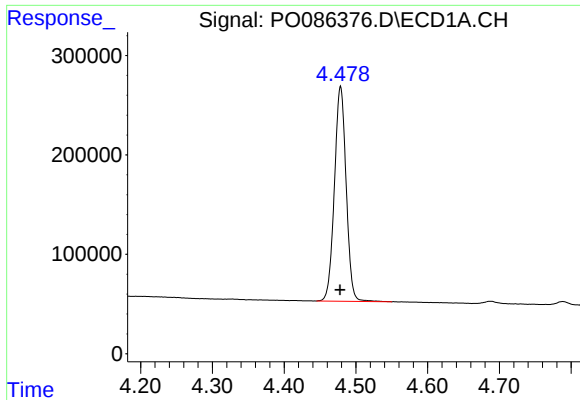

#1 Tetrachloro-m-xylene


R.T.: 4.479 min
Delta R.T.: 0.000 min
Response: 2452291
Conc: 24.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
P-2

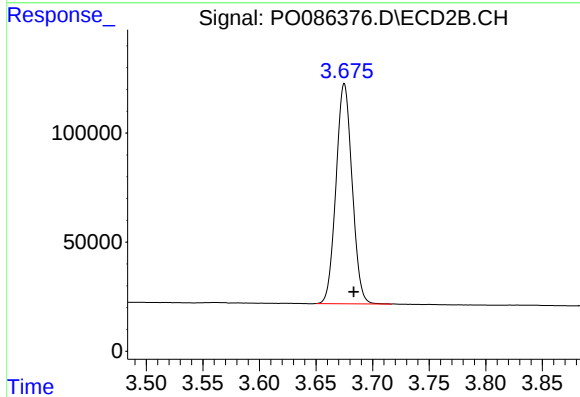


#1 Tetrachloro-m-xylene

R.T.: 3.675 min
Delta R.T.: -0.008 min
Response: 1000392
Conc: 22.97 ng/ml

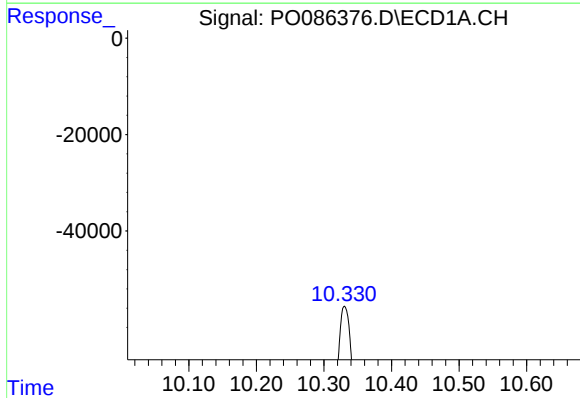

#2 Decachlorobiphenyl

R.T.: 10.330 min
Delta R.T.: 0.005 min
Response: 1091711
Conc: 20.11 ng/ml

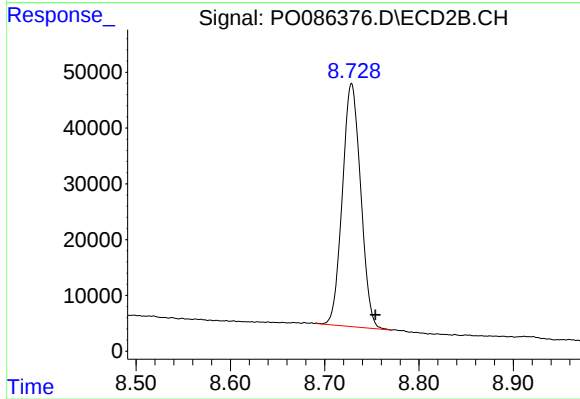

#2 Decachlorobiphenyl

R.T.: 8.729 min
Delta R.T.: -0.025 min
Response: 589304
Conc: 16.93 ng/ml