

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052322\
 Data File : P0086446.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 May 2022 00:44
 Operator : YP\AJ
 Sample : N2876-08
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 P007-SS011-2430-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/24/2022
 Supervised By :Ankita Jodhani 05/24/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 01:49:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 19 09:06:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.478	3.675	2315215	1024002	22.786	23.509
2) SA Decachlor...	10.329	8.725	1128993	618660	20.792	17.777
Target Compounds						
31) L7 AR-1260-1	7.278	6.267	540442	304466	178.575	156.432
32) L7 AR-1260-2	7.537	6.455	655384	360137	181.171	153.229
33) L7 AR-1260-3	7.899	6.610	379771	272229	137.598	126.602
34) L7 AR-1260-4	8.127	7.082	393470	191393	116.619	106.292m
35) L7 AR-1260-5	8.454	7.323	662672	409632	107.390	94.563

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052322\
Data File : P0086446.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 May 2022 00:44
Operator : YP\AJ
Sample : N2876-08
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
P007-SS011-2430-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/24/2022
Supervised By :Ankita Jodhani 05/24/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 01:49:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 19 09:06:34 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

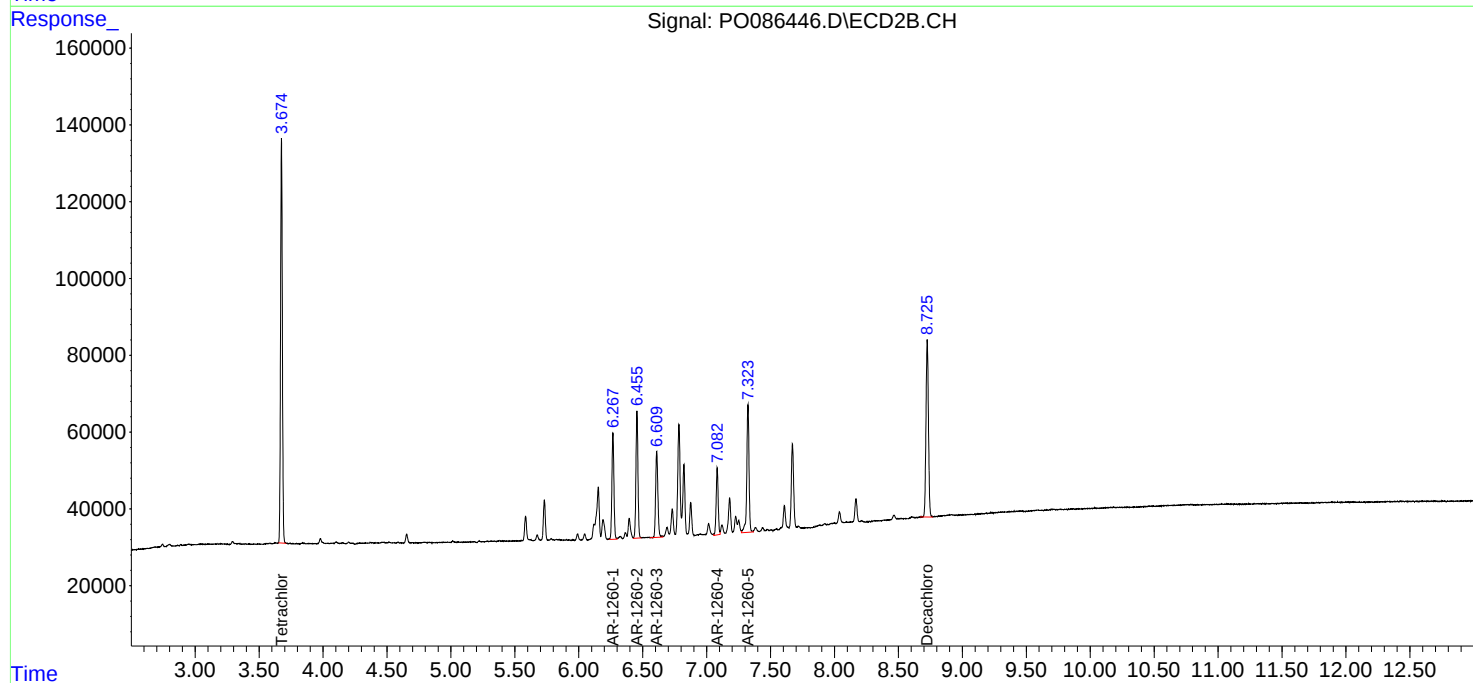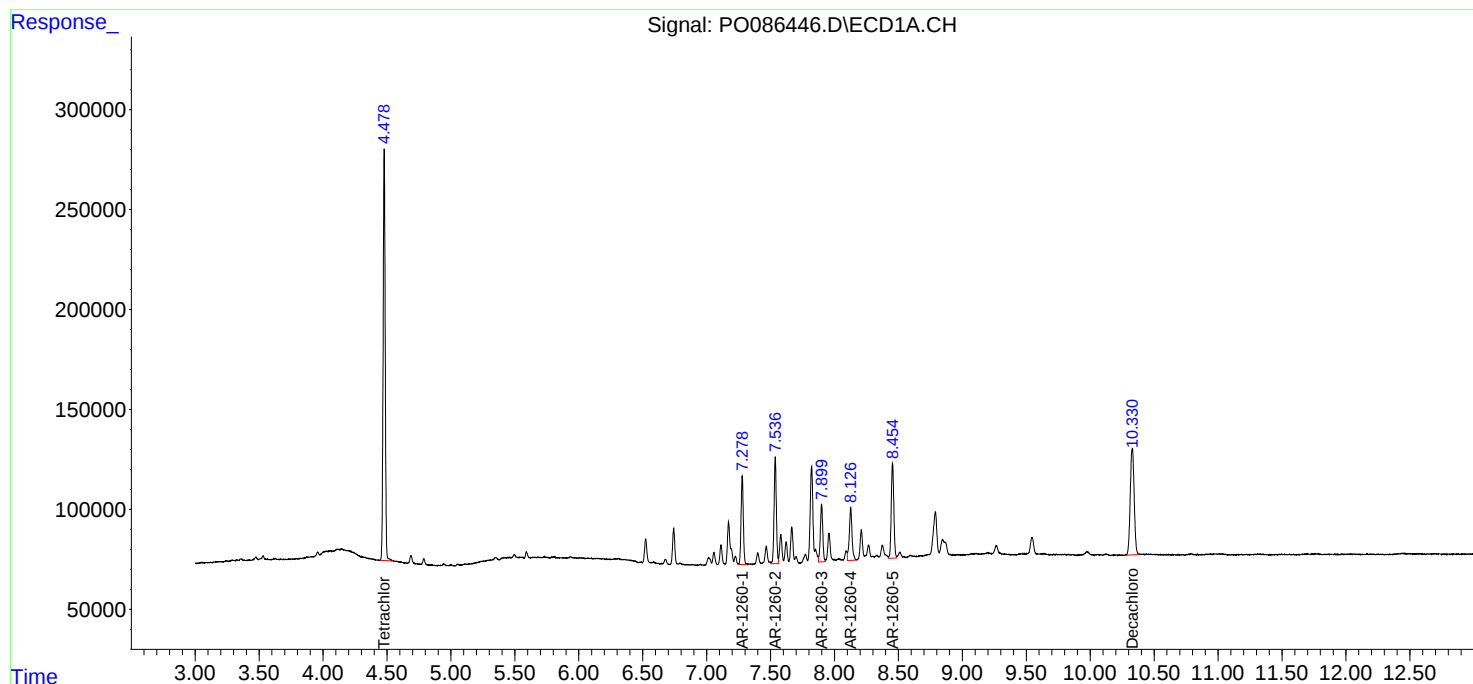

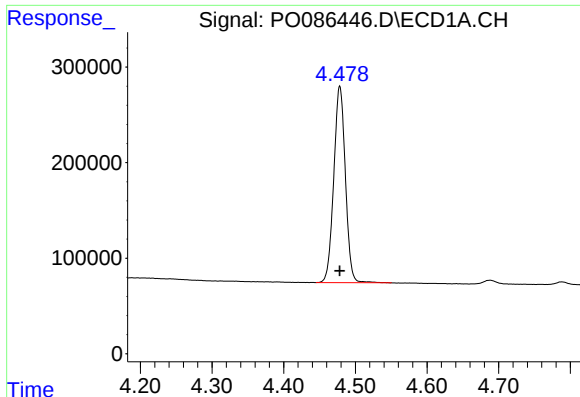


#1 Tetrachloro-m-xylene

R.T.: 4.478 min
Delta R.T.: 0.000 min
Response: 2315215
Conc: 22.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
P007-SS011-2430-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/24/2022
Supervised By :Ankita Jodhani 05/24/2022

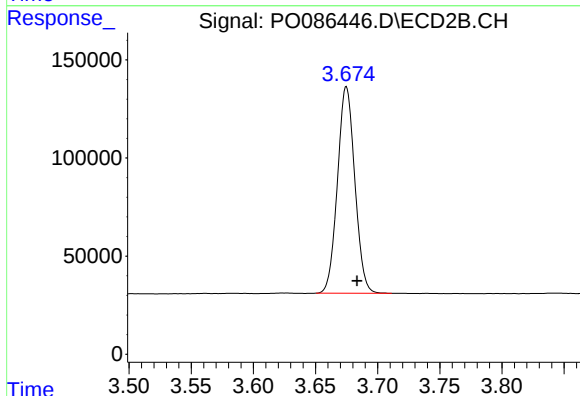


#1 Tetrachloro-m-xylene

R.T.: 3.675 min
Delta R.T.: -0.008 min
Response: 1024002
Conc: 23.51 ng/ml

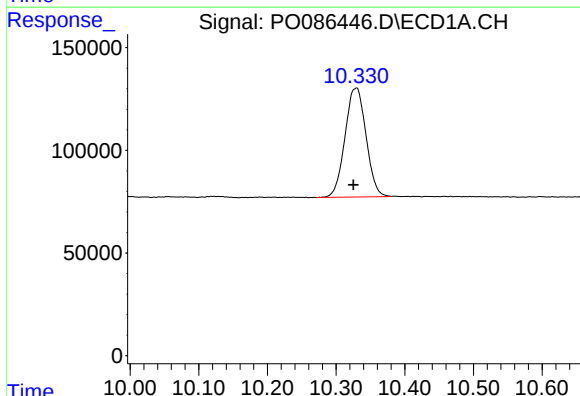


#2 Decachlorobiphenyl

R.T.: 10.329 min
Delta R.T.: 0.004 min
Response: 1128993
Conc: 20.79 ng/ml

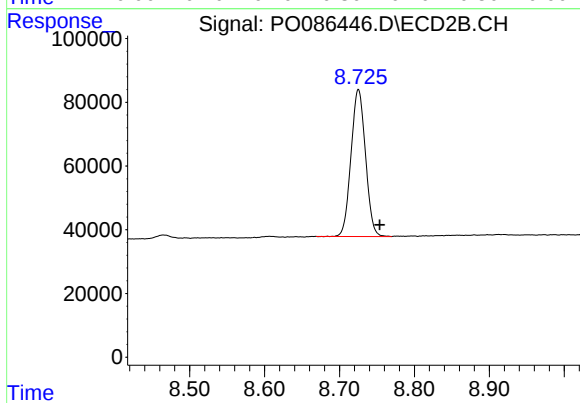

#2 Decachlorobiphenyl

R.T.: 8.725 min
Delta R.T.: -0.029 min
Response: 618660
Conc: 17.78 ng/ml

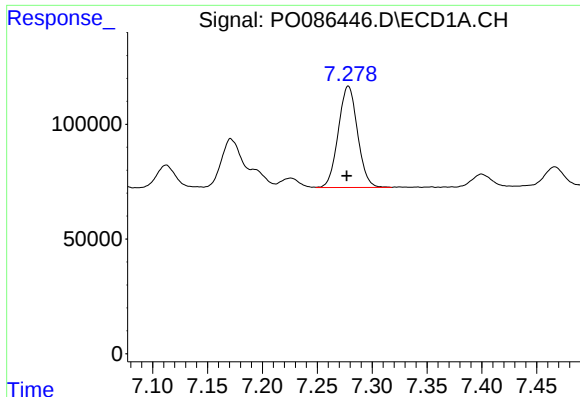


#31 AR-1260-1

R.T.: 7.278 min
Delta R.T.: 0.001 min
Response: 540442
Conc: 178.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
P007-SS011-2430-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/24/2022
Supervised By :Ankita Jodhani 05/24/2022

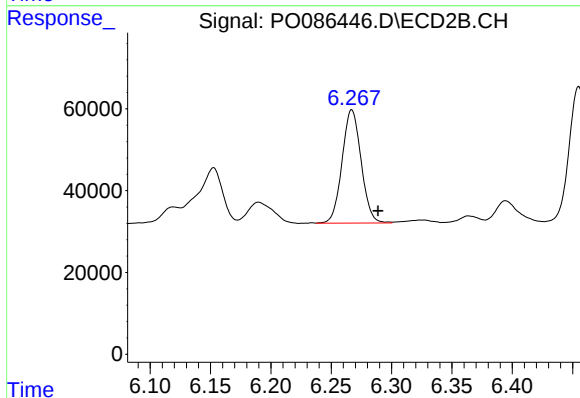


#31 AR-1260-1

R.T.: 6.267 min
Delta R.T.: -0.022 min
Response: 304466
Conc: 156.43 ng/ml

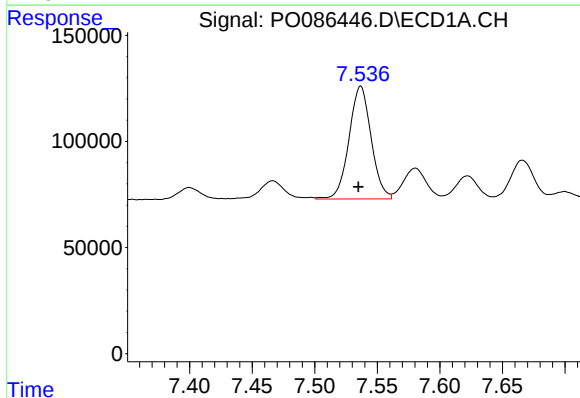


#32 AR-1260-2

R.T.: 7.537 min
Delta R.T.: 0.002 min
Response: 655384
Conc: 181.17 ng/ml

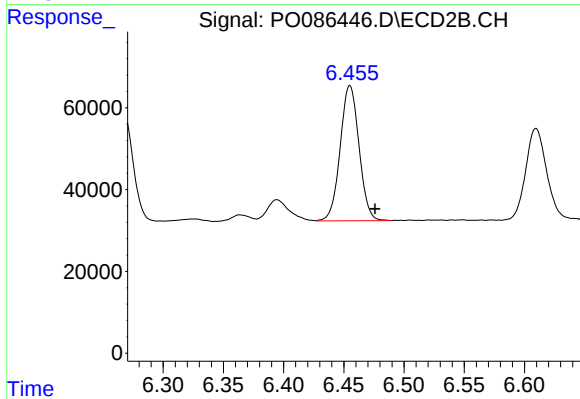

#32 AR-1260-2

R.T.: 6.455 min
Delta R.T.: -0.021 min
Response: 360137
Conc: 153.23 ng/ml

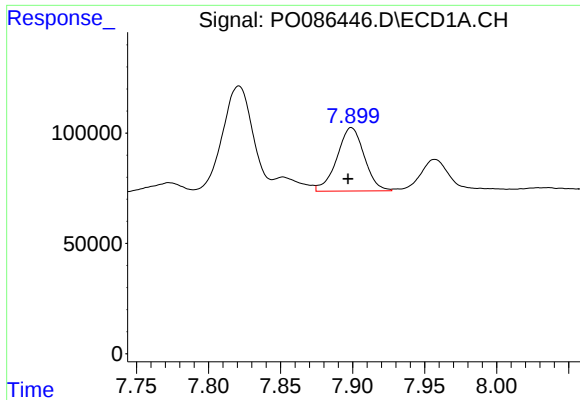


#33 AR-1260-3

R.T.: 7.899 min
Delta R.T.: 0.002 min
Response: 379771
Conc: 137.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
P007-SS011-2430-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/24/2022
Supervised By :Ankita Jodhani 05/24/2022

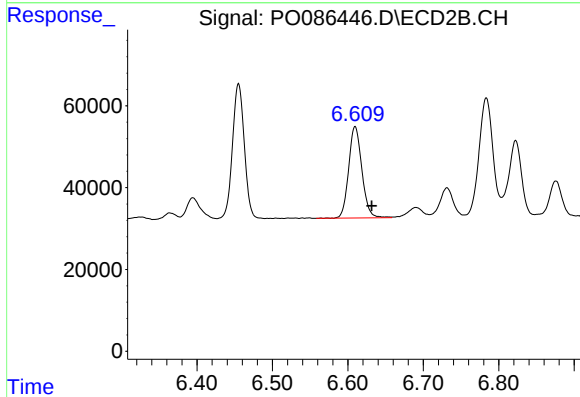


#33 AR-1260-3

R.T.: 6.610 min
Delta R.T.: -0.022 min
Response: 272229
Conc: 126.60 ng/ml

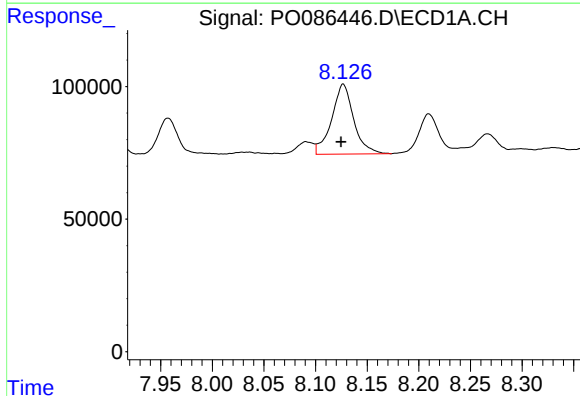


#34 AR-1260-4

R.T.: 8.127 min
Delta R.T.: 0.002 min
Response: 393470
Conc: 116.62 ng/ml

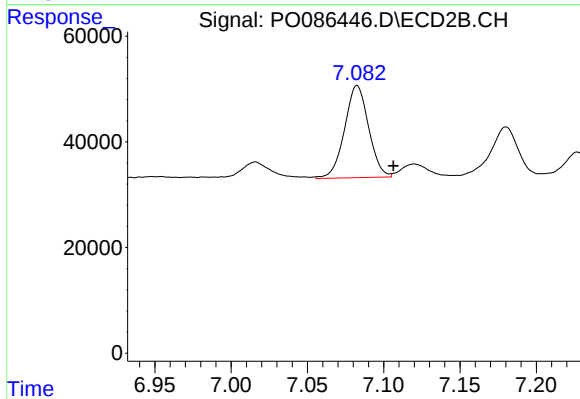

#34 AR-1260-4

R.T.: 7.082 min
Delta R.T.: -0.024 min
Response: 191393
Conc: 106.29 ng/ml m

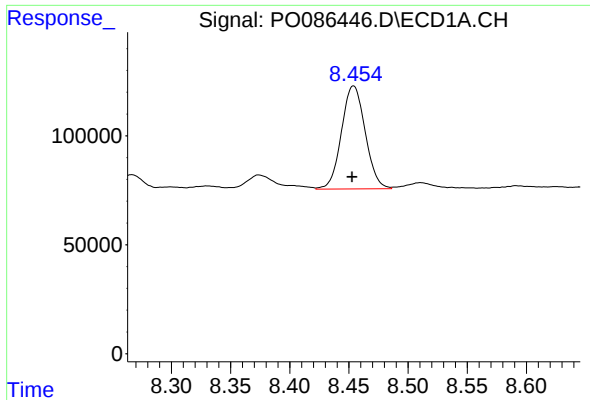


#35 AR-1260-5

R.T.: 8.454 min
Delta R.T.: 0.001 min
Response: 662672
Conc: 107.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
P007-SS011-2430-01

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/24/2022
Supervised By :Ankita Jodhani 05/24/2022

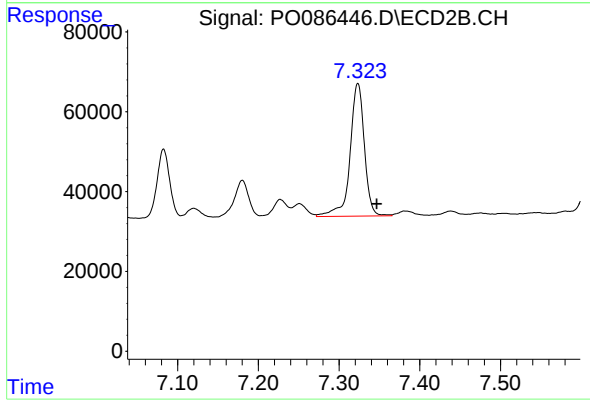

#35 AR-1260-5

R.T.: 7.323 min
Delta R.T.: -0.023 min
Response: 409632
Conc: 94.56 ng/ml