

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052323\
 Data File : P0095276.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2023 21:17
 Operator : YP/AJ
 Sample : 02894-04
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-50A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/24/2023
 Supervised By :Ankita Jodhani 05/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 01:20:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 19 06:20:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.494	3.650	61316607	26682465	21.043	23.498
2) SA Decachlor...	10.558	8.705	44675952	18172942	19.253	18.738m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO052323\
Data File : PO095276.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2023 21:17
Operator : YP/AJ
Sample : 02894-04
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-50A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/24/2023
Supervised By :Ankita Jodhani 05/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 01:20:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051823.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 19 06:20:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

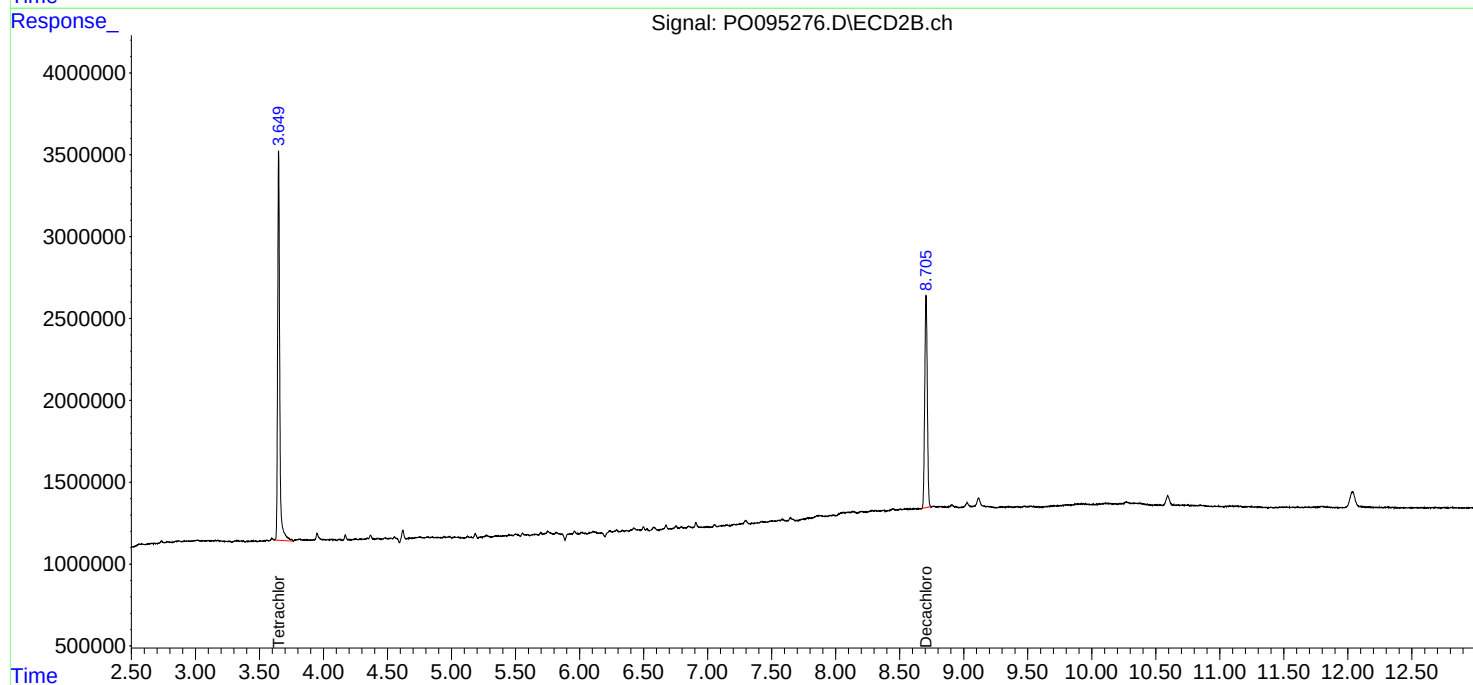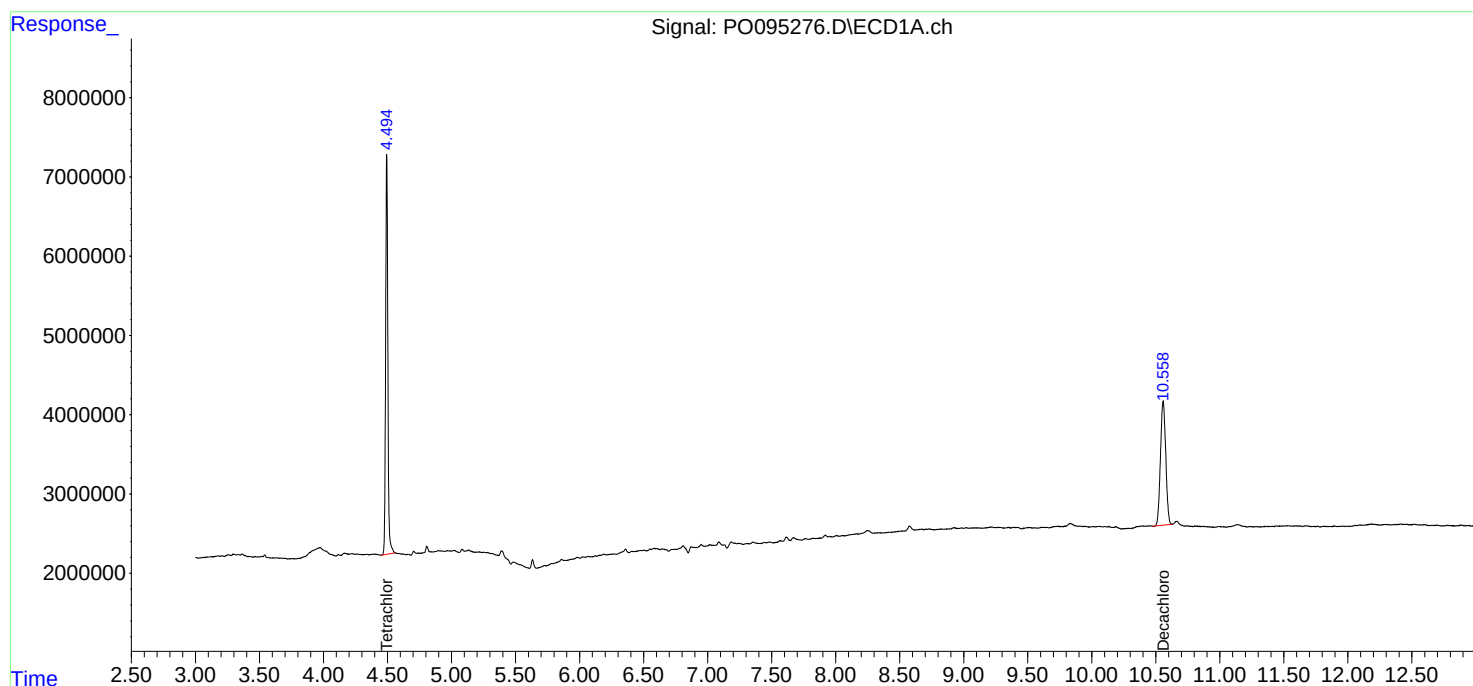

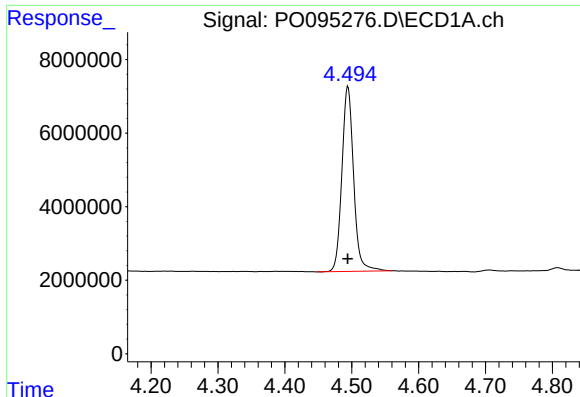


#1 Tetrachloro-m-xylene

R.T.: 4.494 min
Delta R.T.: 0.000 min
Response: 61316607
Conc: 21.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-50A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/24/2023
Supervised By :Ankita Jodhani 05/24/2023

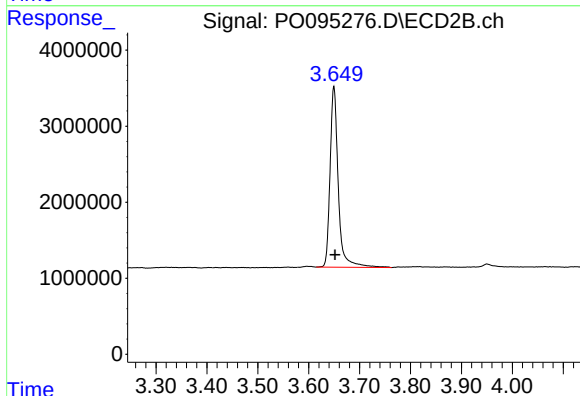


#1 Tetrachloro-m-xylene

R.T.: 3.650 min
Delta R.T.: -0.002 min
Response: 26682465
Conc: 23.50 ng/ml

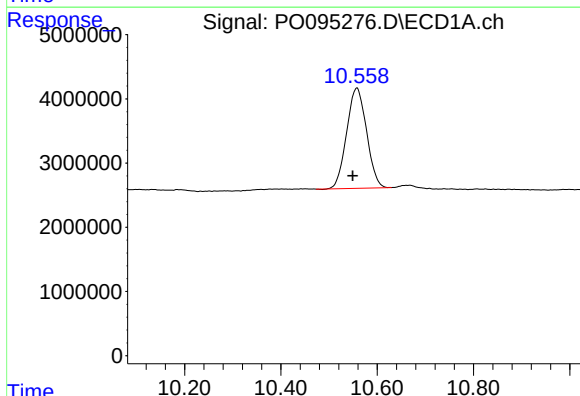

#2 Decachlorobiphenyl

R.T.: 10.558 min
Delta R.T.: 0.009 min
Response: 44675952
Conc: 19.25 ng/ml

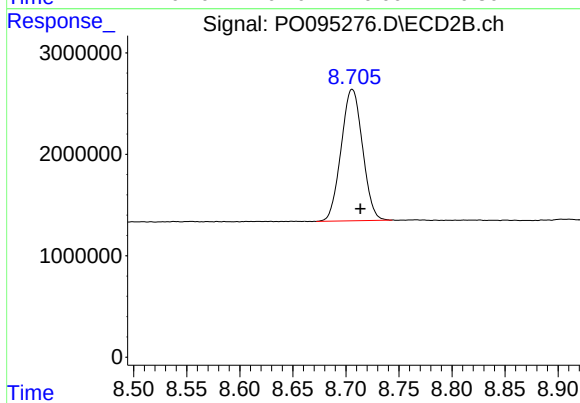

#2 Decachlorobiphenyl

R.T.: 8.705 min
Delta R.T.: -0.008 min
Response: 18172942
Conc: 18.74 ng/ml m