

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052419\
 Data File : P0056619.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 May 2019 6:39
 Operator : SM/SJ
 Sample : K3010-03
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FESB-22(1.5-2)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 23:37:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.255	3.573	1200803	961570	31.366	29.158
2) SA Decachlor...	9.830	8.508	965264	661294	19.666	18.546
Target Compounds						
9) L2 AR-1221-2	0.000	3.871	0	17674	N.D.	46.896 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO052419\
Data File : PO056619.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 May 2019 6:39
Operator : SM/SJ
Sample : K3010-03
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FESB-22(1.5-2)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 23:37:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

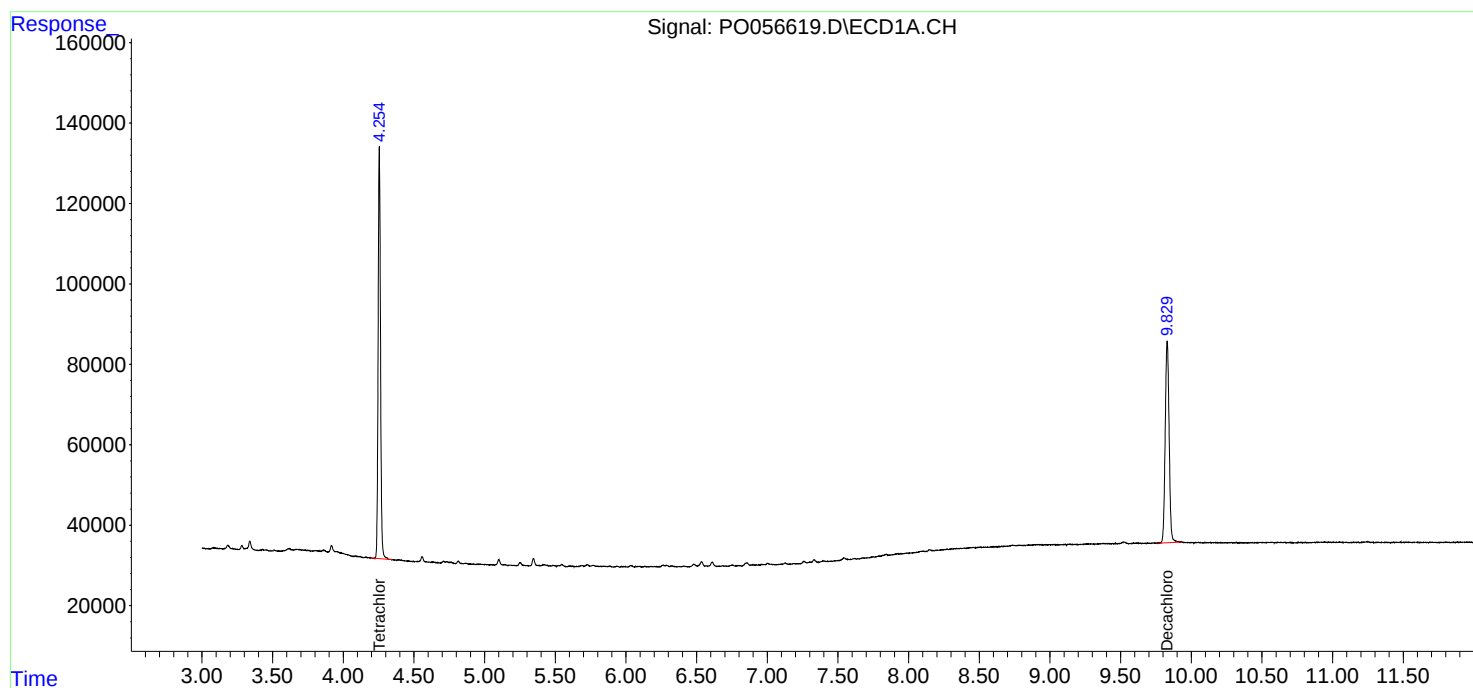


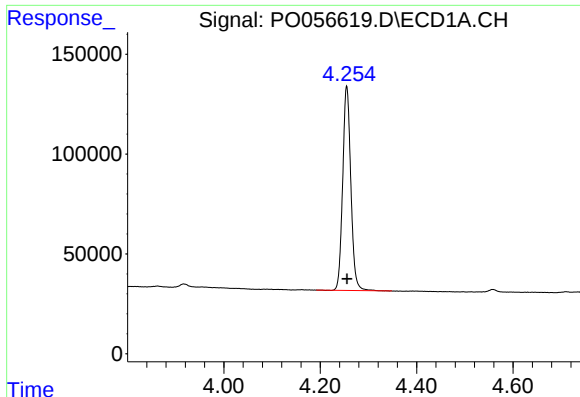

#1 Tetrachloro-m-xylene


R.T.: 4.255 min
Delta R.T.: -0.001 min
Response: 1200803
Conc: 31.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
FESB-22(1.5-2)

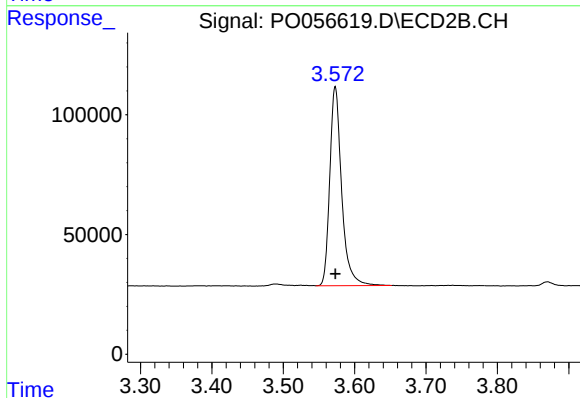


#1 Tetrachloro-m-xylene

R.T.: 3.573 min
Delta R.T.: 0.000 min
Response: 961570
Conc: 29.16 ng/ml

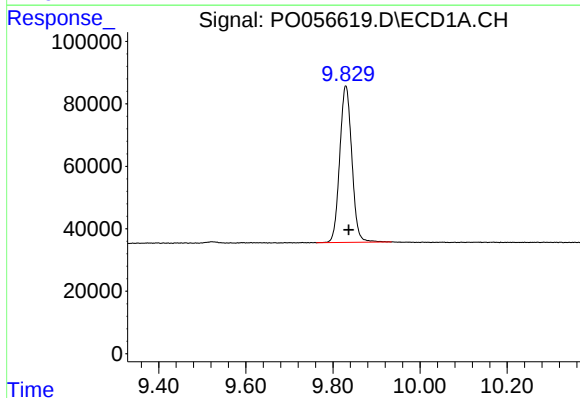


#2 Decachlorobiphenyl

R.T.: 9.830 min
Delta R.T.: -0.007 min
Response: 965264
Conc: 19.67 ng/ml

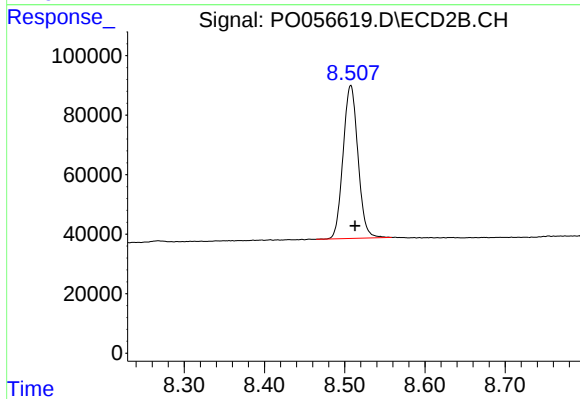

#2 Decachlorobiphenyl


R.T.: 8.508 min
Delta R.T.: -0.005 min
Response: 661294
Conc: 18.55 ng/ml

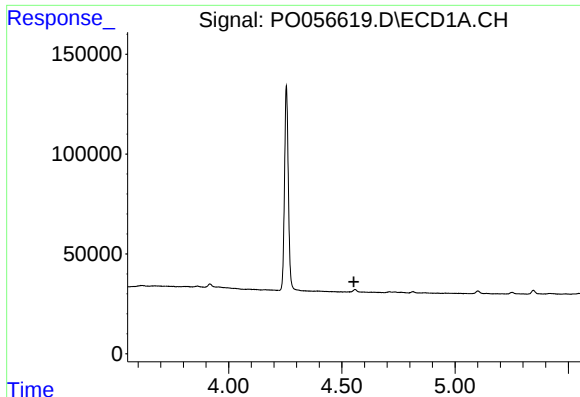

#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 4.553 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FESB-22(1.5-2)

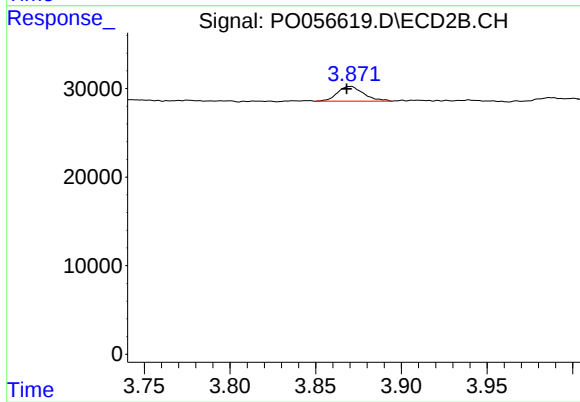

#9 AR-1221-2

R.T.: 3.871 min
Delta R.T.: 0.003 min
Response: 17674
Conc: 46.90 ng/ml