

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052419\
 Data File : P0056547.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 May 2019 9:53
 Operator : SM/SJ
 Sample : K2964-04RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 51030RE

Manual Integrations
 APPROVED

mohammad
 5/25/2019 9:57:05 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 05:50:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.259	3.578	325945	221543	8.514m	6.718m
2)	SA Decachlor...	9.838	8.518	494614	101140	10.077m	2.836m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052419\
Data File : P0056547.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 May 2019 9:53
Operator : SM/SJ
Sample : K2964-04RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
51030RE


Manual Integrations
APPROVED

mohammad
5/25/2019 9:57:05 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 05:50:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

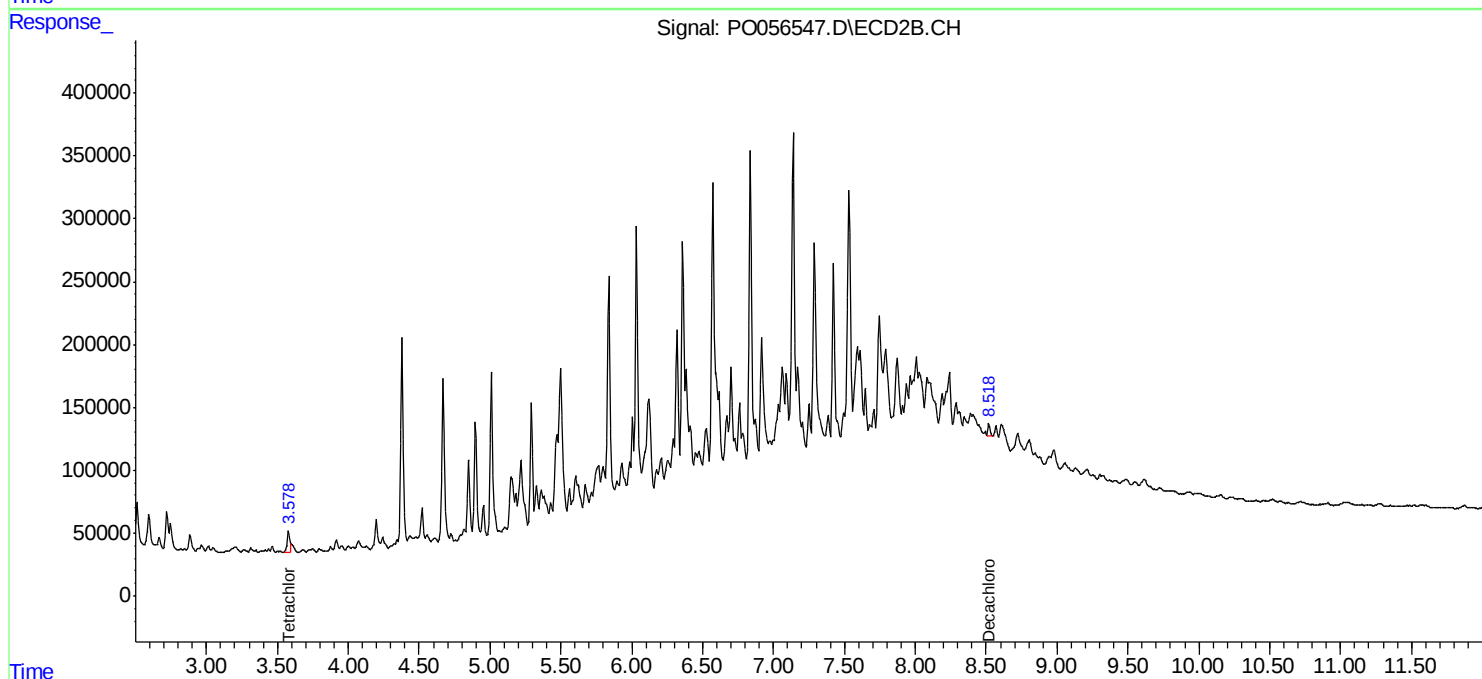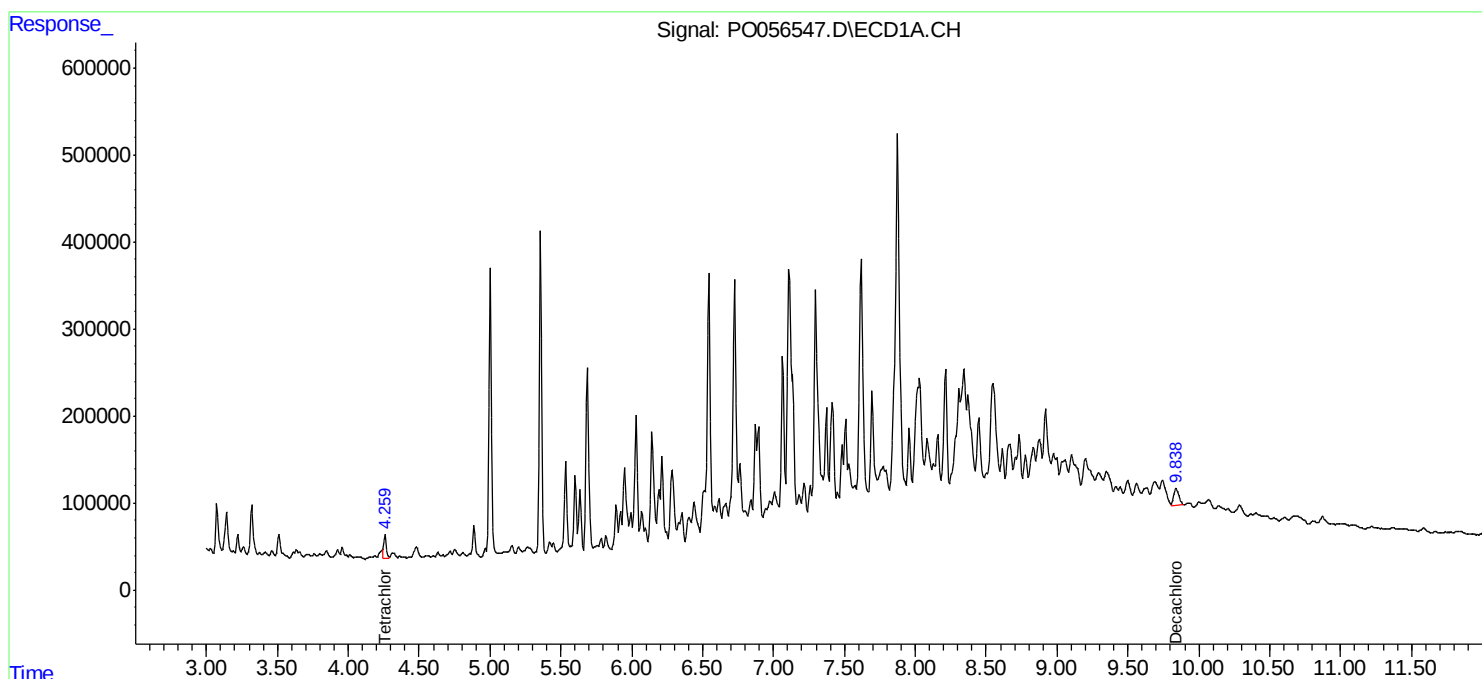

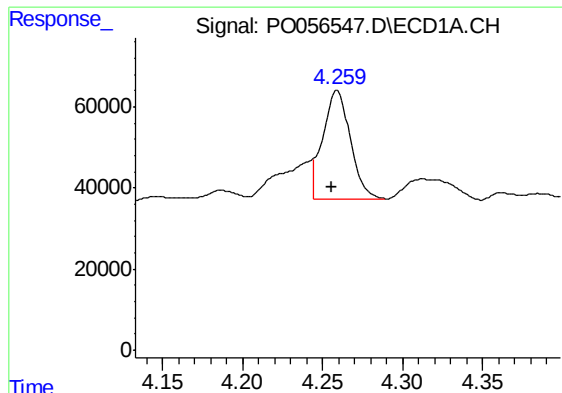


#1 Tetrachloro-m-xylene

R.T.: 4.259 min
Delta R.T.: 0.003 min
Response: 325945
Conc: 8.51 ng/ml m

Instrument :
ECD_O
ClientSampleId :
51030RE


Manual Integrations
APPROVED

mohammad
5/25/2019 9:57:05 AM

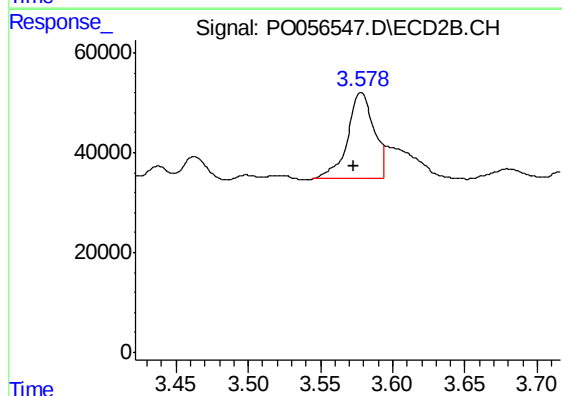


#1 Tetrachloro-m-xylene

R.T.: 3.578 min
Delta R.T.: 0.005 min
Response: 221543
Conc: 6.72 ng/ml m

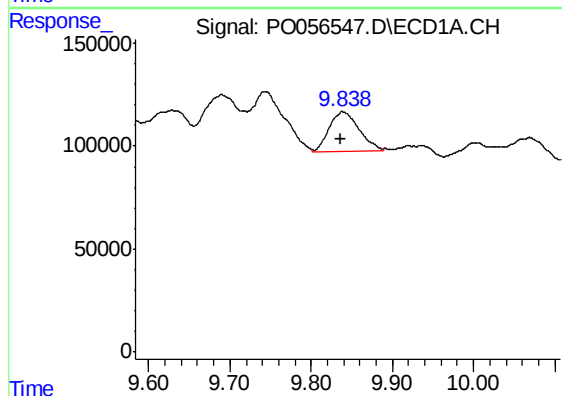

#2 Decachlorobiphenyl

R.T.: 9.838 min
Delta R.T.: 0.001 min
Response: 494614
Conc: 10.08 ng/ml m

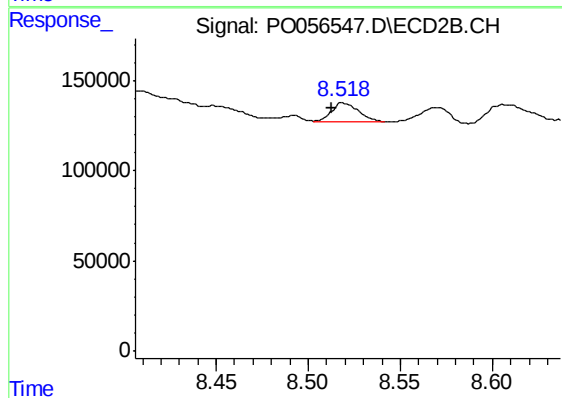

#2 Decachlorobiphenyl

R.T.: 8.518 min
Delta R.T.: 0.005 min
Response: 101140
Conc: 2.84 ng/ml m