

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052419\
 Data File : P0056548.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 May 2019 10:09
 Operator : SM/SJ
 Sample : K2964-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 13818

Manual Integrations
 APPROVED

mohammad
 5/25/2019 9:57:32 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 22:20:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.256	3.573	225386	165990	5.887	5.033
2)	SA Decachlor...	9.836	8.512	173669	116389	3.538m	3.264

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052419\
Data File : P0056548.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 May 2019 10:09
Operator : SM/SJ
Sample : K2964-05
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
13818


Manual Integrations
APPROVED

mohammad
5/25/2019 9:57:32 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 22:20:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

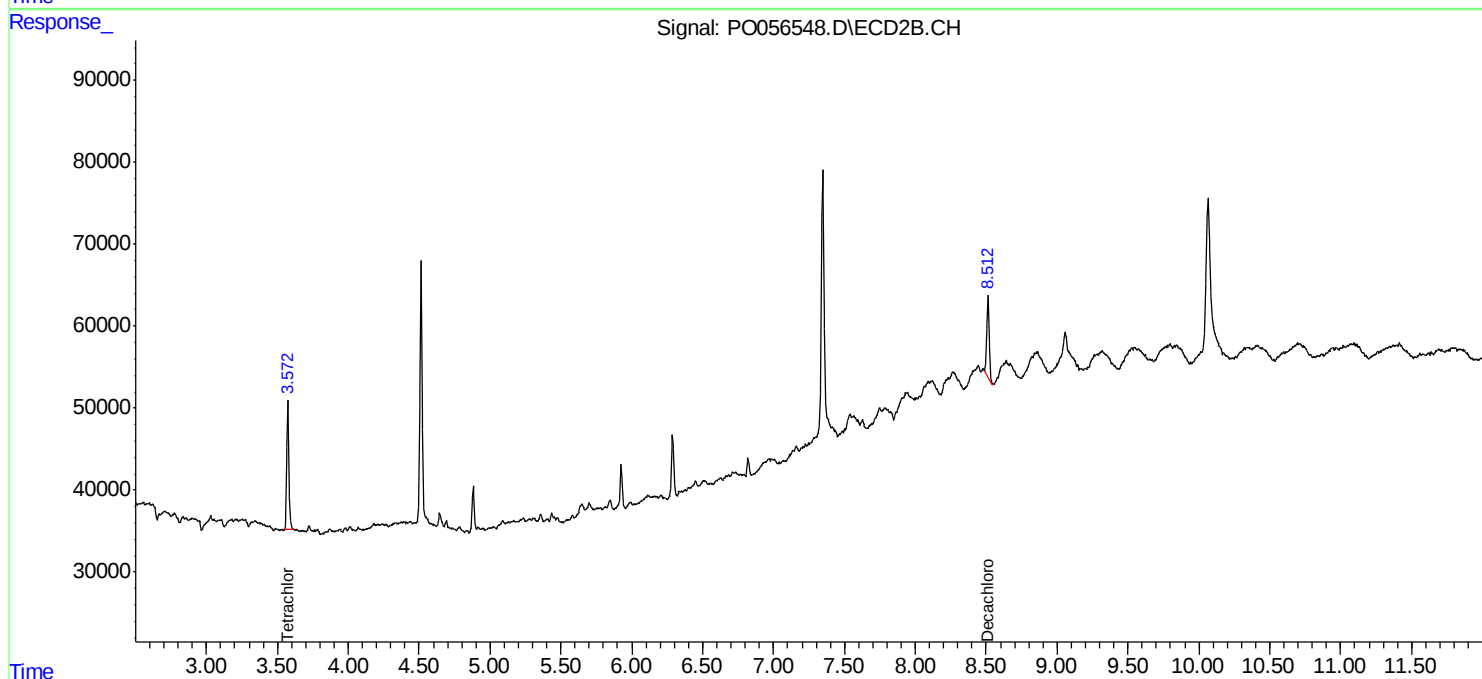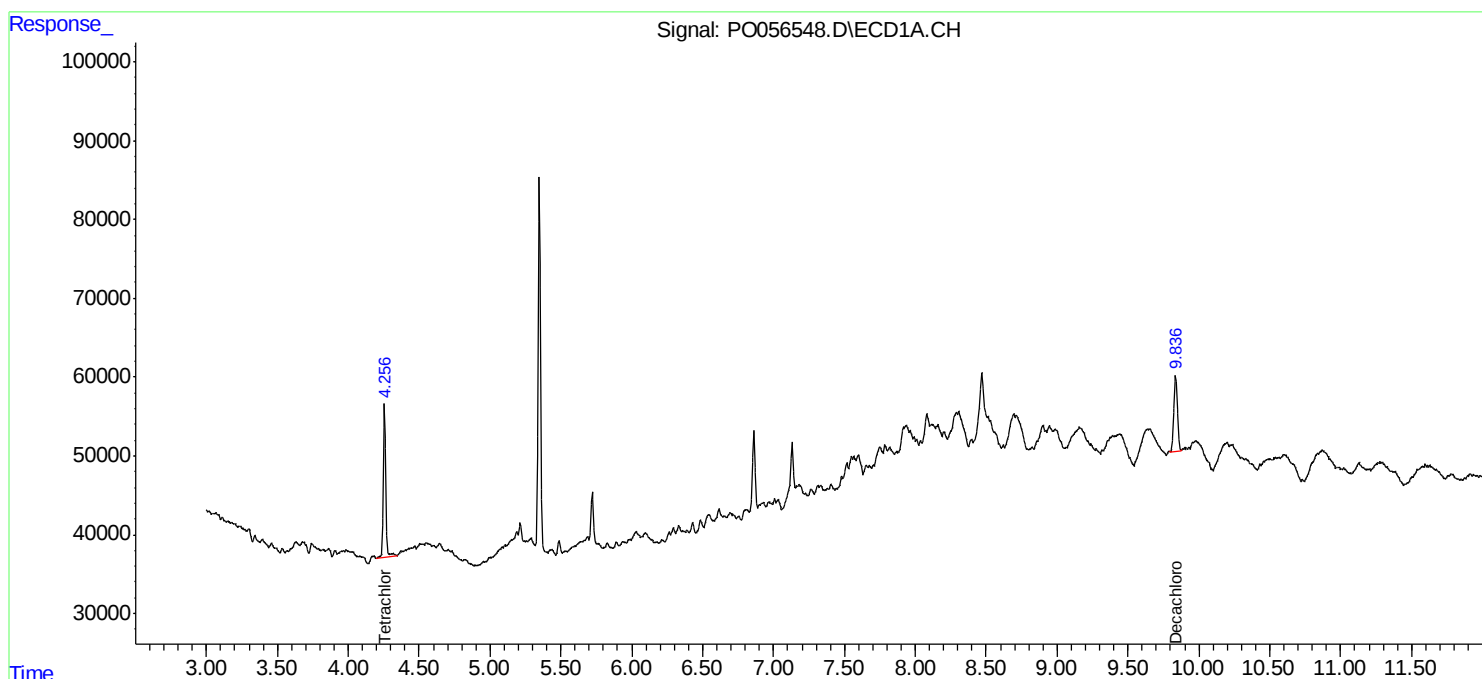

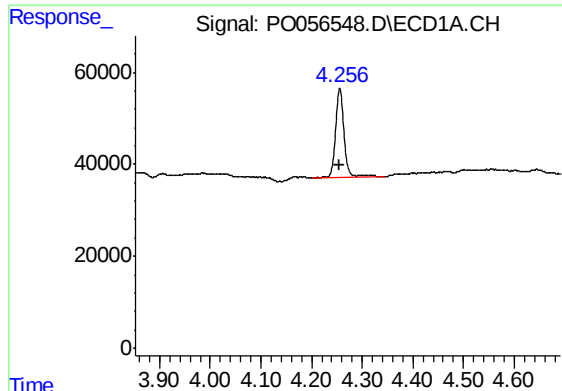


#1 Tetrachloro-m-xylene

R.T.: 4.256 min
Delta R.T.: 0.000 min
Response: 225386
Conc: 5.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
13818


Manual Integrations
APPROVED

mohammad
5/25/2019 9:57:32 AM

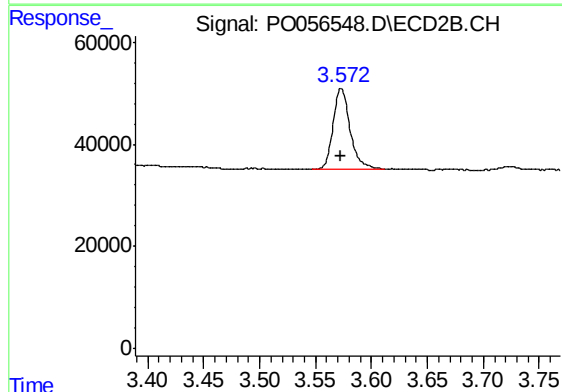


#1 Tetrachloro-m-xylene

R.T.: 3.573 min
Delta R.T.: 0.000 min
Response: 165990
Conc: 5.03 ng/ml

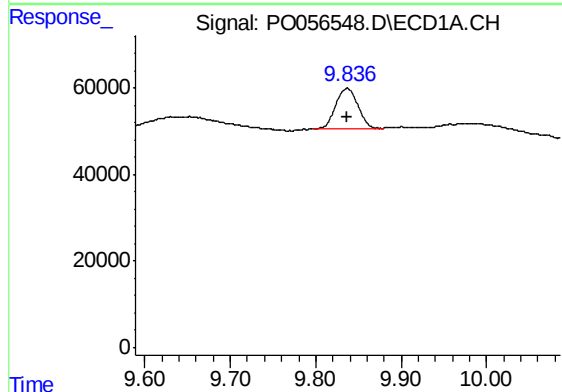

#2 Decachlorobiphenyl

R.T.: 9.836 min
Delta R.T.: 0.000 min
Response: 173669
Conc: 3.54 ng/ml m

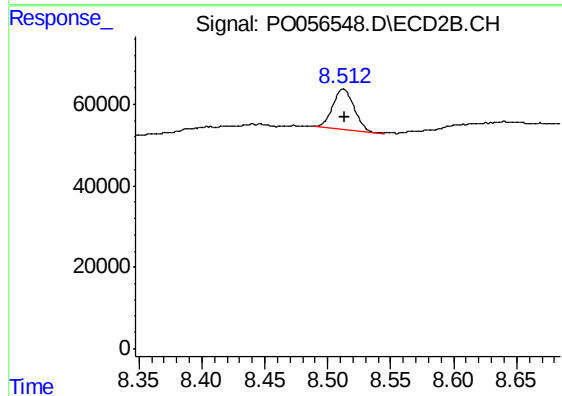

#2 Decachlorobiphenyl

R.T.: 8.512 min
Delta R.T.: 0.000 min
Response: 116389
Conc: 3.26 ng/ml