

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052419\
 Data File : P0056550.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 May 2019 10:43
 Operator : SM/SJ
 Sample : K2964-05RE
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 13818RE

Manual Integrations
 APPROVED

mohammad
 5/25/2019 9:57:49 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 22:21:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.256	3.573	231066	178874	6.036m	5.424
2)	SA Decachlor...	9.836	8.513	207543	129717	4.228	3.638

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052419\
Data File : P0056550.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 May 2019 10:43
Operator : SM/SJ
Sample : K2964-05RE
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
13818RE


Manual Integrations
APPROVED

mohammad
5/25/2019 9:57:49 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 22:21:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

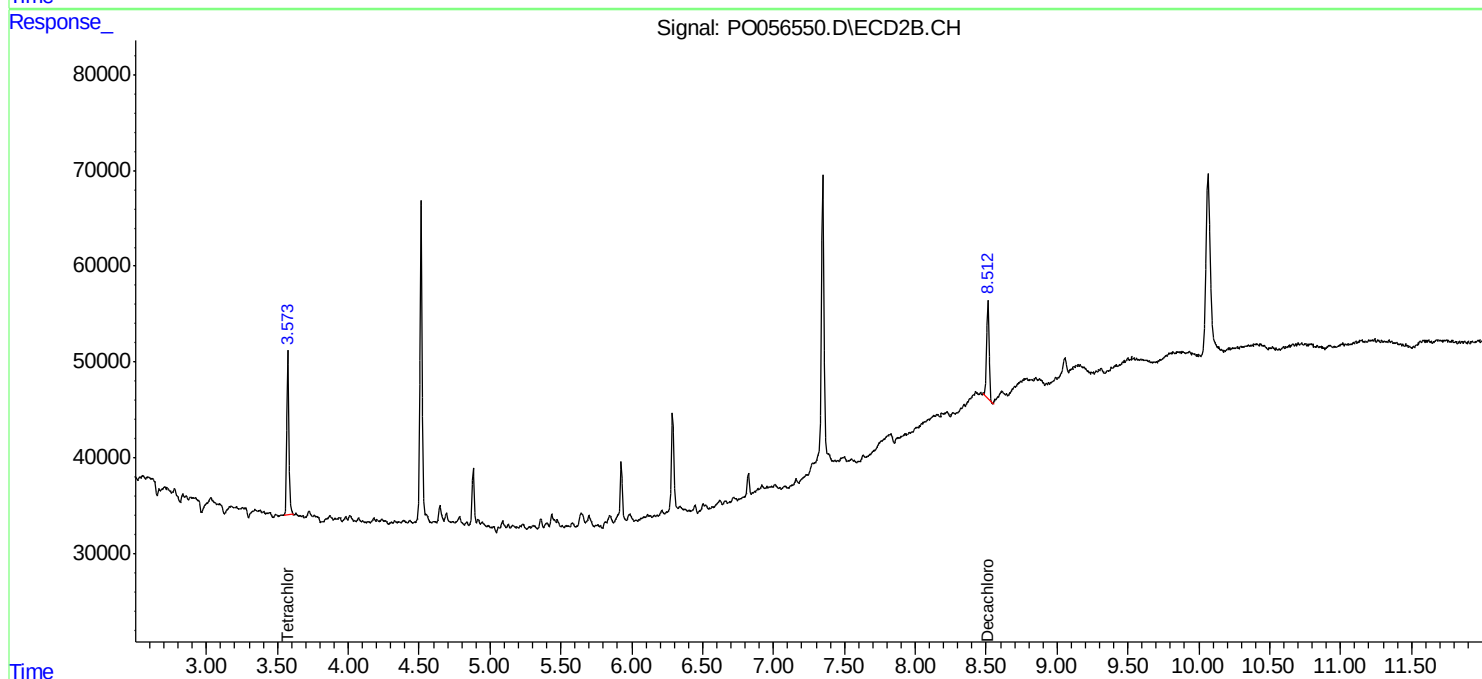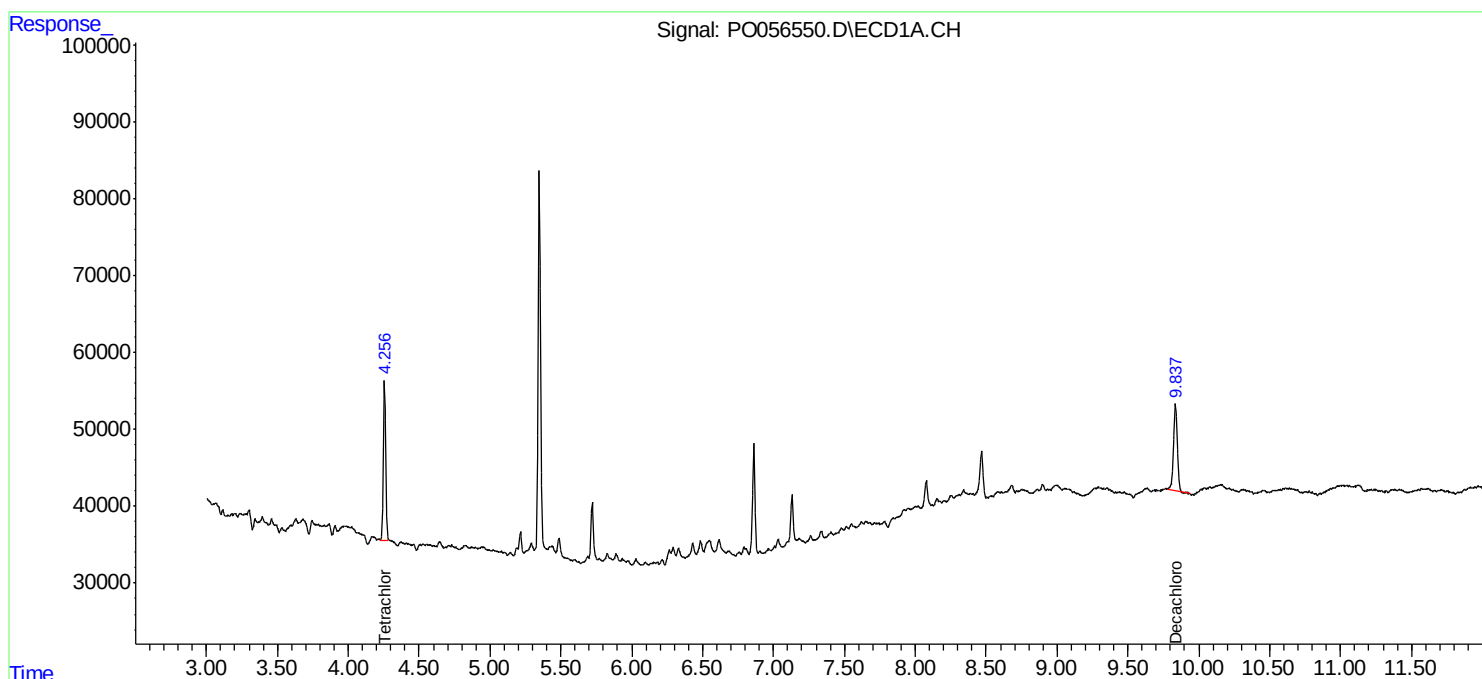

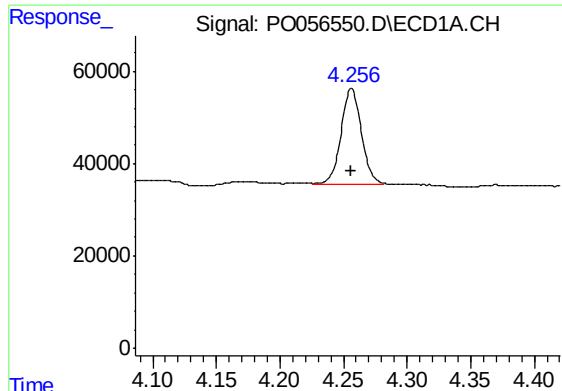


#1 Tetrachloro-m-xylene

R.T.: 4.256 min
Delta R.T.: 0.000 min
Response: 231066
Conc: 6.04 ng/ml m

Instrument :
ECD_O
ClientSampleId :
13818RE


Manual Integrations
APPROVED

mohammad
5/25/2019 9:57:49 AM

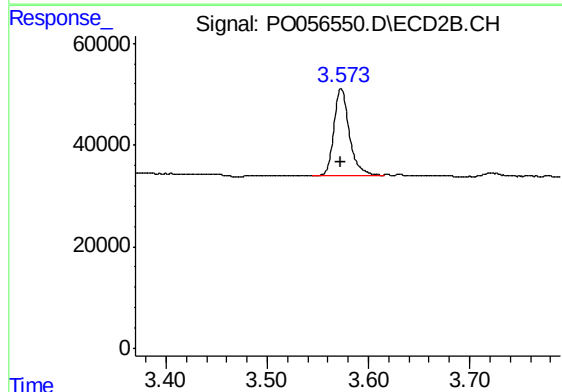


#1 Tetrachloro-m-xylene

R.T.: 3.573 min
Delta R.T.: 0.000 min
Response: 178874
Conc: 5.42 ng/ml

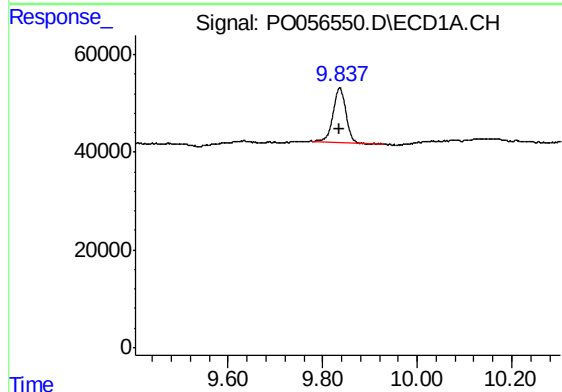

#2 Decachlorobiphenyl

R.T.: 9.836 min
Delta R.T.: 0.000 min
Response: 207543
Conc: 4.23 ng/ml

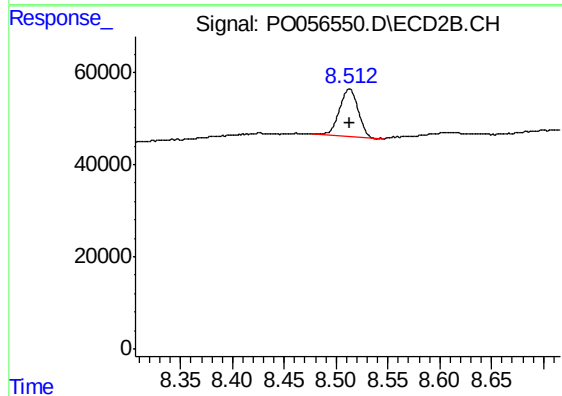

#2 Decachlorobiphenyl

R.T.: 8.513 min
Delta R.T.: 0.000 min
Response: 129717
Conc: 3.64 ng/ml