

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052419\
 Data File : P0056615.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 May 2019 5:31
 Operator : SM/SJ
 Sample : K3008-03
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-20

Manual Integrations
 APPROVED

mohammad
 5/25/2019 10:02:16 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 06:10:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.255	3.574	862816	686397	22.538	20.814
2)	SA Decachlor...	9.830	8.509	789096	516128	16.076	14.475
Target Compounds							
31)	L7 AR-1260-1	7.003	6.107	209529	178377	81.650m	89.172
32)	L7 AR-1260-2	7.259	6.294	534414	196473	176.715	79.706 #
33)	L7 AR-1260-3	7.615	6.445	135974	172158	56.443	76.746m#
34)	L7 AR-1260-4	7.839	6.914	168483	100724	64.326	54.123
35)	L7 AR-1260-5	8.149	7.155	238609	236941	49.897	54.945m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052419\
Data File : P0056615.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 May 2019 5:31
Operator : SM/SJ
Sample : K3008-03
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-20


Manual Integrations
APPROVED

mohammad
5/25/2019 10:02:16 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 06:10:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

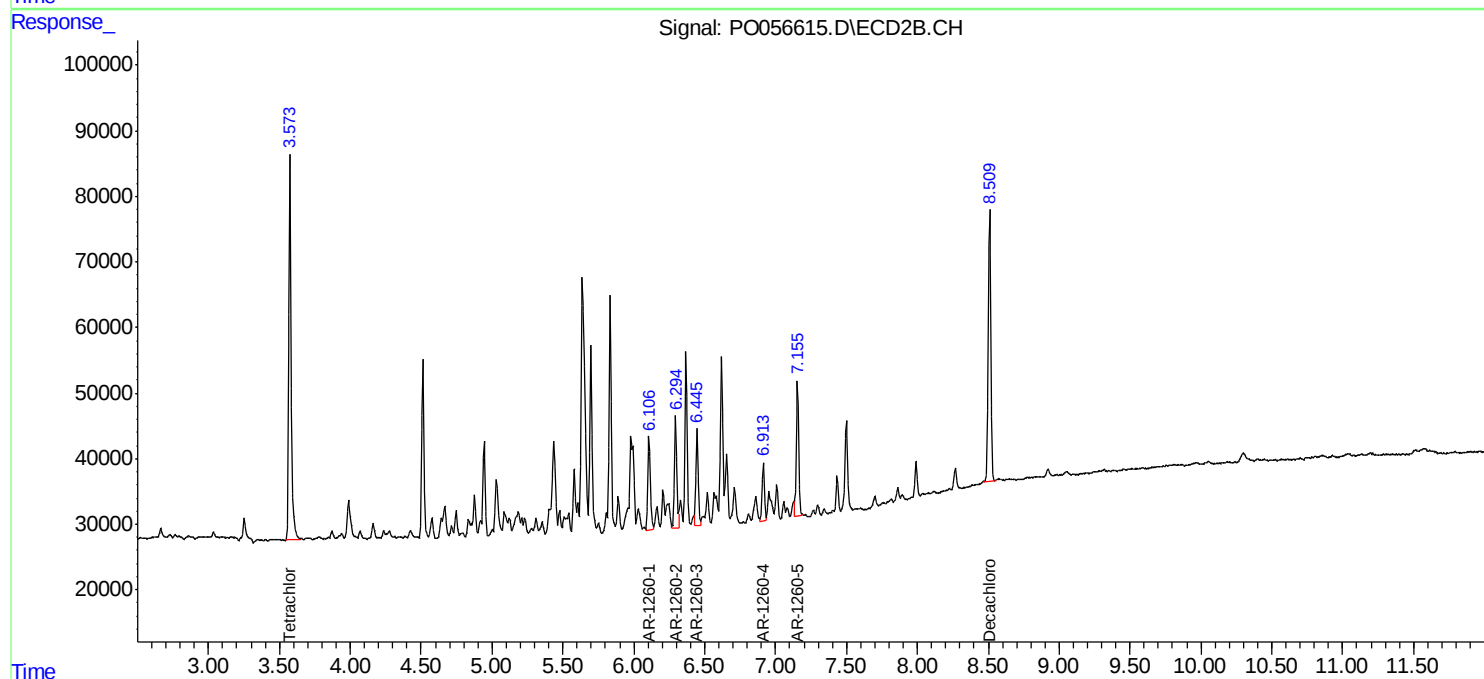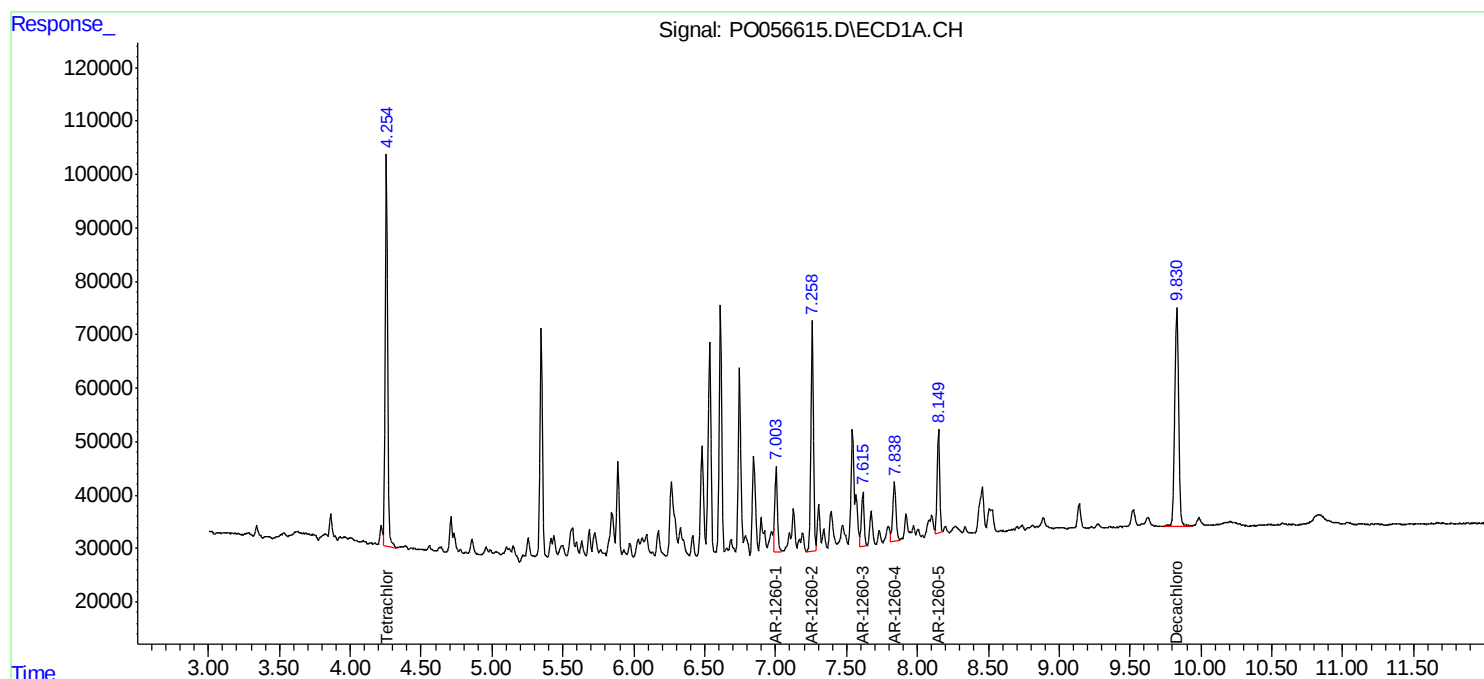

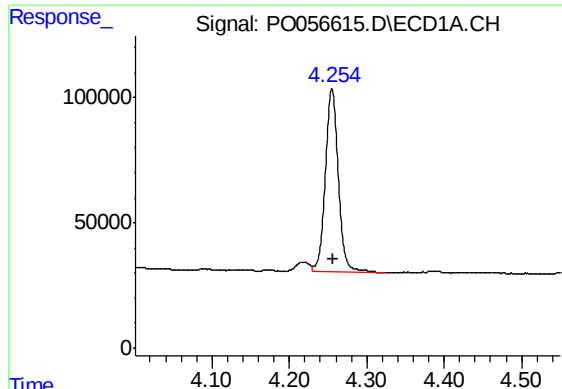


#1 Tetrachloro-m-xylene

R.T.: 4.255 min
Delta R.T.: 0.000 min
Response: 862816
Conc: 22.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-20


Manual Integrations
APPROVED

mohammad
5/25/2019 10:02:16 AM

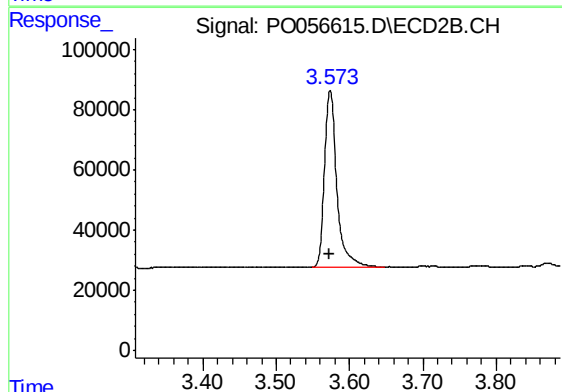


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: 0.000 min
Response: 686397
Conc: 20.81 ng/ml

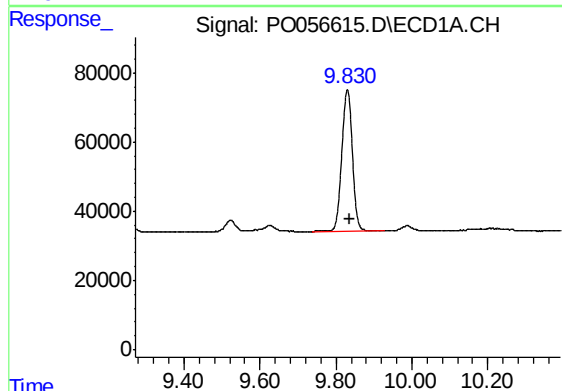


#2 Decachlorobiphenyl

R.T.: 9.830 min
Delta R.T.: -0.006 min
Response: 789096
Conc: 16.08 ng/ml

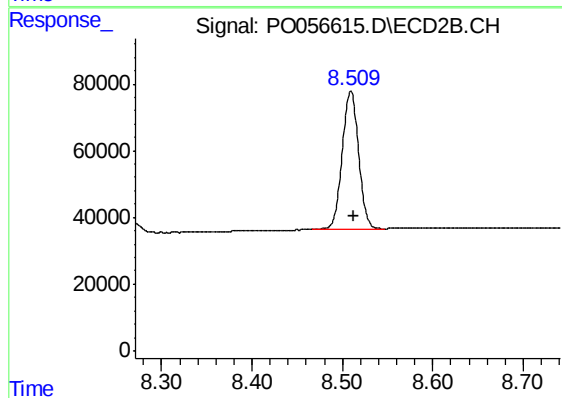

#2 Decachlorobiphenyl

R.T.: 8.509 min
Delta R.T.: -0.004 min
Response: 516128
Conc: 14.47 ng/ml

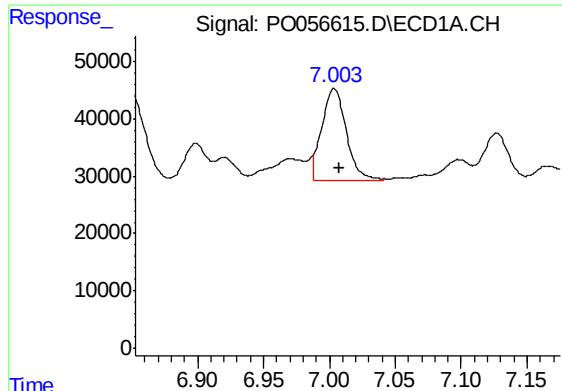


#31 AR-1260-1

R.T.: 7.003 min
Delta R.T.: -0.004 min
Response: 209529
Conc: 81.65 ng/ml m

Instrument :
ECD_O
ClientSampleId :
COMP-20


Manual Integrations
APPROVED

mohammad
5/25/2019 10:02:16 AM

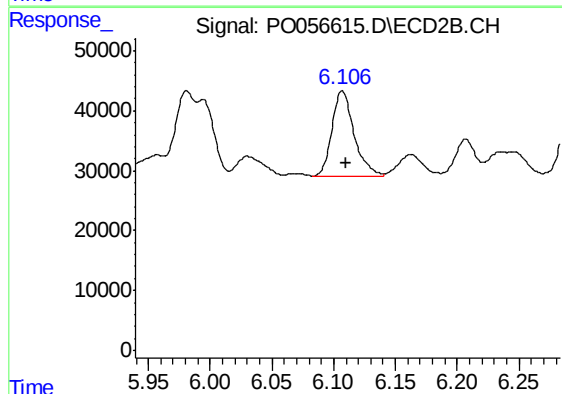


#31 AR-1260-1

R.T.: 6.107 min
Delta R.T.: -0.003 min
Response: 178377
Conc: 89.17 ng/ml

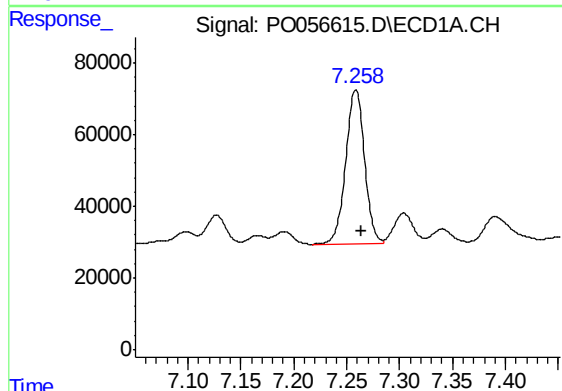


#32 AR-1260-2

R.T.: 7.259 min
Delta R.T.: -0.005 min
Response: 534414
Conc: 176.71 ng/ml

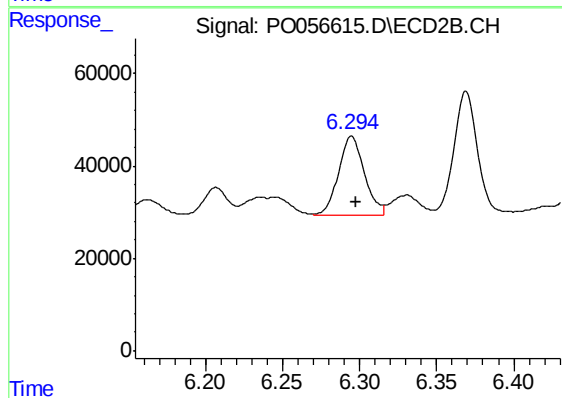

#32 AR-1260-2

R.T.: 6.294 min
Delta R.T.: -0.003 min
Response: 196473
Conc: 79.71 ng/ml

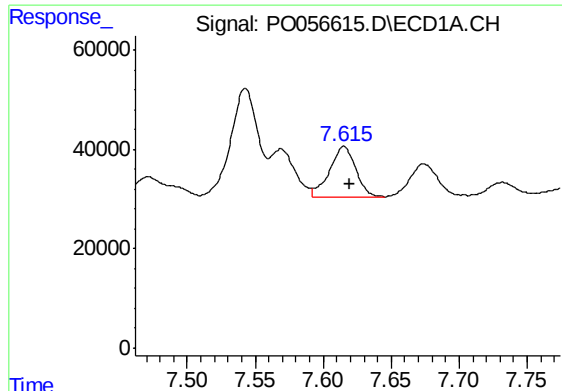


#33 AR-1260-3

R.T.: 7.615 min
Delta R.T.: -0.005 min
Response: 135974
Conc: 56.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-20


Manual Integrations
APPROVED

mohammad
5/25/2019 10:02:16 AM

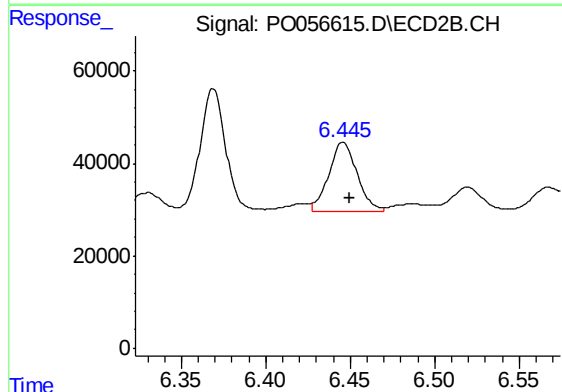


#33 AR-1260-3

R.T.: 6.445 min
Delta R.T.: -0.004 min
Response: 172158
Conc: 76.75 ng/ml m

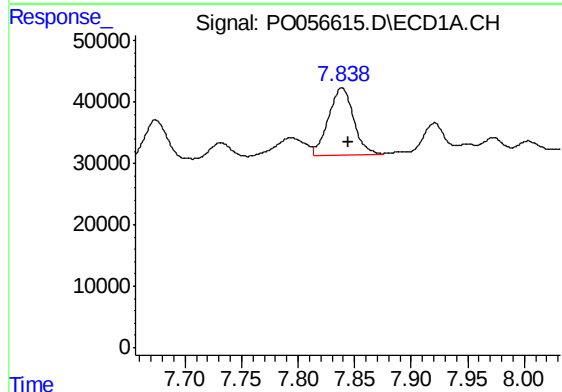


#34 AR-1260-4

R.T.: 7.839 min
Delta R.T.: -0.006 min
Response: 168483
Conc: 64.33 ng/ml

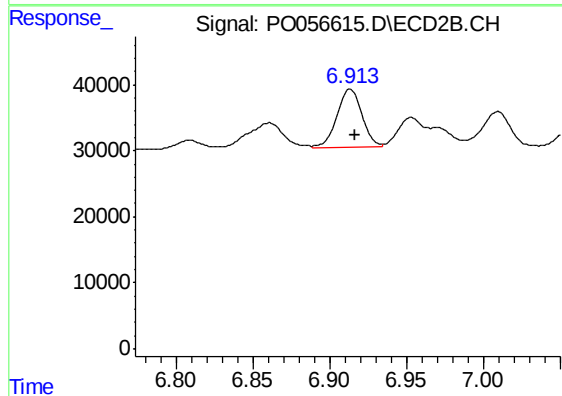

#34 AR-1260-4

R.T.: 6.914 min
Delta R.T.: -0.003 min
Response: 100724
Conc: 54.12 ng/ml

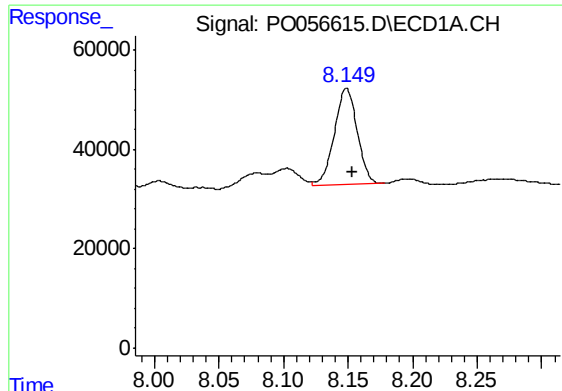


#35 AR-1260-5

R.T.: 8.149 min
Delta R.T.: -0.005 min
Response: 238609
Conc: 49.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-20

Manual Integrations
APPROVED

mohammad
5/25/2019 10:02:16 AM

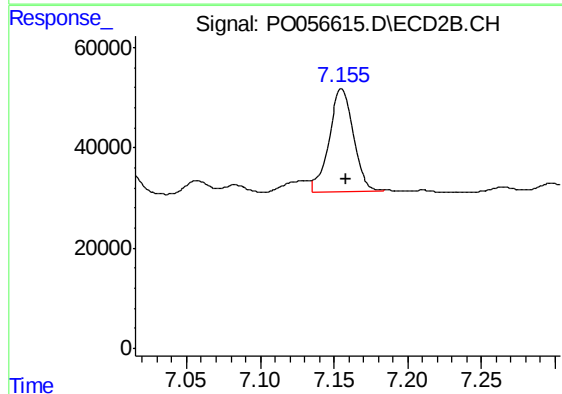

#35 AR-1260-5

R.T.: 7.155 min
Delta R.T.: -0.003 min
Response: 236941
Conc: 54.94 ng/ml m