

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052419\
 Data File : P0056618.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 May 2019 6:22
 Operator : SM/SJ
 Sample : K3010-02
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FESB-23(3-3.5)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 23:37:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.255	3.573	1013608	828267	26.476	25.115
2)	SA Decachlor...	9.830	8.508	890792	612825	18.148	17.187

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO052419\
Data File : PO056618.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 May 2019 6:22
Operator : SM/SJ
Sample : K3010-02
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FESB-23(3-3.5)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 23:37:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

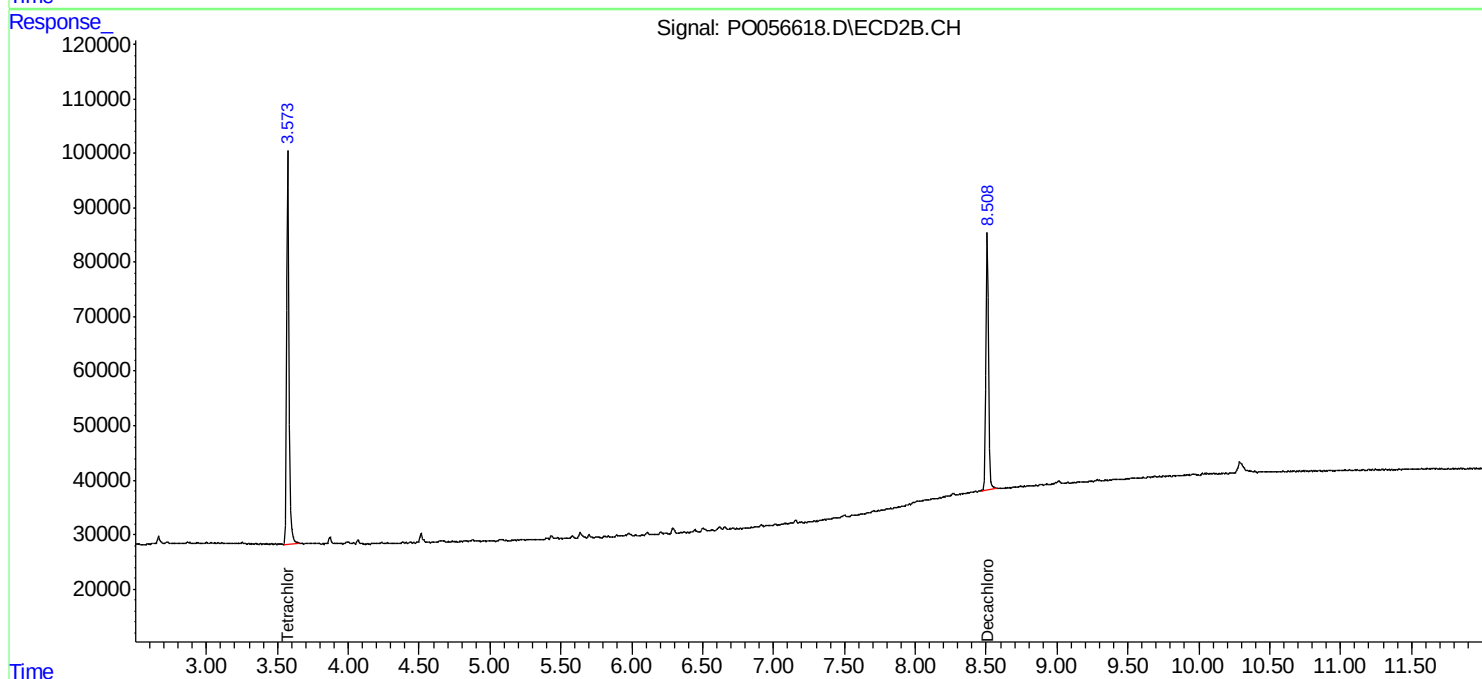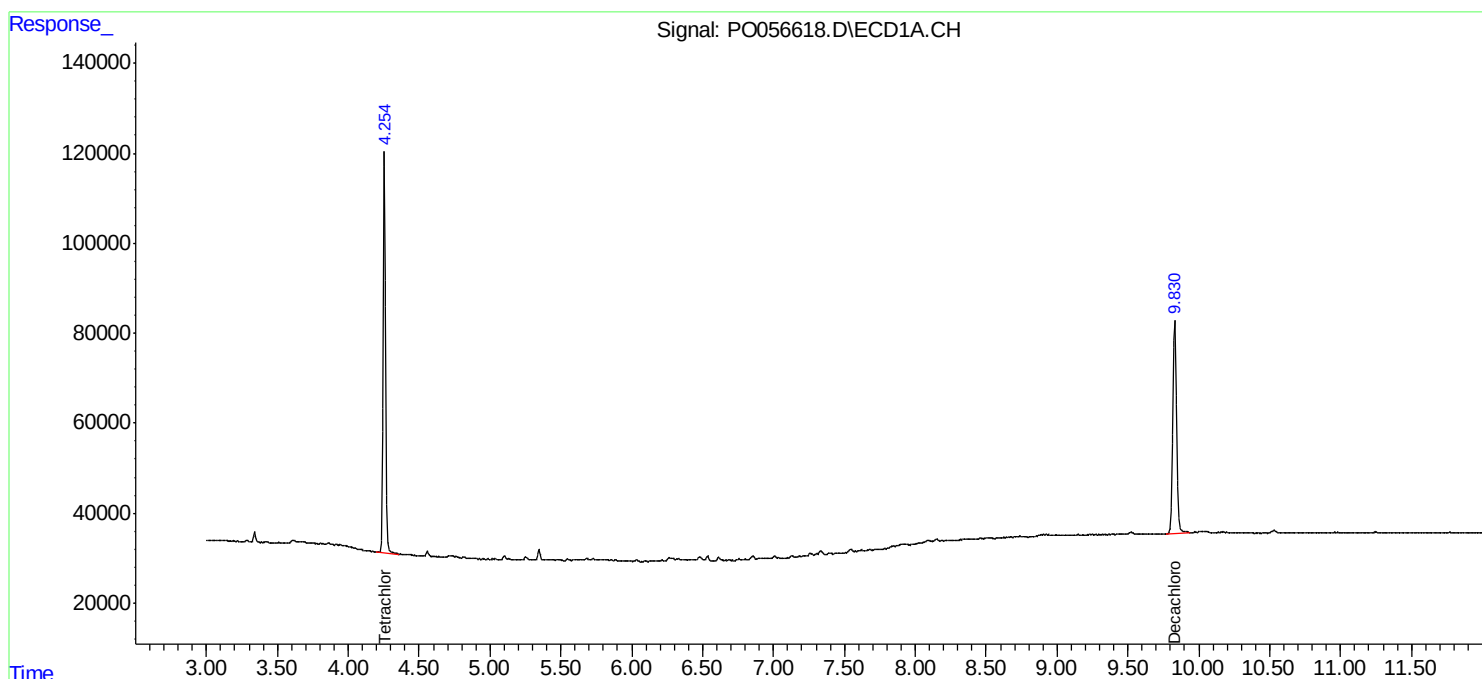


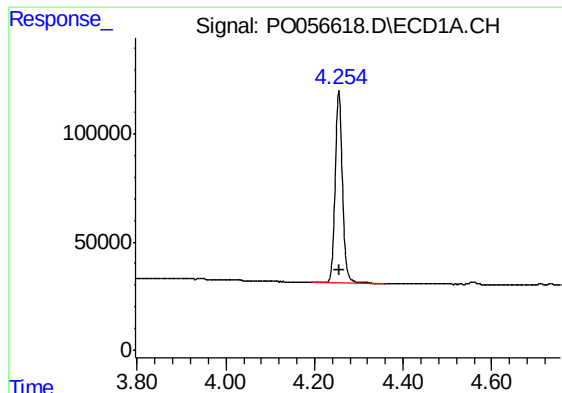

#1 Tetrachloro-m-xylene


R.T.: 4.255 min
Delta R.T.: -0.001 min
Response: 1013608
Conc: 26.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
FESB-23(3-3.5)

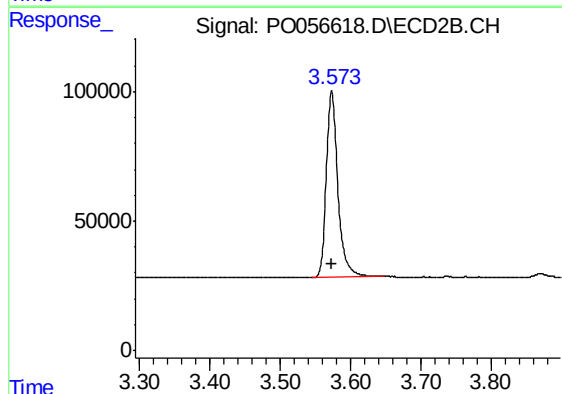


#1 Tetrachloro-m-xylene

R.T.: 3.573 min
Delta R.T.: 0.000 min
Response: 828267
Conc: 25.12 ng/ml

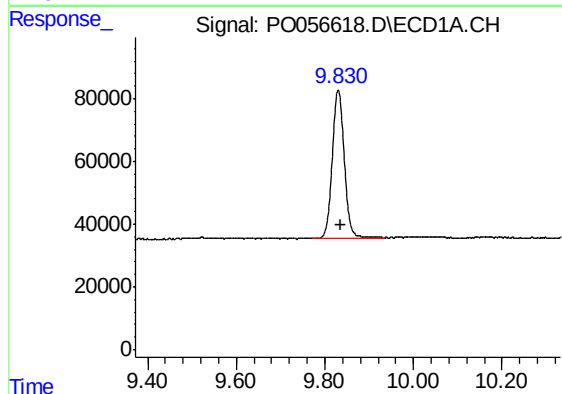

#2 Decachlorobiphenyl

R.T.: 9.830 min
Delta R.T.: -0.006 min
Response: 890792
Conc: 18.15 ng/ml

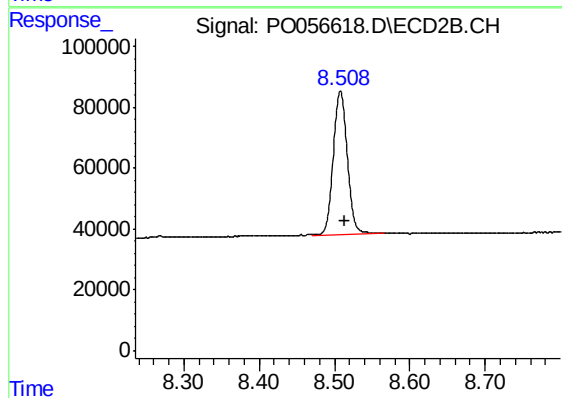

#2 Decachlorobiphenyl

R.T.: 8.508 min
Delta R.T.: -0.005 min
Response: 612825
Conc: 17.19 ng/ml