

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052422\
 Data File : P0086488.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 May 2022 16:14
 Operator : YP\AJ
 Sample : N2876-21
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 P007-SS014-0006-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/25/2022
 Supervised By :Ankita Jodhani 05/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 02:33:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 19 09:06:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.477	3.673	3070890	1329463	30.223	30.522
2) SA Decachlor...	10.328	8.723	1817038	1018073	33.464	29.254
Target Compounds						
31) L7 AR-1260-1	7.277	6.266	42172	22157	13.935	11.384
32) L7 AR-1260-2	7.535	6.453	68256	37597	18.868	15.996
33) L7 AR-1260-3	7.898	6.614	38851	44938	14.076	20.899m#
34) L7 AR-1260-4	8.114	7.080	57281	10614	16.977	5.895m#
35) L7 AR-1260-5	8.453	7.321	43965	23336	7.125	5.387

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO052422\
Data File : PO086488.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 May 2022 16:14
Operator : YP\AJ
Sample : N2876-21
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
P007-SS014-0006-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/25/2022
Supervised By :Ankita Jodhani 05/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 02:33:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 19 09:06:34 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

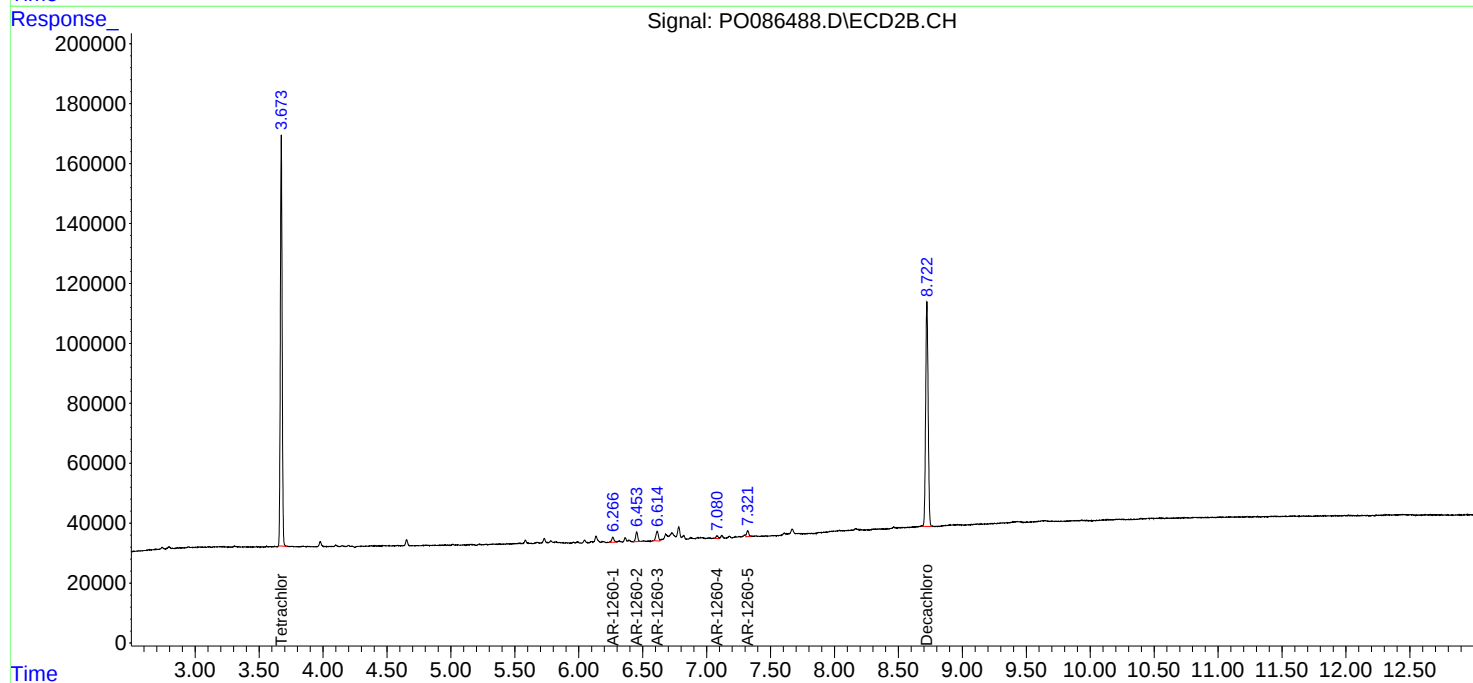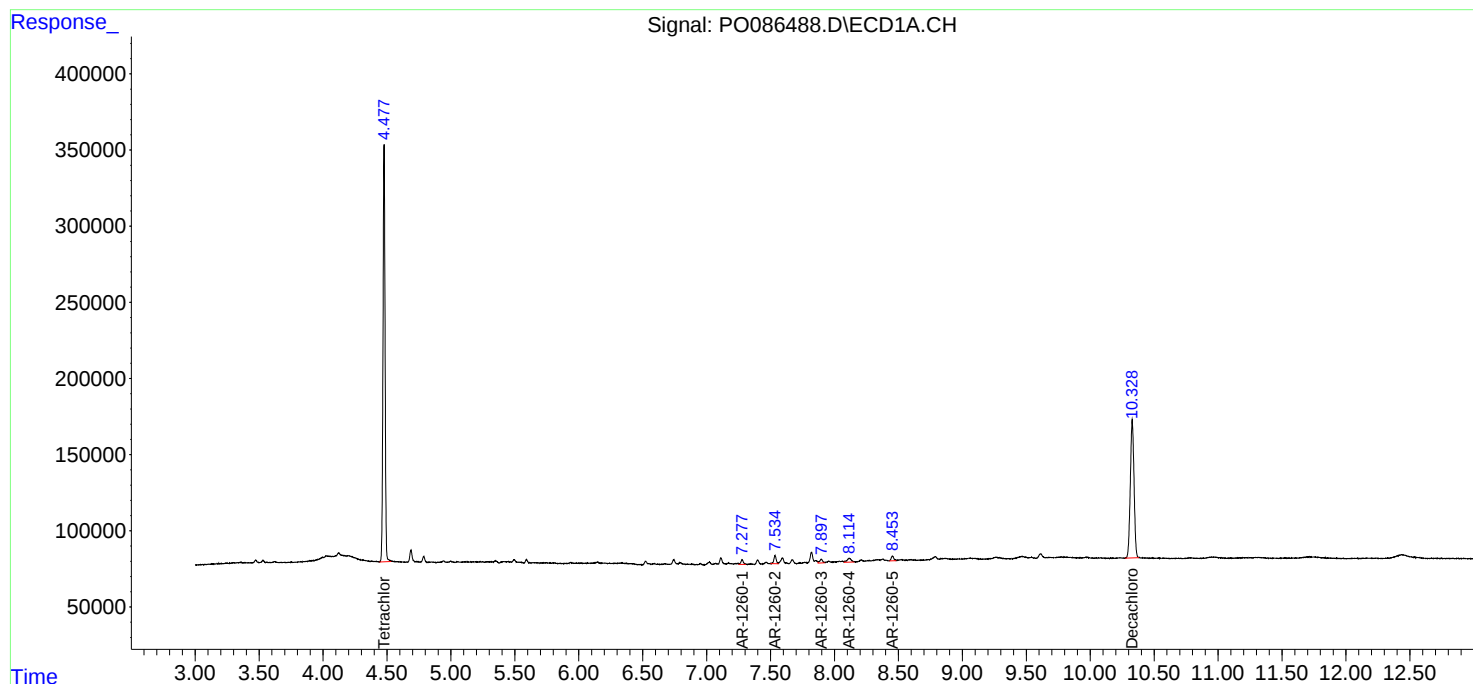

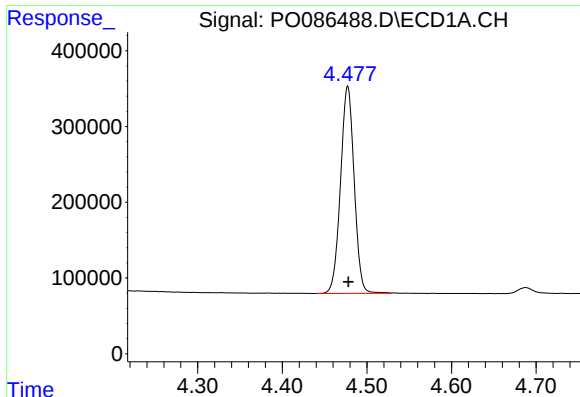


#1 Tetrachloro-m-xylene

R.T.: 4.477 min
Delta R.T.: 0.000 min
Response: 3070890
Conc: 30.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
P007-SS014-0006-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/25/2022
Supervised By :Ankita Jodhani 05/25/2022

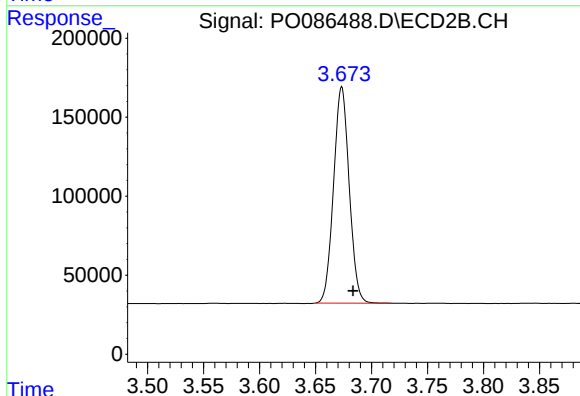


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: -0.010 min
Response: 1329463
Conc: 30.52 ng/ml

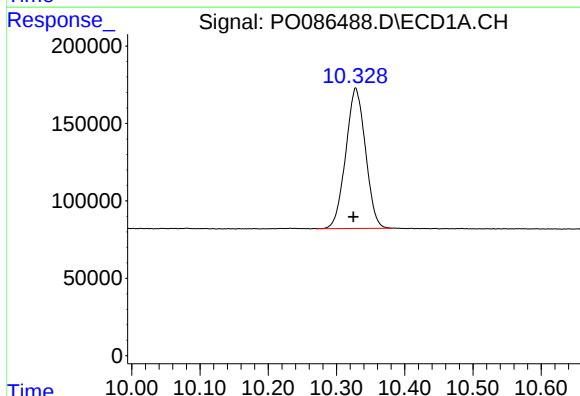


#2 Decachlorobiphenyl

R.T.: 10.328 min
Delta R.T.: 0.003 min
Response: 1817038
Conc: 33.46 ng/ml

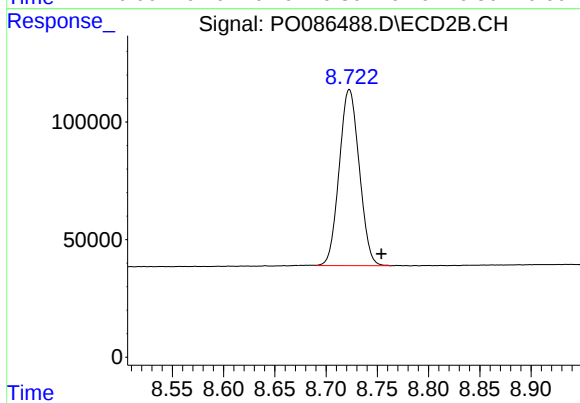

#2 Decachlorobiphenyl

R.T.: 8.723 min
Delta R.T.: -0.031 min
Response: 1018073
Conc: 29.25 ng/ml

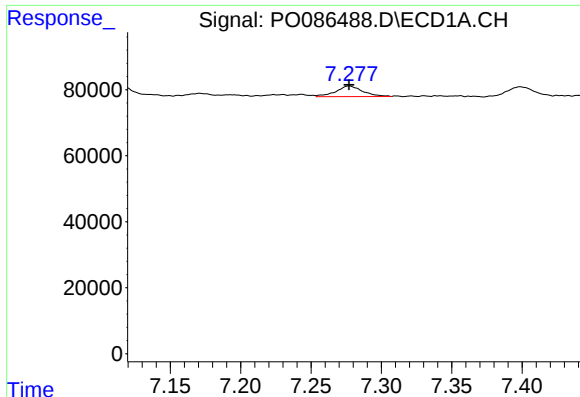


#31 AR-1260-1

R.T.: 7.277 min
Delta R.T.: 0.000 min
Response: 42172
Conc: 13.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
P007-SS014-0006-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/25/2022
Supervised By :Ankita Jodhani 05/25/2022

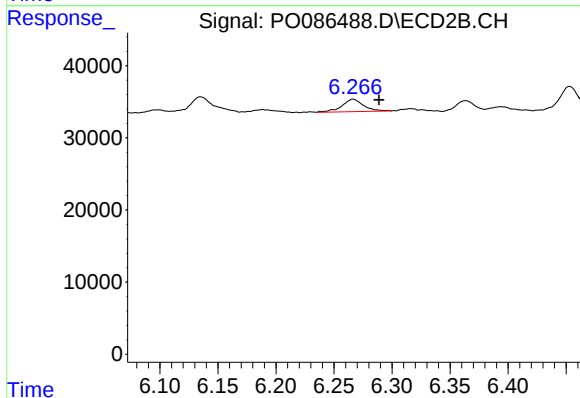


#31 AR-1260-1

R.T.: 6.266 min
Delta R.T.: -0.022 min
Response: 22157
Conc: 11.38 ng/ml

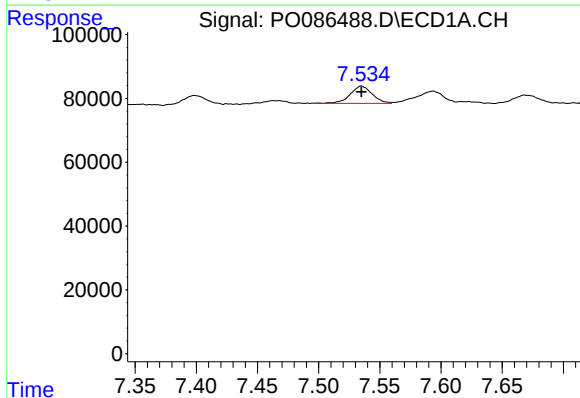


#32 AR-1260-2

R.T.: 7.535 min
Delta R.T.: 0.000 min
Response: 68256
Conc: 18.87 ng/ml

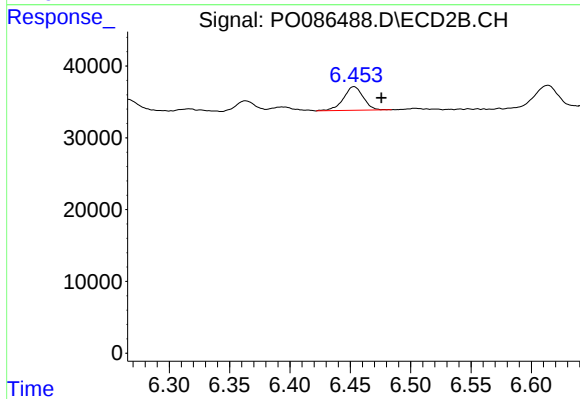

#32 AR-1260-2

R.T.: 6.453 min
Delta R.T.: -0.023 min
Response: 37597
Conc: 16.00 ng/ml

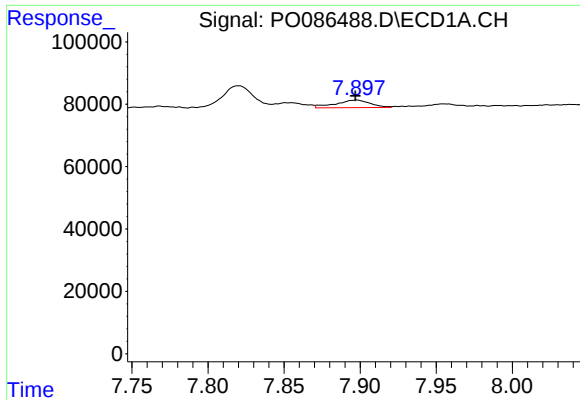


#33 AR-1260-3

R.T.: 7.898 min
Delta R.T.: 0.001 min
Response: 38851
Conc: 14.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
P007-SS014-0006-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/25/2022
Supervised By :Ankita Jodhani 05/25/2022

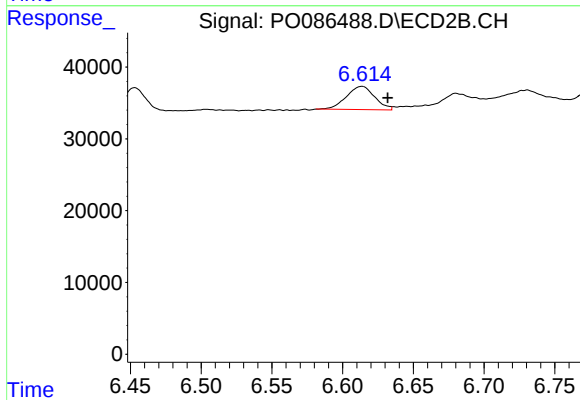


#33 AR-1260-3

R.T.: 6.614 min
Delta R.T.: -0.018 min
Response: 44938
Conc: 20.90 ng/ml m

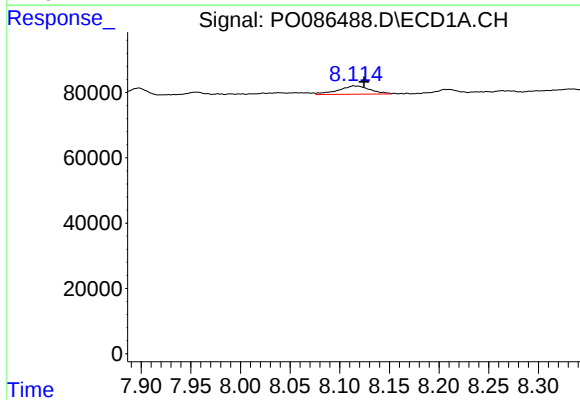


#34 AR-1260-4

R.T.: 8.114 min
Delta R.T.: -0.011 min
Response: 57281
Conc: 16.98 ng/ml

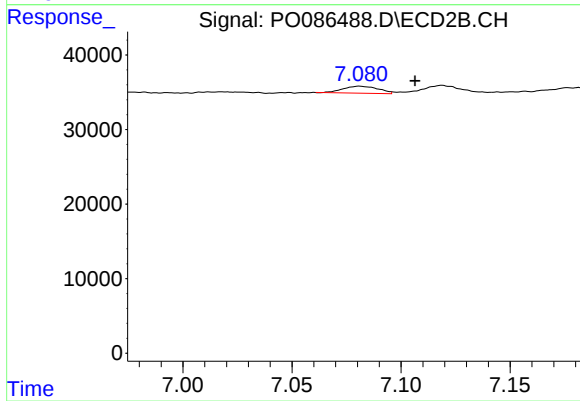

#34 AR-1260-4

R.T.: 7.080 min
Delta R.T.: -0.026 min
Response: 10614
Conc: 5.89 ng/ml m

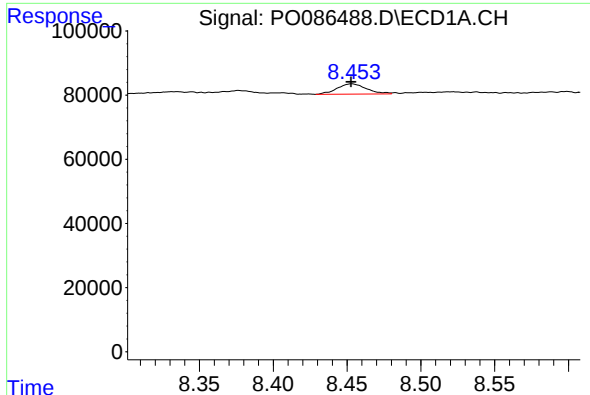


#35 AR-1260-5

R.T.: 8.453 min
Delta R.T.: 0.000 min
Response: 43965
Conc: 7.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
P007-SS014-0006-01

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/25/2022
Supervised By :Ankita Jodhani 05/25/2022

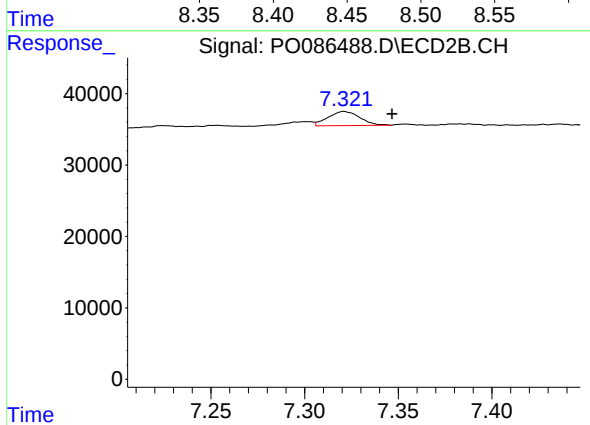

#35 AR-1260-5

R.T.: 7.321 min
Delta R.T.: -0.026 min
Response: 23336
Conc: 5.39 ng/ml