

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0052422\
 Data File : P0086504.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 May 2022 21:23
 Operator : YP\AJ
 Sample : N2896-04
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 P038-SS001-0006-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/25/2022
 Supervised By :Ankita Jodhani 05/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 02:39:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 19 09:06:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.477	3.673	2409520	1071509	23.714	24.600
2) SA Decachlor...	10.326	8.722	1428921	788623	26.316	22.661
Target Compounds						
31) L7 AR-1260-1	7.276	6.266	263406	103845	87.036	53.355 #
32) L7 AR-1260-2	7.534	6.453	268416	150447	74.199	64.011
33) L7 AR-1260-3	7.897	6.609	199872	78124	72.417	36.332 #
34) L7 AR-1260-4	8.125	7.080	191587	73737	56.784	40.950m#
35) L7 AR-1260-5	8.451	7.321	382535	220467	61.992	50.895

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052422\
Data File : P0086504.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 May 2022 21:23
Operator : YP\AJ
Sample : N2896-04
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
P038-SS001-0006-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/25/2022
Supervised By :Ankita Jodhani 05/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 02:39:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 19 09:06:34 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

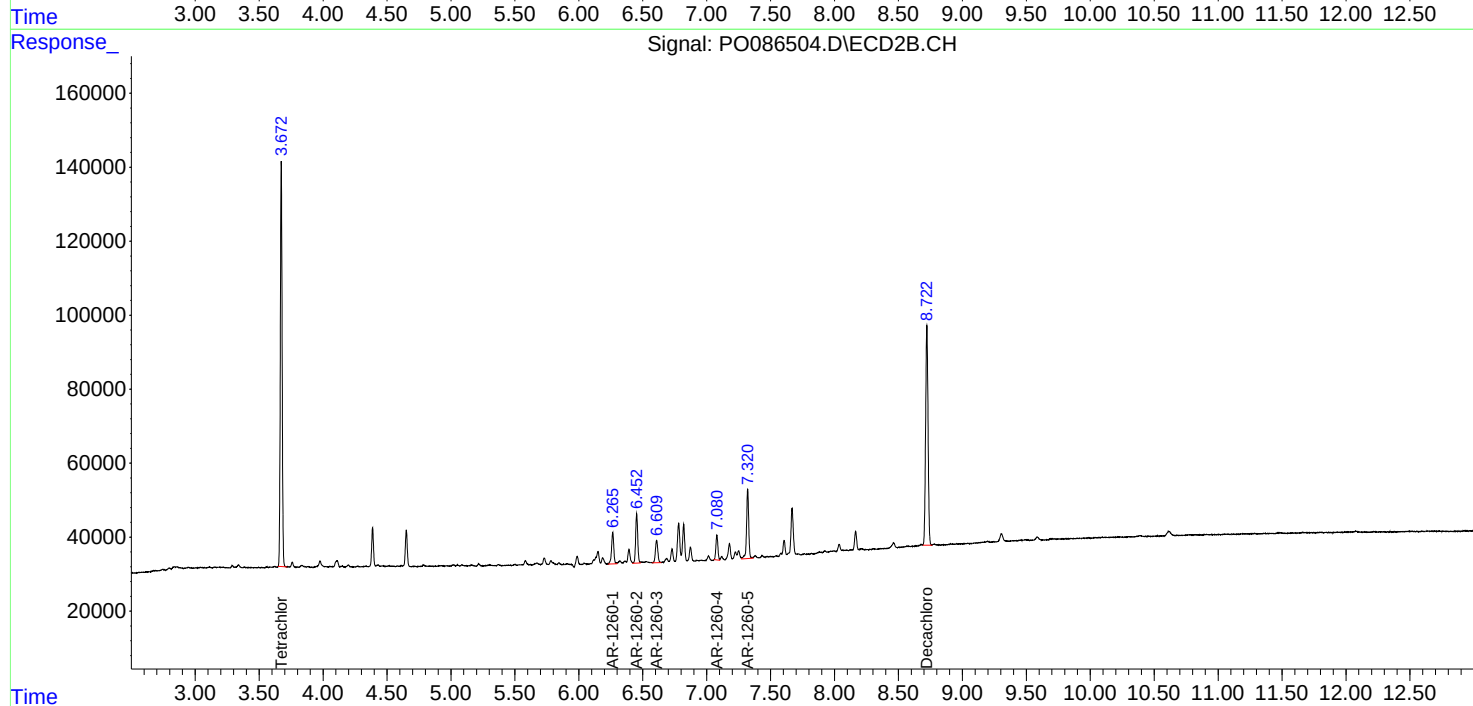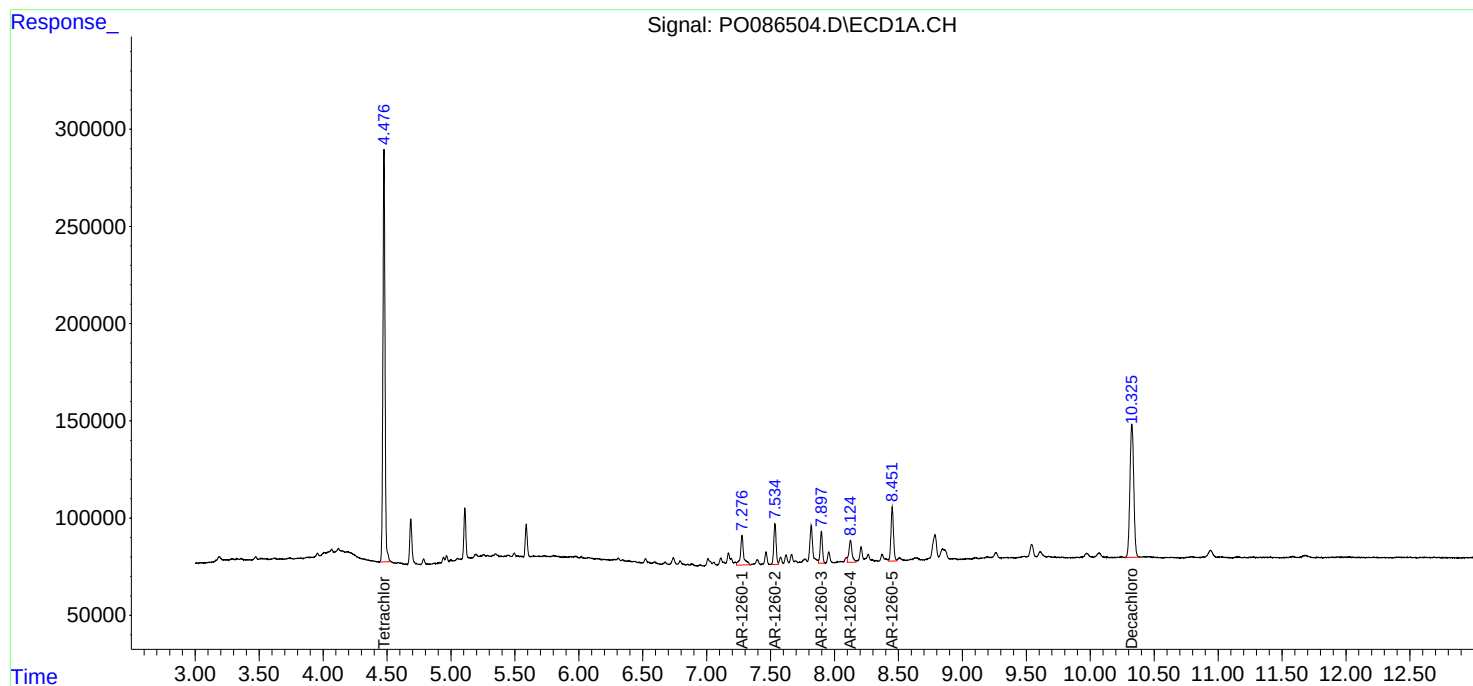

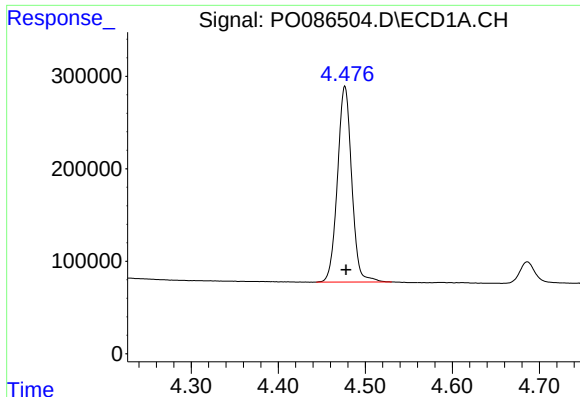


#1 Tetrachloro-m-xylene

R.T.: 4.477 min
Delta R.T.: -0.001 min
Response: 2409520
Conc: 23.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
P038-SS001-0006-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/25/2022
Supervised By :Ankita Jodhani 05/25/2022

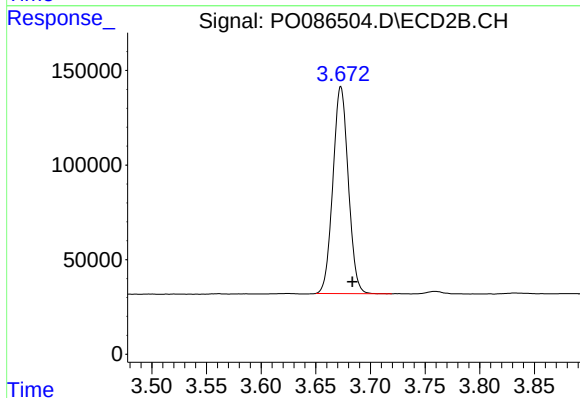


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: -0.010 min
Response: 1071509
Conc: 24.60 ng/ml

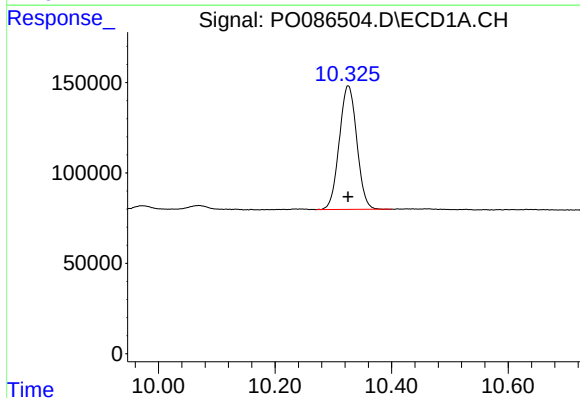


#2 Decachlorobiphenyl

R.T.: 10.326 min
Delta R.T.: 0.000 min
Response: 1428921
Conc: 26.32 ng/ml

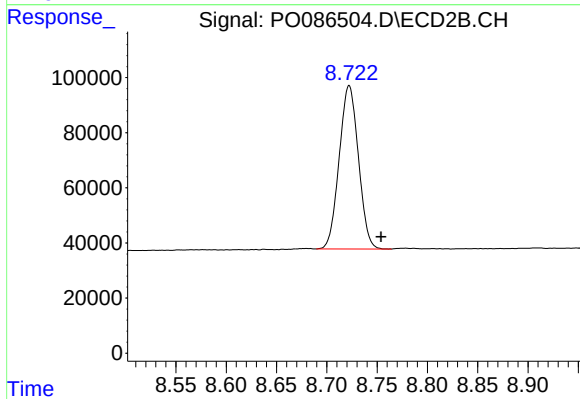

#2 Decachlorobiphenyl

R.T.: 8.722 min
Delta R.T.: -0.032 min
Response: 788623
Conc: 22.66 ng/ml

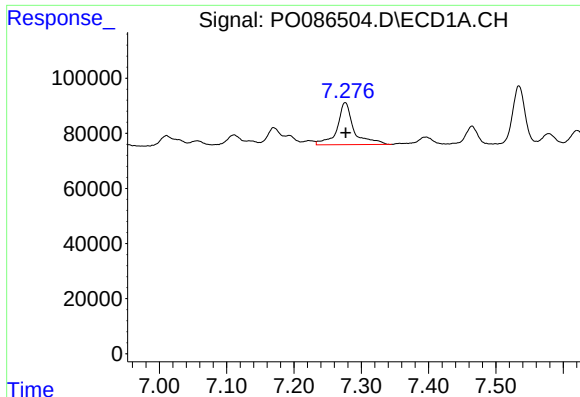


#31 AR-1260-1

R.T.: 7.276 min
Delta R.T.: 0.000 min
Response: 263406
Conc: 87.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
P038-SS001-0006-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/25/2022
Supervised By :Ankita Jodhani 05/25/2022

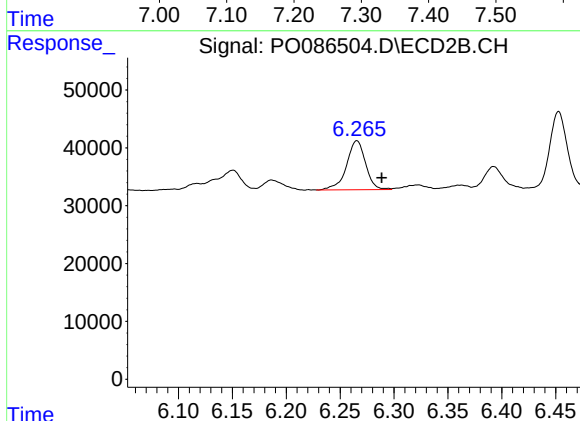


#31 AR-1260-1

R.T.: 6.266 min
Delta R.T.: -0.023 min
Response: 103845
Conc: 53.35 ng/ml

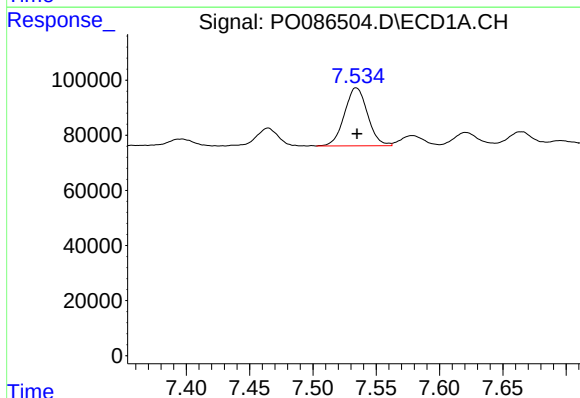


#32 AR-1260-2

R.T.: 7.534 min
Delta R.T.: 0.000 min
Response: 268416
Conc: 74.20 ng/ml

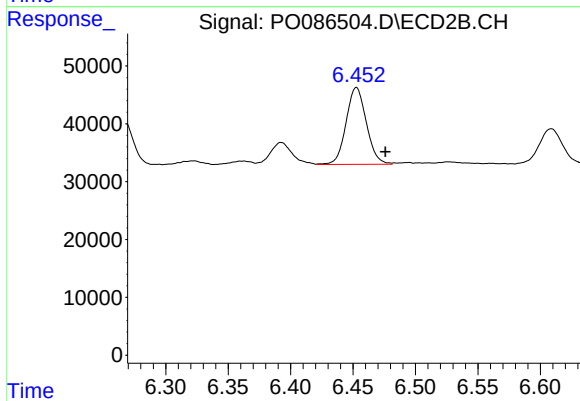

#32 AR-1260-2

R.T.: 6.453 min
Delta R.T.: -0.023 min
Response: 150447
Conc: 64.01 ng/ml

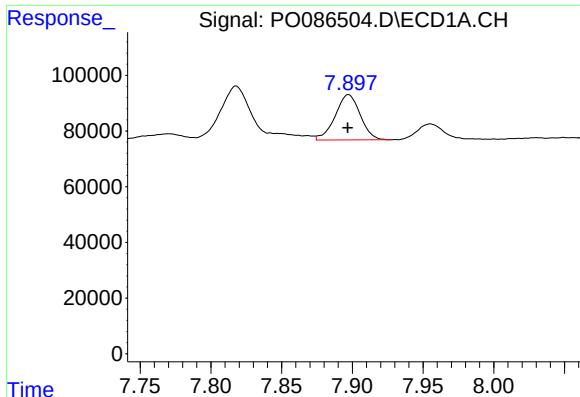


#33 AR-1260-3

R.T.: 7.897 min
Delta R.T.: 0.000 min
Response: 199872
Conc: 72.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
P038-SS001-0006-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/25/2022
Supervised By :Ankita Jodhani 05/25/2022

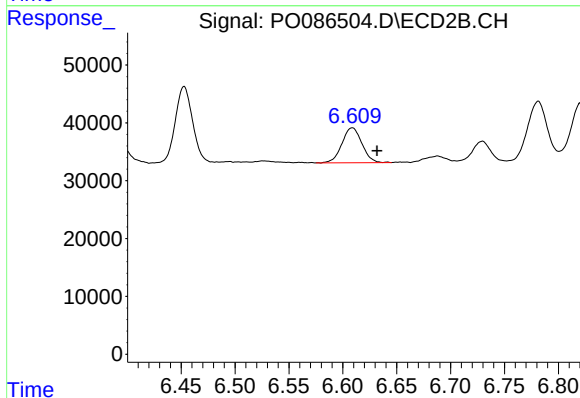


#33 AR-1260-3

R.T.: 6.609 min
Delta R.T.: -0.023 min
Response: 78124
Conc: 36.33 ng/ml

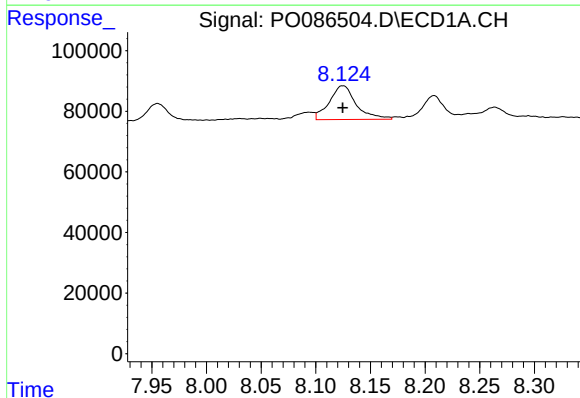


#34 AR-1260-4

R.T.: 8.125 min
Delta R.T.: 0.000 min
Response: 191587
Conc: 56.78 ng/ml

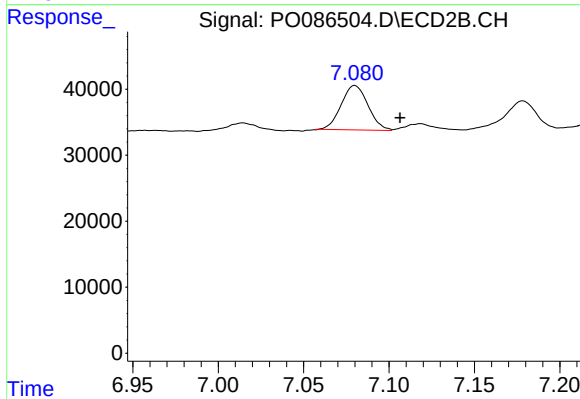

#34 AR-1260-4

R.T.: 7.080 min
Delta R.T.: -0.027 min
Response: 73737
Conc: 40.95 ng/ml m

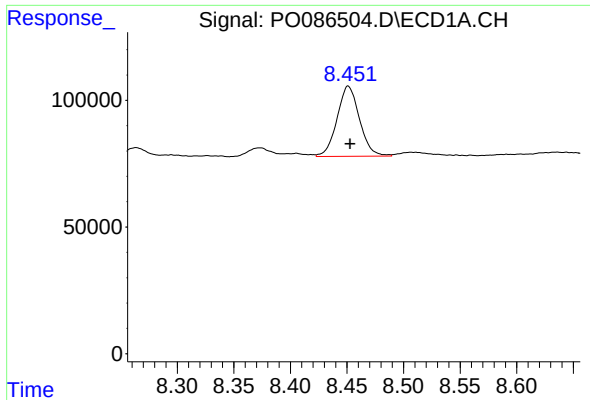


#35 AR-1260-5

R.T.: 8.451 min
Delta R.T.: -0.002 min
Response: 382535
Conc: 61.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
P038-SS001-0006-01

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/25/2022
Supervised By :Ankita Jodhani 05/25/2022

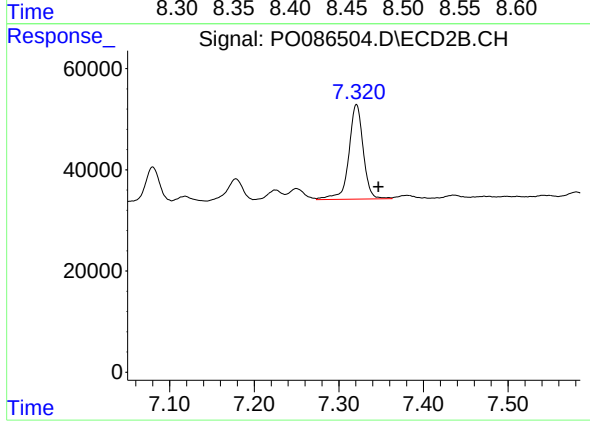

#35 AR-1260-5

R.T.: 7.321 min
Delta R.T.: -0.026 min
Response: 220467
Conc: 50.89 ng/ml