

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052422\
 Data File : P0086519.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 May 2022 1:27
 Operator : YP\AJ
 Sample : N2896-19
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 P040-SS001-1218-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/25/2022
 Supervised By :Ankita Jodhani 05/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 02:46:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 19 09:06:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.476	3.672	2558965	1073924	25.185	24.655
2) SA Decachlor...	10.328	8.721	1229630	656742	22.646m	18.872
Target Compounds						
31) L7 AR-1260-1	7.276	6.265	122997	65816	40.641	33.816
32) L7 AR-1260-2	7.534	6.452	253699	132875	70.131	56.535m
33) L7 AR-1260-3	7.897	6.609	207247	58460	75.090	27.187 #
34) L7 AR-1260-4	8.124	7.078	154428	70994	45.770m	39.427m
35) L7 AR-1260-5	8.453	7.320	410038	271210	66.449	62.609

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052422\
Data File : P0086519.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 May 2022 1:27
Operator : YP\AJ
Sample : N2896-19
Misc :
ALS Vial : 53 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
P040-SS001-1218-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/25/2022
Supervised By :Ankita Jodhani 05/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 02:46:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 19 09:06:34 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

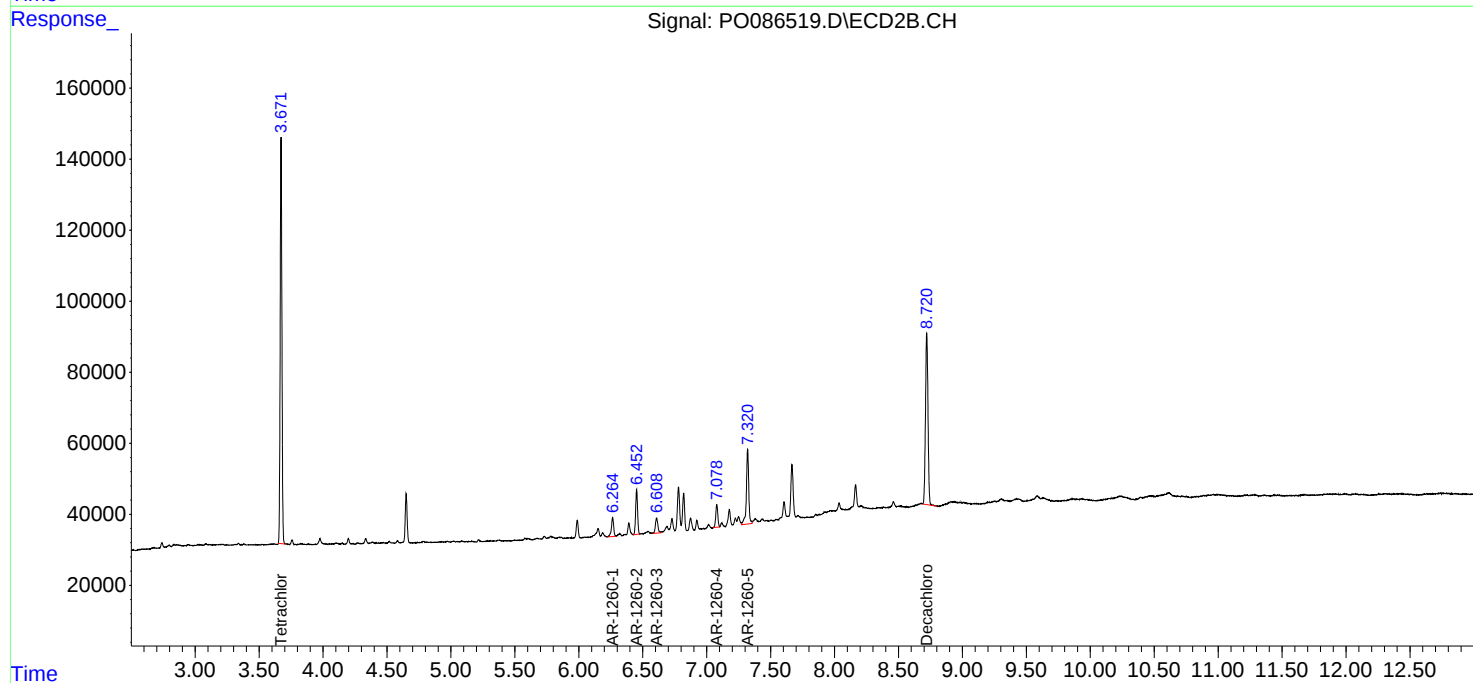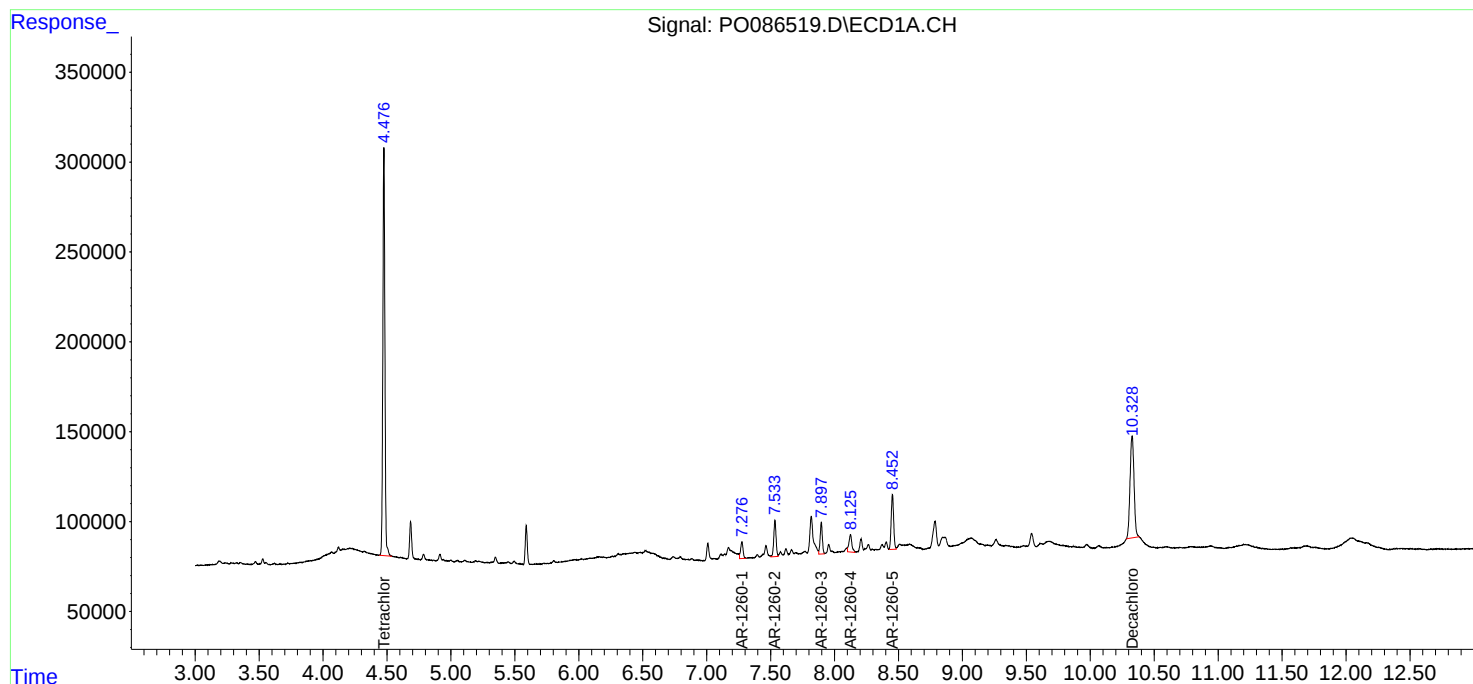

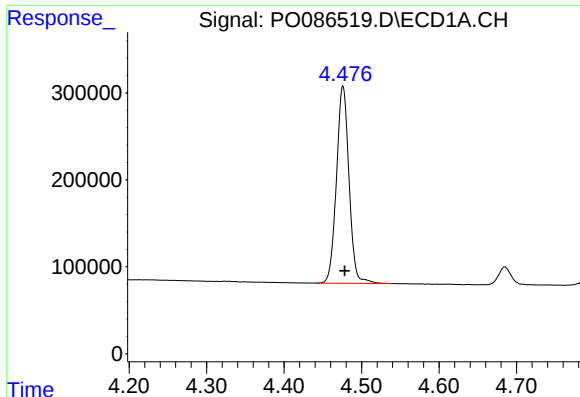


#1 Tetrachloro-m-xylene

R.T.: 4.476 min
Delta R.T.: -0.002 min
Response: 2558965
Conc: 25.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
P040-SS001-1218-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/25/2022
Supervised By :Ankita Jodhani 05/25/2022

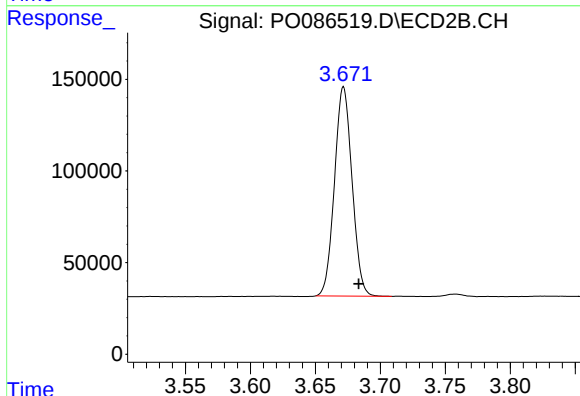


#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: -0.012 min
Response: 1073924
Conc: 24.66 ng/ml

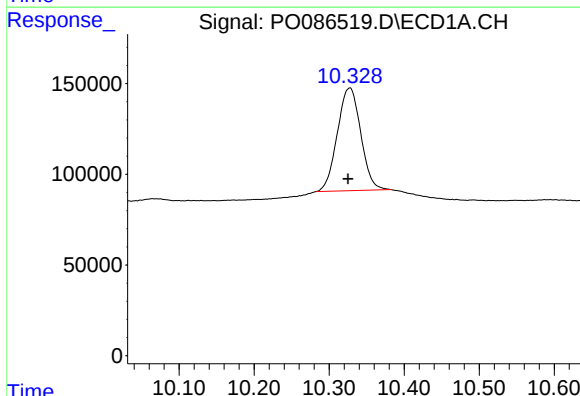


#2 Decachlorobiphenyl

R.T.: 10.328 min
Delta R.T.: 0.003 min
Response: 1229630
Conc: 22.65 ng/ml m

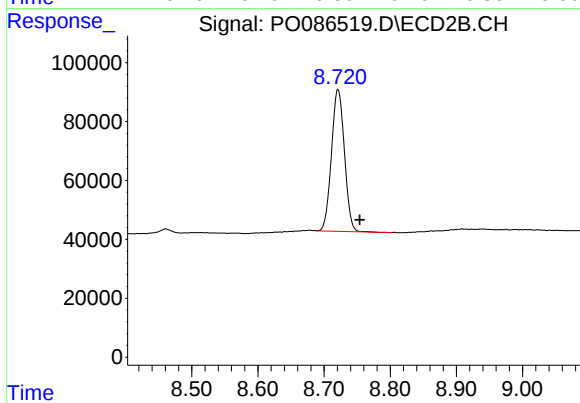

#2 Decachlorobiphenyl

R.T.: 8.721 min
Delta R.T.: -0.033 min
Response: 656742
Conc: 18.87 ng/ml

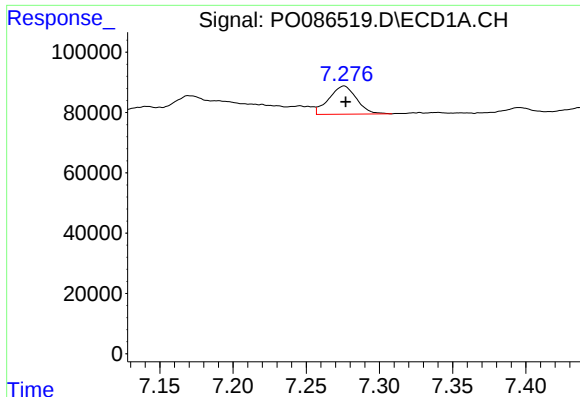


#31 AR-1260-1

R.T.: 7.276 min
Delta R.T.: -0.001 min
Response: 122997
Conc: 40.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
P040-SS001-1218-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/25/2022
Supervised By :Ankita Jodhani 05/25/2022

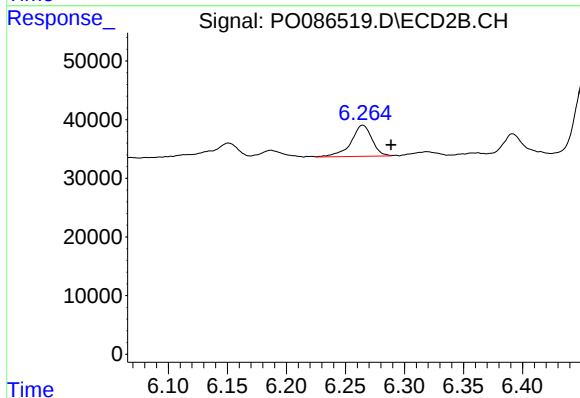


#31 AR-1260-1

R.T.: 6.265 min
Delta R.T.: -0.024 min
Response: 65816
Conc: 33.82 ng/ml

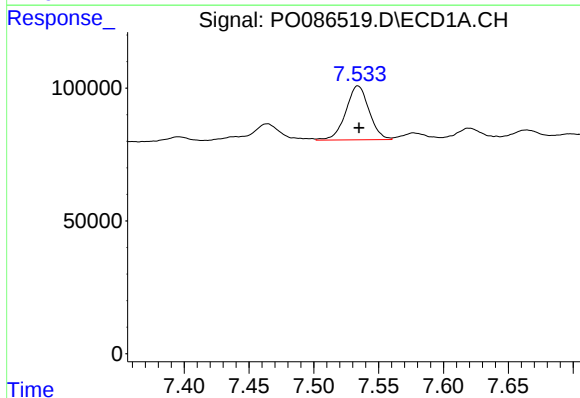


#32 AR-1260-2

R.T.: 7.534 min
Delta R.T.: 0.000 min
Response: 253699
Conc: 70.13 ng/ml

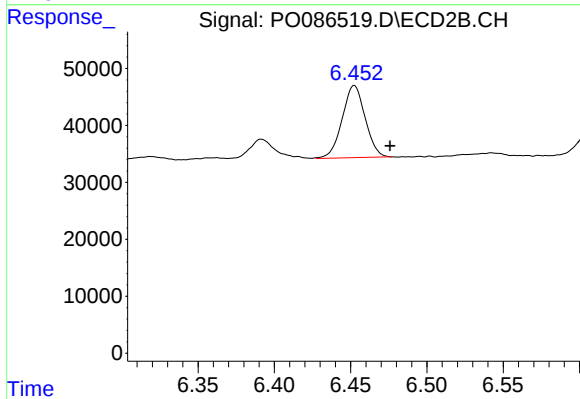

#32 AR-1260-2

R.T.: 6.452 min
Delta R.T.: -0.024 min
Response: 132875
Conc: 56.53 ng/ml m

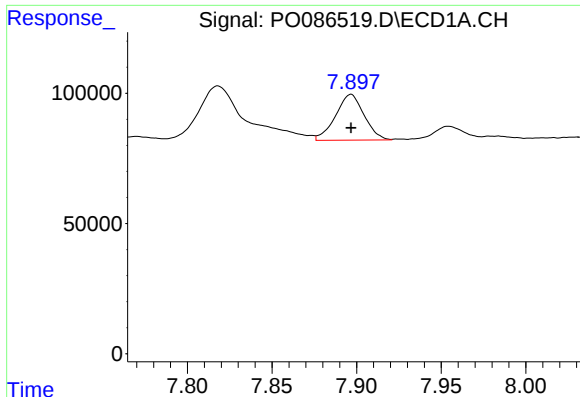


#33 AR-1260-3

R.T.: 7.897 min
Delta R.T.: 0.000 min
Response: 207247
Conc: 75.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
P040-SS001-1218-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/25/2022
Supervised By :Ankita Jodhani 05/25/2022

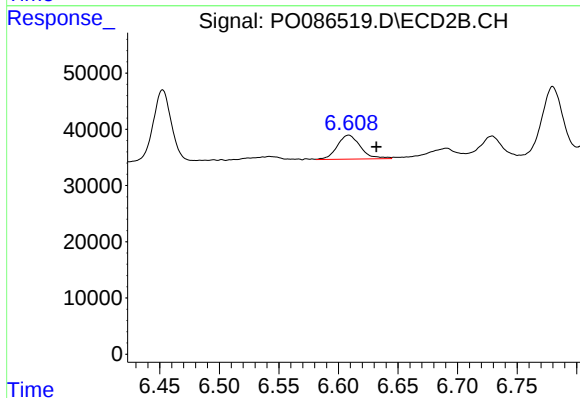


#33 AR-1260-3

R.T.: 6.609 min
Delta R.T.: -0.023 min
Response: 58460
Conc: 27.19 ng/ml

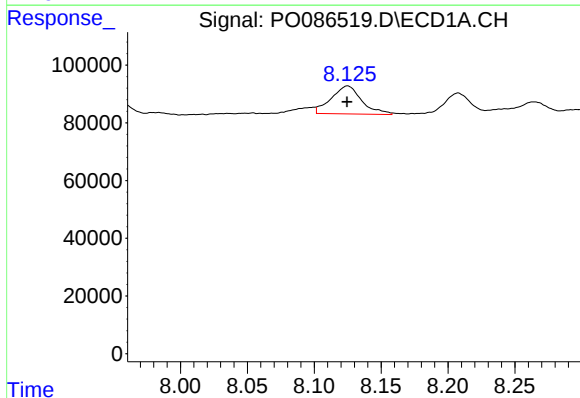


#34 AR-1260-4

R.T.: 8.124 min
Delta R.T.: 0.000 min
Response: 154428
Conc: 45.77 ng/ml m

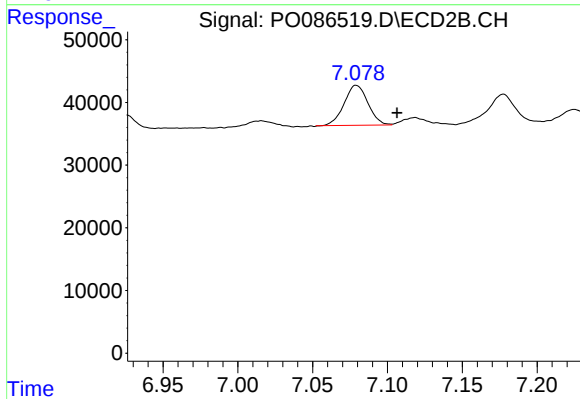

#34 AR-1260-4

R.T.: 7.078 min
Delta R.T.: -0.028 min
Response: 70994
Conc: 39.43 ng/ml m

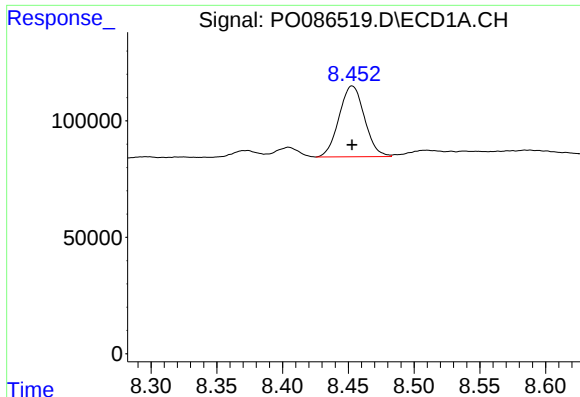


#35 AR-1260-5

R.T.: 8.453 min
Delta R.T.: 0.000 min
Response: 410038
Conc: 66.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
P040-SS001-1218-01

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/25/2022
Supervised By :Ankita Jodhani 05/25/2022

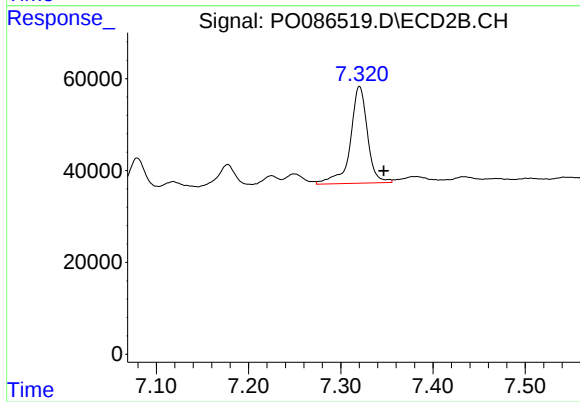

#35 AR-1260-5

R.T.: 7.320 min
Delta R.T.: -0.026 min
Response: 271210
Conc: 62.61 ng/ml