

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052422\
 Data File : P0086523.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 May 2022 3:03
 Operator : YP\AJ
 Sample : N2896-21
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 P040-SS001-2430-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/25/2022
 Supervised By :Ankita Jodhani 05/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 06:30:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 19 09:06:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.477	3.673	2129659	858786	20.960	19.716
2) SA Decachlor...	10.326	8.720	716185	395921	13.190	11.377
Target Compounds						
31) L7 AR-1260-1	7.276	6.264	133449	71734	44.095	36.856
32) L7 AR-1260-2	7.534	6.452	443507	238496	122.601	101.474
33) L7 AR-1260-3	7.897	6.610	749793	85858	271.664	39.929 #
34) L7 AR-1260-4	8.123	7.079	509234	143231	150.929	79.545m#
35) L7 AR-1260-5	8.452	7.320	1074045	668434	174.055	154.308

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052422\
Data File : P0086523.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 May 2022 3:03
Operator : YP\AJ
Sample : N2896-21
Misc :
ALS Vial : 55 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
P040-SS001-2430-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/25/2022
Supervised By :Ankita Jodhani 05/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 06:30:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 19 09:06:34 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

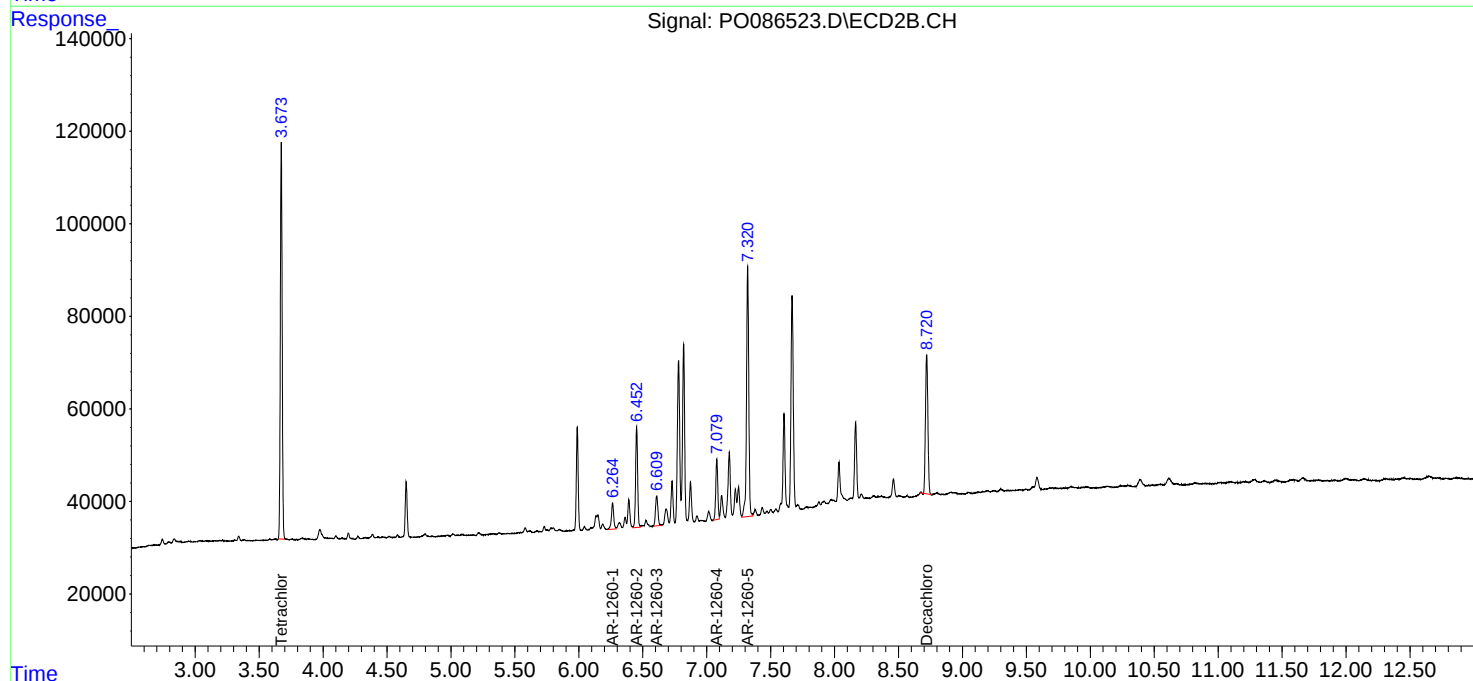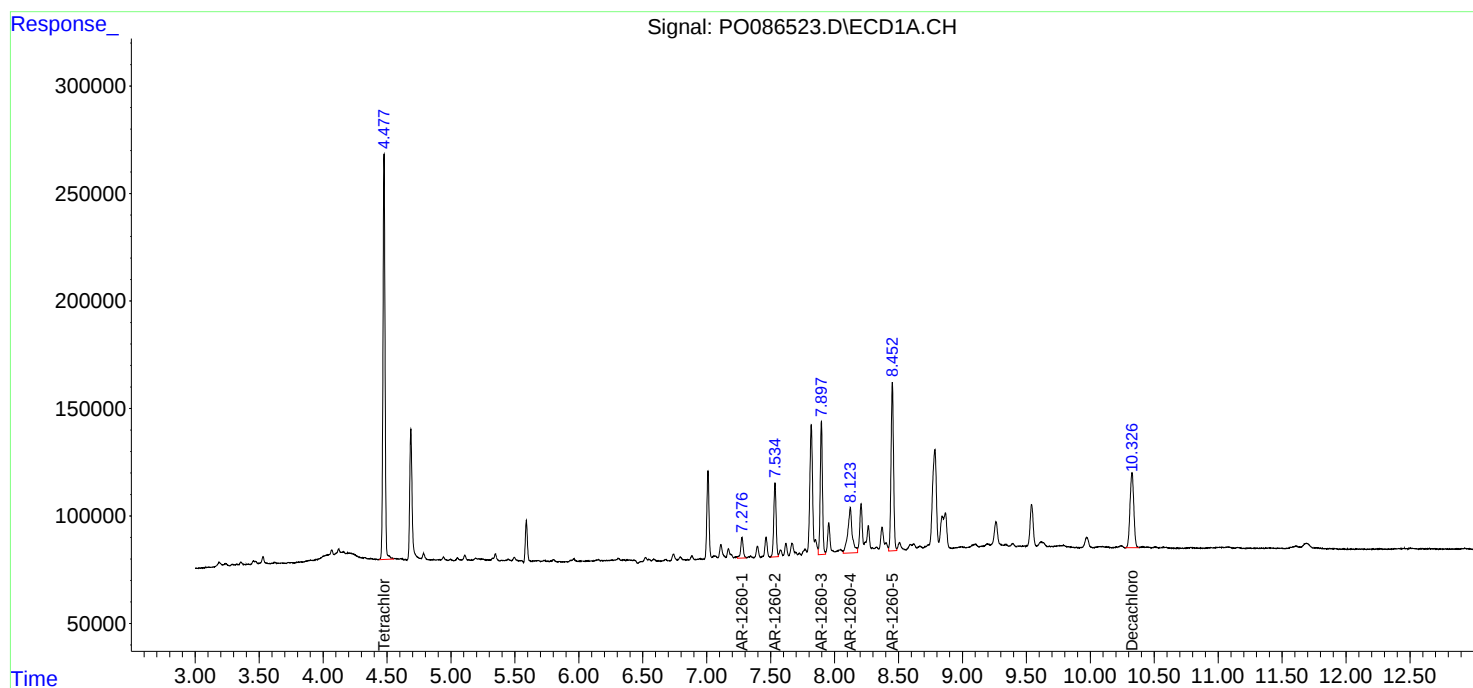

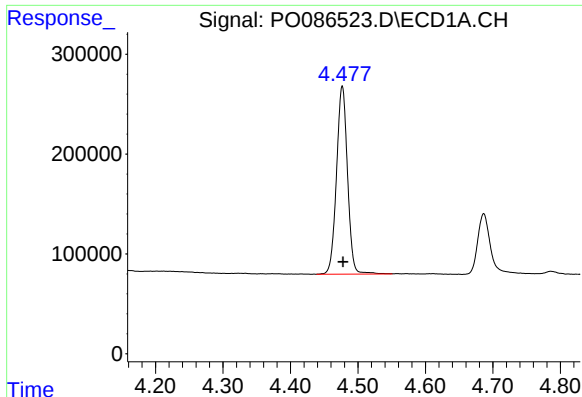


#1 Tetrachloro-m-xylene

R.T.: 4.477 min
Delta R.T.: -0.001 min
Response: 2129659
Conc: 20.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
P040-SS001-2430-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/25/2022
Supervised By :Ankita Jodhani 05/25/2022

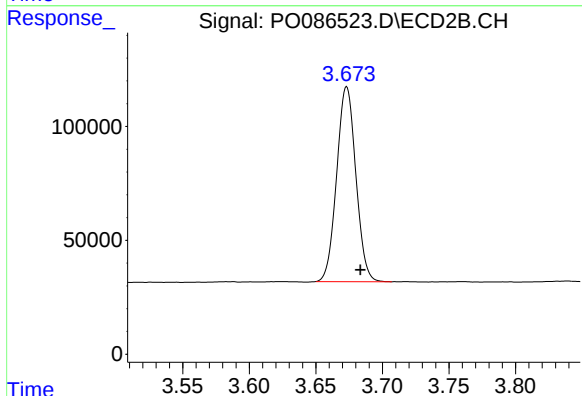


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: -0.010 min
Response: 858786
Conc: 19.72 ng/ml

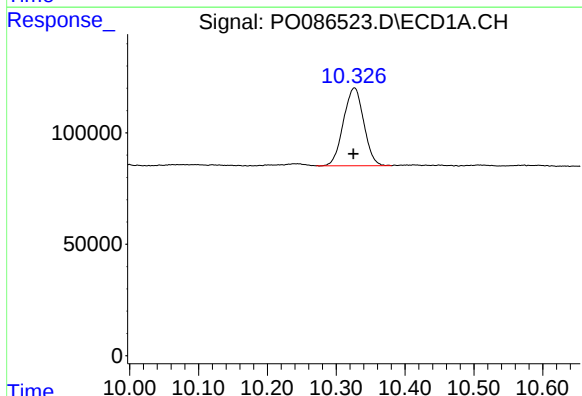


#2 Decachlorobiphenyl

R.T.: 10.326 min
Delta R.T.: 0.001 min
Response: 716185
Conc: 13.19 ng/ml

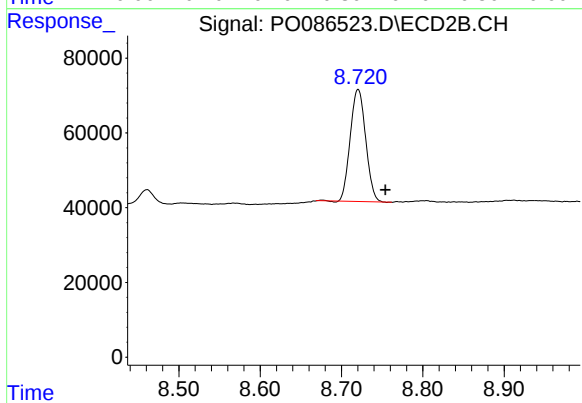

#2 Decachlorobiphenyl

R.T.: 8.720 min
Delta R.T.: -0.033 min
Response: 395921
Conc: 11.38 ng/ml

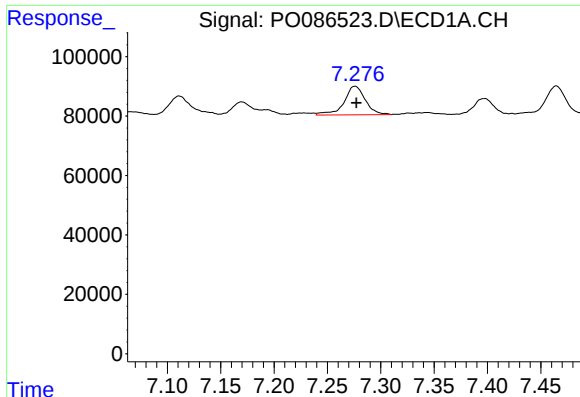


#31 AR-1260-1

R.T.: 7.276 min
Delta R.T.: 0.000 min
Response: 133449
Conc: 44.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
P040-SS001-2430-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/25/2022
Supervised By :Ankita Jodhani 05/25/2022

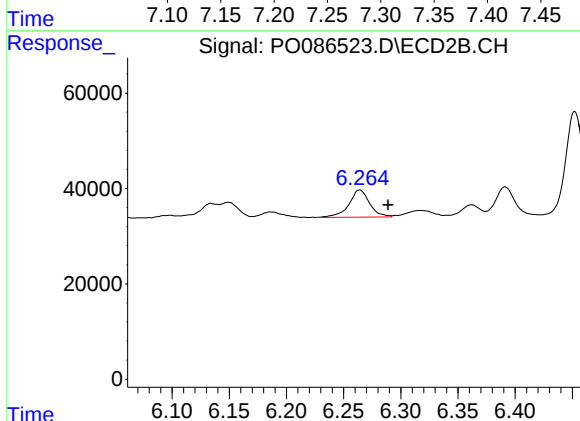


#31 AR-1260-1

R.T.: 6.264 min
Delta R.T.: -0.024 min
Response: 71734
Conc: 36.86 ng/ml

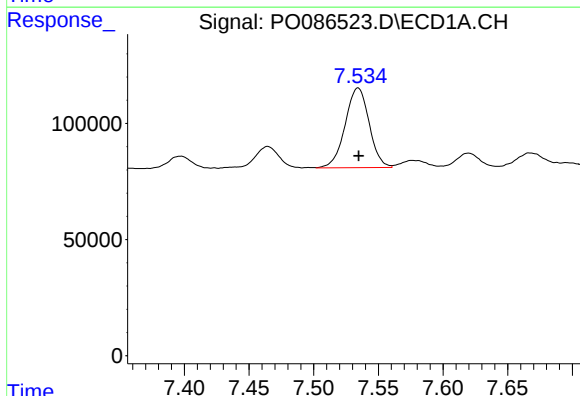


#32 AR-1260-2

R.T.: 7.534 min
Delta R.T.: 0.000 min
Response: 443507
Conc: 122.60 ng/ml

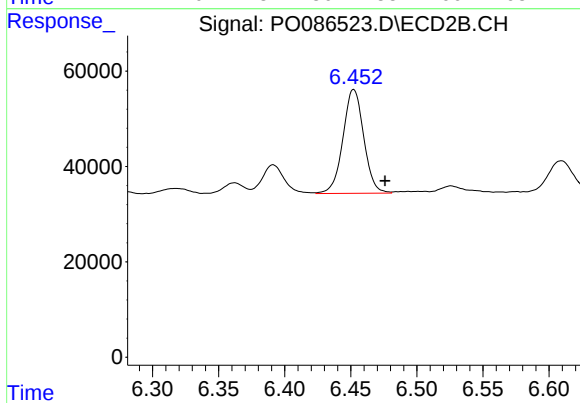

#32 AR-1260-2

R.T.: 6.452 min
Delta R.T.: -0.024 min
Response: 238496
Conc: 101.47 ng/ml

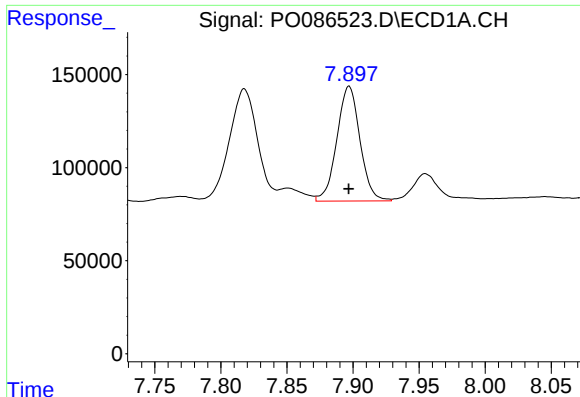


#33 AR-1260-3

R.T.: 7.897 min
Delta R.T.: 0.000 min
Response: 749793
Conc: 271.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
P040-SS001-2430-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/25/2022
Supervised By :Ankita Jodhani 05/25/2022

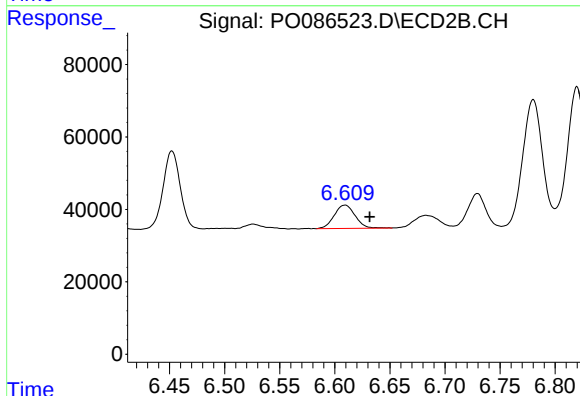


#33 AR-1260-3

R.T.: 6.610 min
Delta R.T.: -0.022 min
Response: 85858
Conc: 39.93 ng/ml

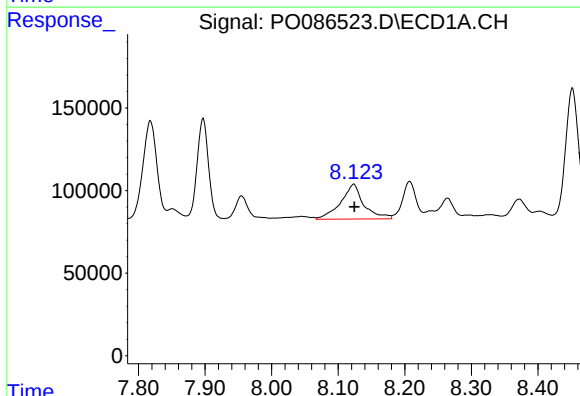


#34 AR-1260-4

R.T.: 8.123 min
Delta R.T.: -0.001 min
Response: 509234
Conc: 150.93 ng/ml

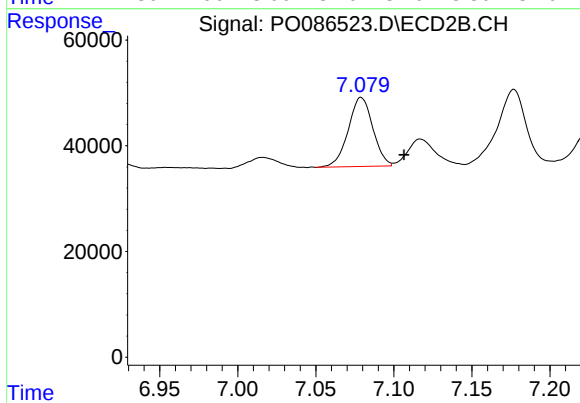

#34 AR-1260-4

R.T.: 7.079 min
Delta R.T.: -0.028 min
Response: 143231
Conc: 79.54 ng/ml m

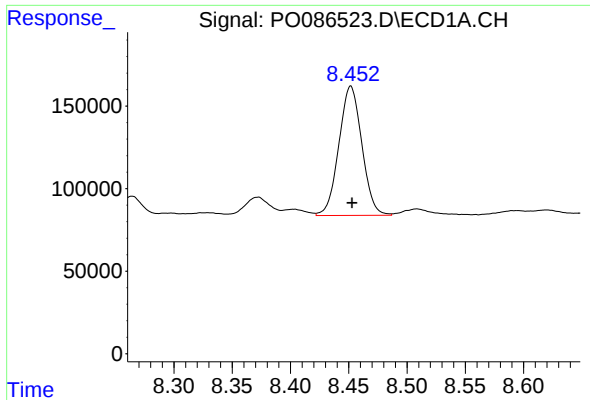


#35 AR-1260-5

R.T.: 8.452 min
Delta R.T.: 0.000 min
Response: 1074045
Conc: 174.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
P040-SS001-2430-01

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/25/2022
Supervised By :Ankita Jodhani 05/25/2022

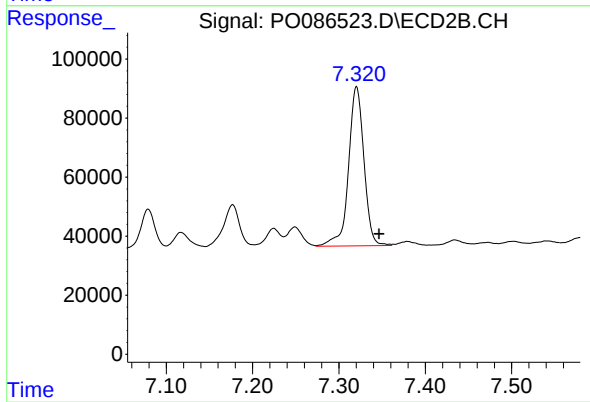

#35 AR-1260-5

R.T.: 7.320 min
Delta R.T.: -0.026 min
Response: 668434
Conc: 154.31 ng/ml