

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052521\
 Data File : P0078142.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 May 2021 15:02
 Operator : DD\AJ
 Sample : PB136626BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 16:56:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.343	3.621	1376301	614096	18.622	20.323
2)	SA Decachlor...	9.957	8.810	1001056	607623	20.248	20.897
Target Compounds							
8)	L2 AR-1221-1	4.588	0.000	139841	0	169.902	N.D. #
9)	L2 AR-1221-2	0.000	3.961	0	11651	N.D.	42.295 #
28)	L6 AR-1254-3	7.150	0.000	38206	0	9.738	N.D. #
30)	L6 AR-1254-5	7.849	6.936	23525	23517	8.044	10.346 #
36)	L8 AR-1262-1	0.000	6.936	0	23517	N.D.	20.042 #
38)	L8 AR-1262-3	8.766f	0.000	11780	0	2.917	N.D. #
39)	L8 AR-1262-4	8.821	0.000	13503	0	4.330	N.D. #
42)	L9 AR-1268-2	8.821	0.000	13503	0	2.087	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052521\
Data File : P0078142.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 May 2021 15:02
Operator : DD\AJ
Sample : PB136626BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 16:56:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

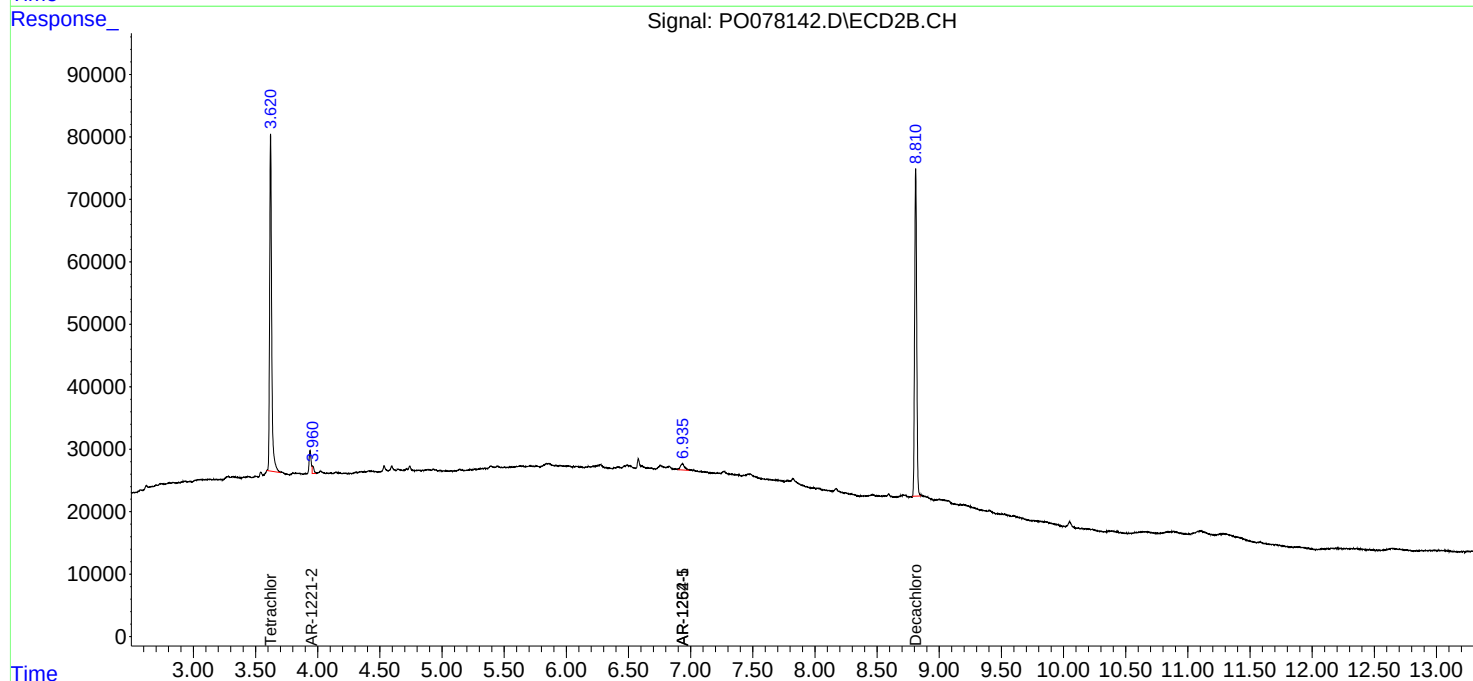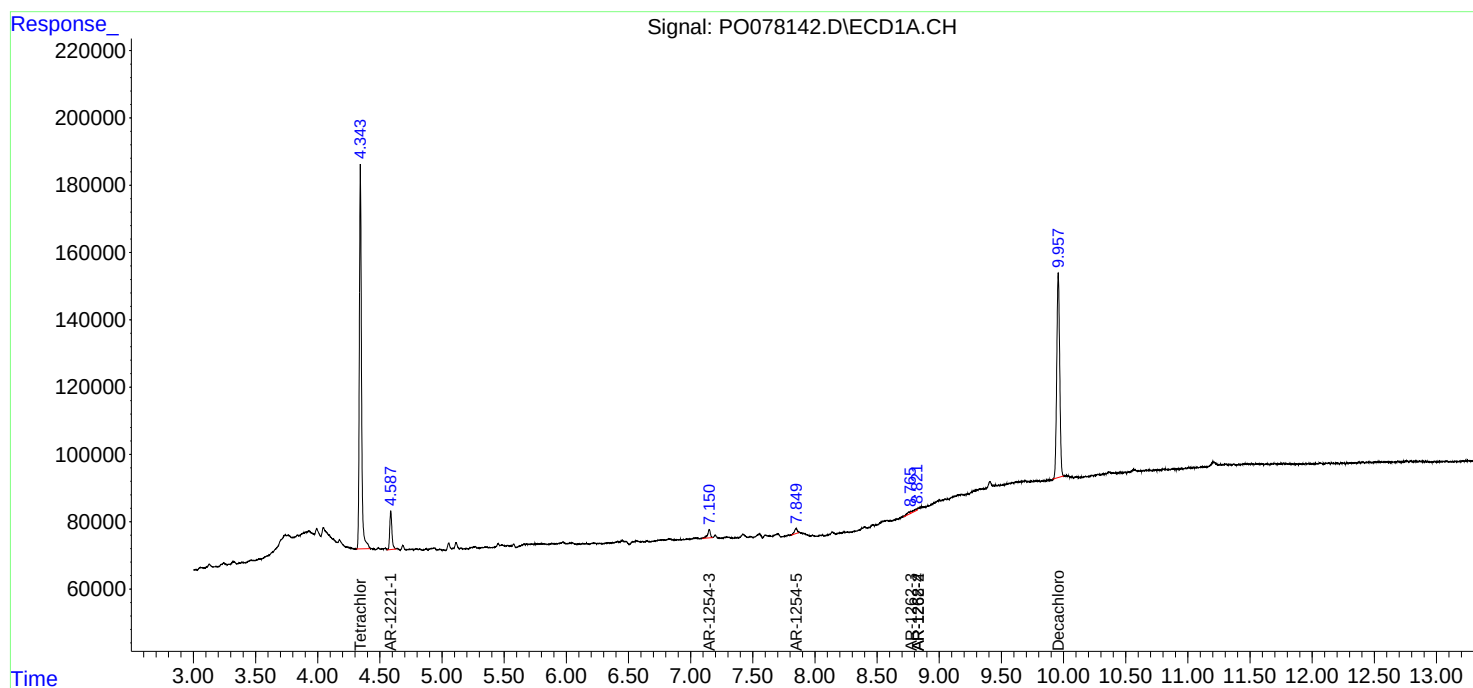


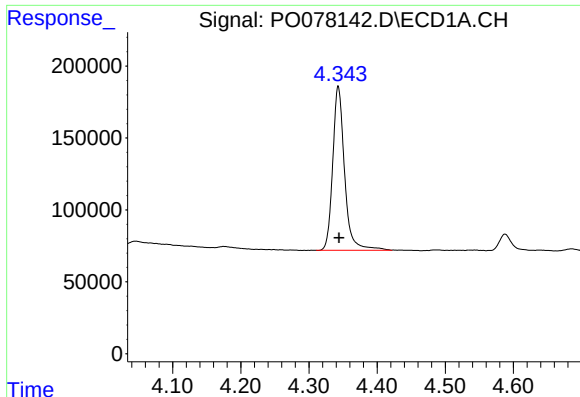

#1 Tetrachloro-m-xylene


R.T.: 4.343 min
Delta R.T.: 0.000 min
Response: 1376301
Conc: 18.62 ng/ml

Instrument :
ECD_O
ClientSampleId :

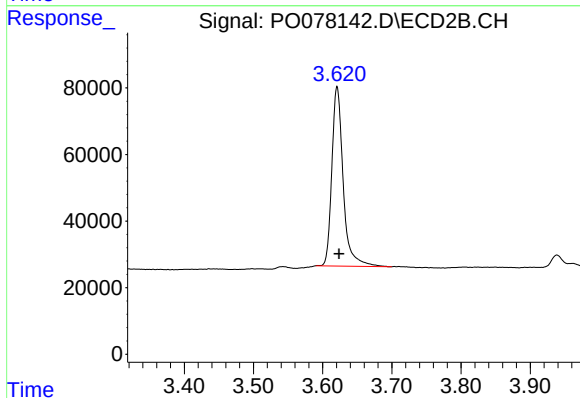


#1 Tetrachloro-m-xylene

R.T.: 3.621 min
Delta R.T.: -0.003 min
Response: 614096
Conc: 20.32 ng/ml

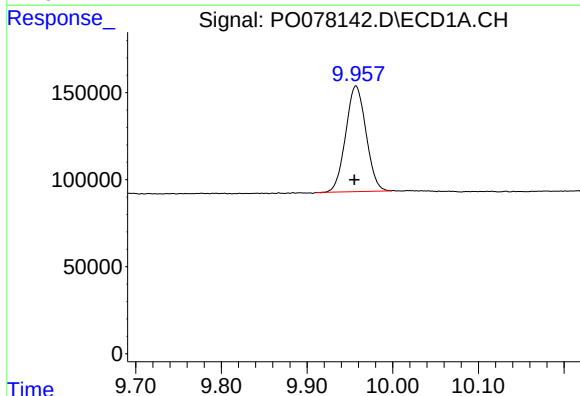


#2 Decachlorobiphenyl

R.T.: 9.957 min
Delta R.T.: 0.002 min
Response: 1001056
Conc: 20.25 ng/ml

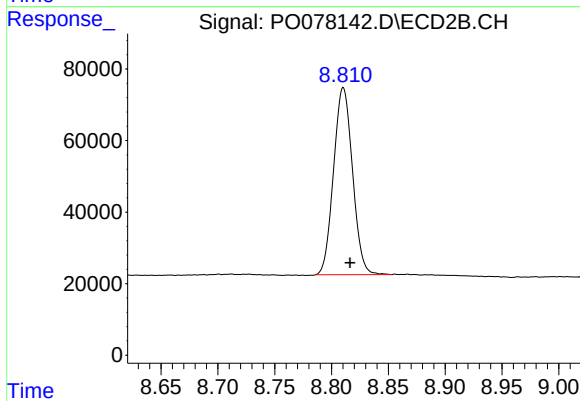

#2 Decachlorobiphenyl


R.T.: 8.810 min
Delta R.T.: -0.006 min
Response: 607623
Conc: 20.90 ng/ml

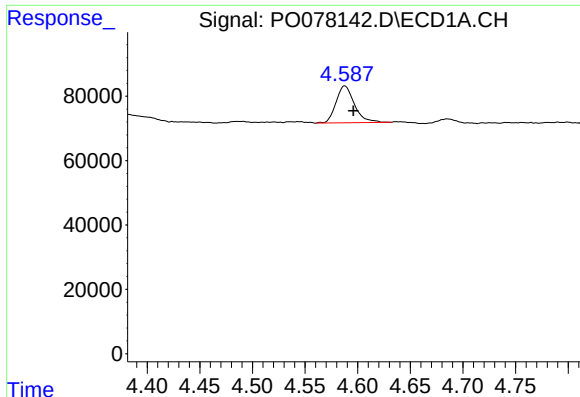

#8 AR-1221-1


R.T.: 4.588 min
Delta R.T.: -0.008 min
Response: 139841
Conc: 169.90 ng/ml

Instrument :
ECD_O
ClientSampleId :

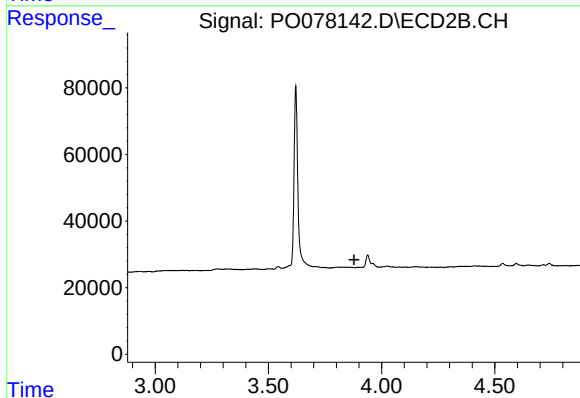


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 3.878 min
Response: 0
Conc: N.D.

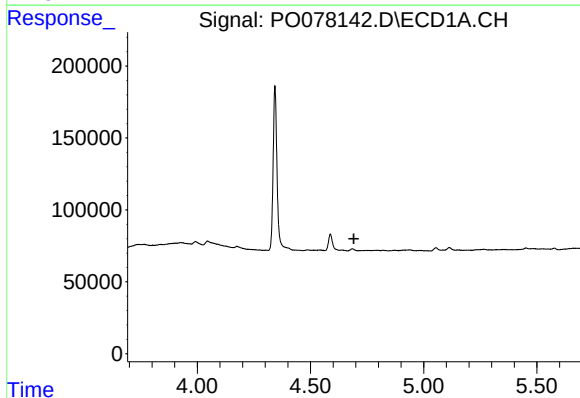


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.691 min
Response: 0
Conc: N.D.

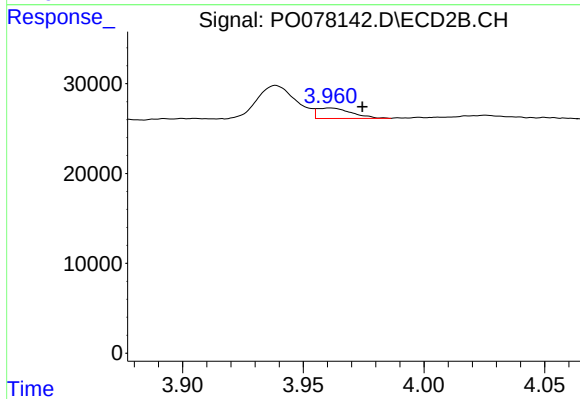

#9 AR-1221-2


R.T.: 3.961 min
Delta R.T.: -0.013 min
Response: 11651
Conc: 42.30 ng/ml

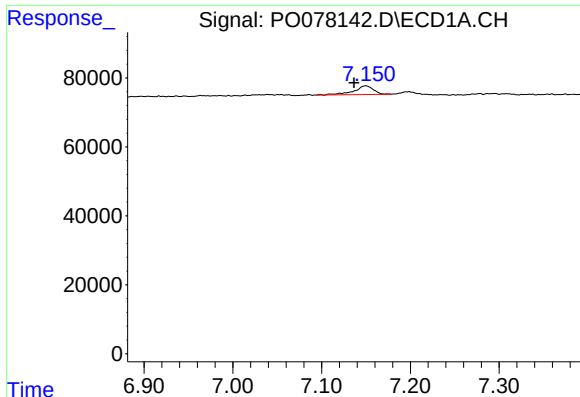

#28 AR-1254-3


R.T.: 7.150 min
Delta R.T.: 0.013 min
Response: 38206
Conc: 9.74 ng/ml

Instrument :
ECD_O
ClientSampleId :

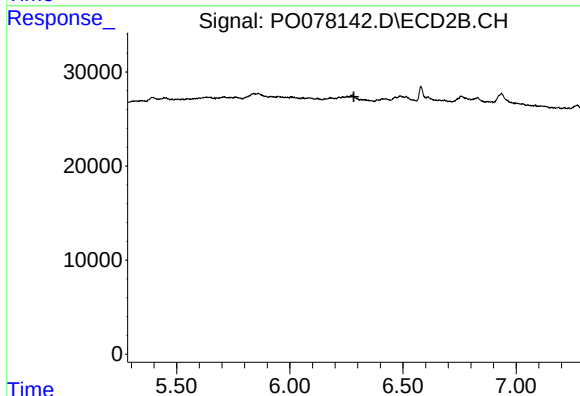


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.283 min
Response: 0
Conc: N.D.

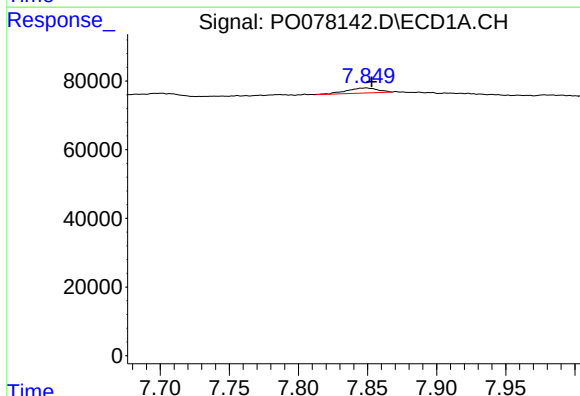


#30 AR-1254-5

R.T.: 7.849 min
Delta R.T.: -0.004 min
Response: 23525
Conc: 8.04 ng/ml

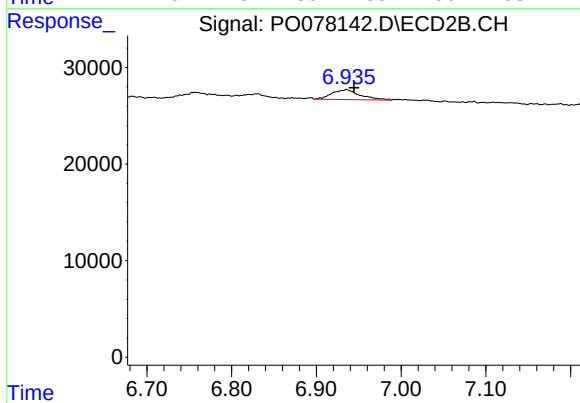

#30 AR-1254-5


R.T.: 6.936 min
Delta R.T.: -0.009 min
Response: 23517
Conc: 10.35 ng/ml

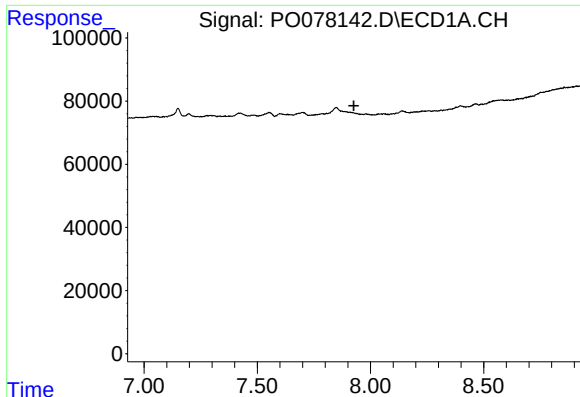

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 7.927 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

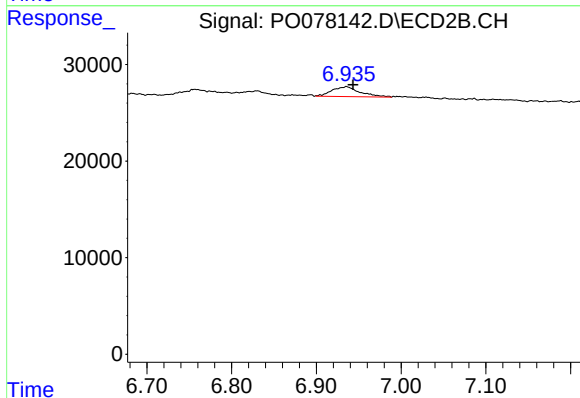


#36 AR-1262-1

R.T.: 6.936 min
Delta R.T.: -0.008 min
Response: 23517
Conc: 20.04 ng/ml

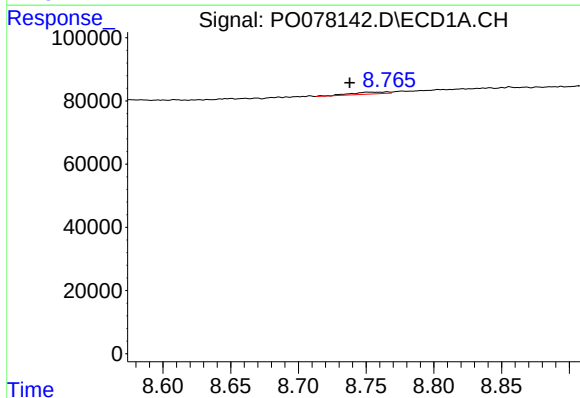


#38 AR-1262-3

R.T.: 8.766 min
Delta R.T.: 0.028 min
Response: 11780
Conc: 2.92 ng/ml

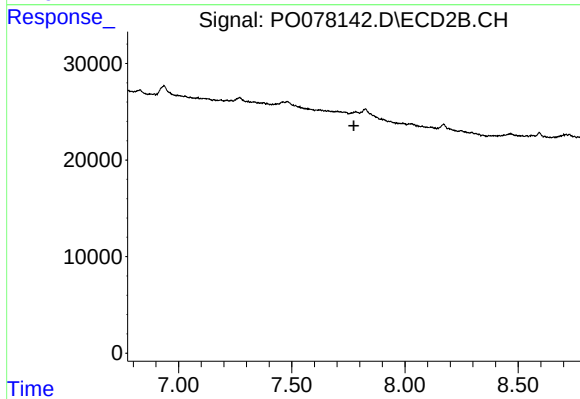

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 7.774 min
Response: 0
Conc: N.D.

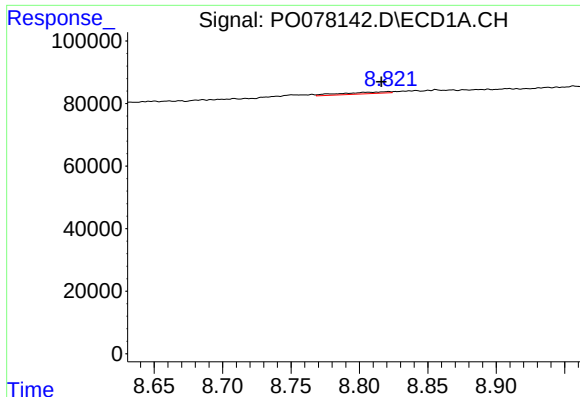

#39 AR-1262-4


R.T.: 8.821 min
Delta R.T.: 0.005 min
Response: 13503
Conc: 4.33 ng/ml

Instrument :
ECD_O
ClientSampleId :

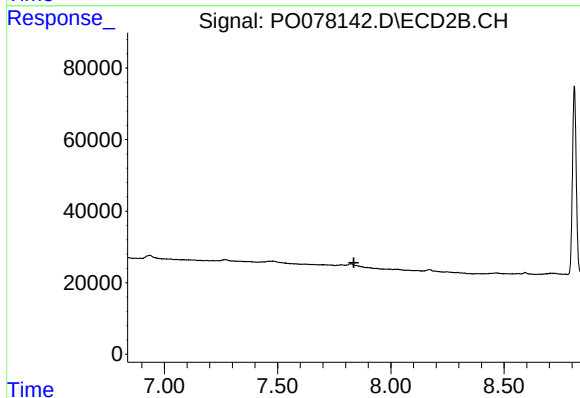


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.837 min
Response: 0
Conc: N.D.

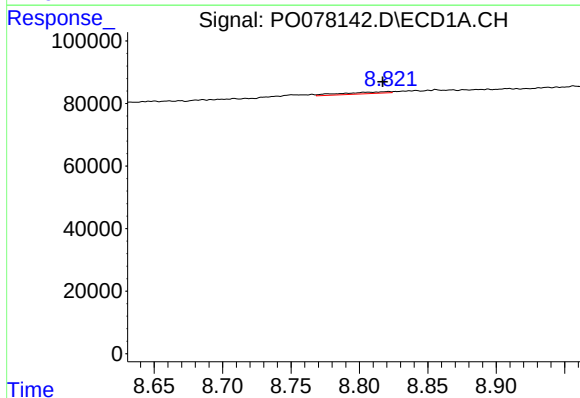

#42 AR-1268-2

R.T.: 8.821 min
Delta R.T.: 0.004 min
Response: 13503
Conc: 2.09 ng/ml

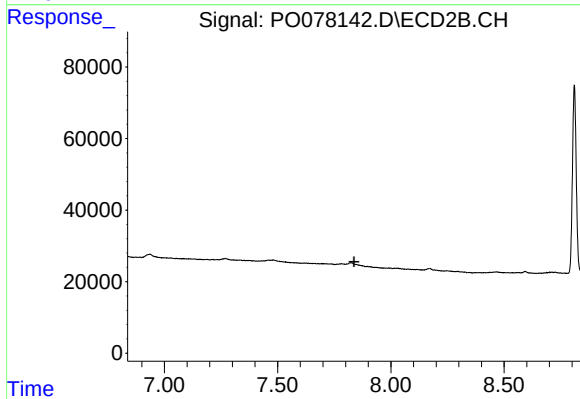

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.837 min
Response: 0
Conc: N.D.