

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0052522\
 Data File : P0086566.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 May 2022 19:08
 Operator : YP\AJ
 Sample : N2895-10
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 P030-SS002-0006-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/26/2022
 Supervised By :Ankita Jodhani 05/26/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 06:46:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 19 09:06:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.477	3.673	2243242	910359	22.078	20.900
2) SA Decachlor...	10.324	8.721	1009221	590285	18.586	16.962
Target Compounds						
31) L7 AR-1260-1	7.276	6.264	72797	38777	24.054	19.923m
32) L7 AR-1260-2	7.535	6.452	353268	188621	97.655	80.253
33) L7 AR-1260-3	7.896	6.607	290980	48805	105.427	22.697 #
34) L7 AR-1260-4	8.126	7.079	209546	77771	62.106m	43.191 #
35) L7 AR-1260-5	8.451	7.320	459514	314626	74.467	72.631

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052522\
Data File : P0086566.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 May 2022 19:08
Operator : YP\AJ
Sample : N2895-10
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
P030-SS002-0006-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 06:46:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 19 09:06:34 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

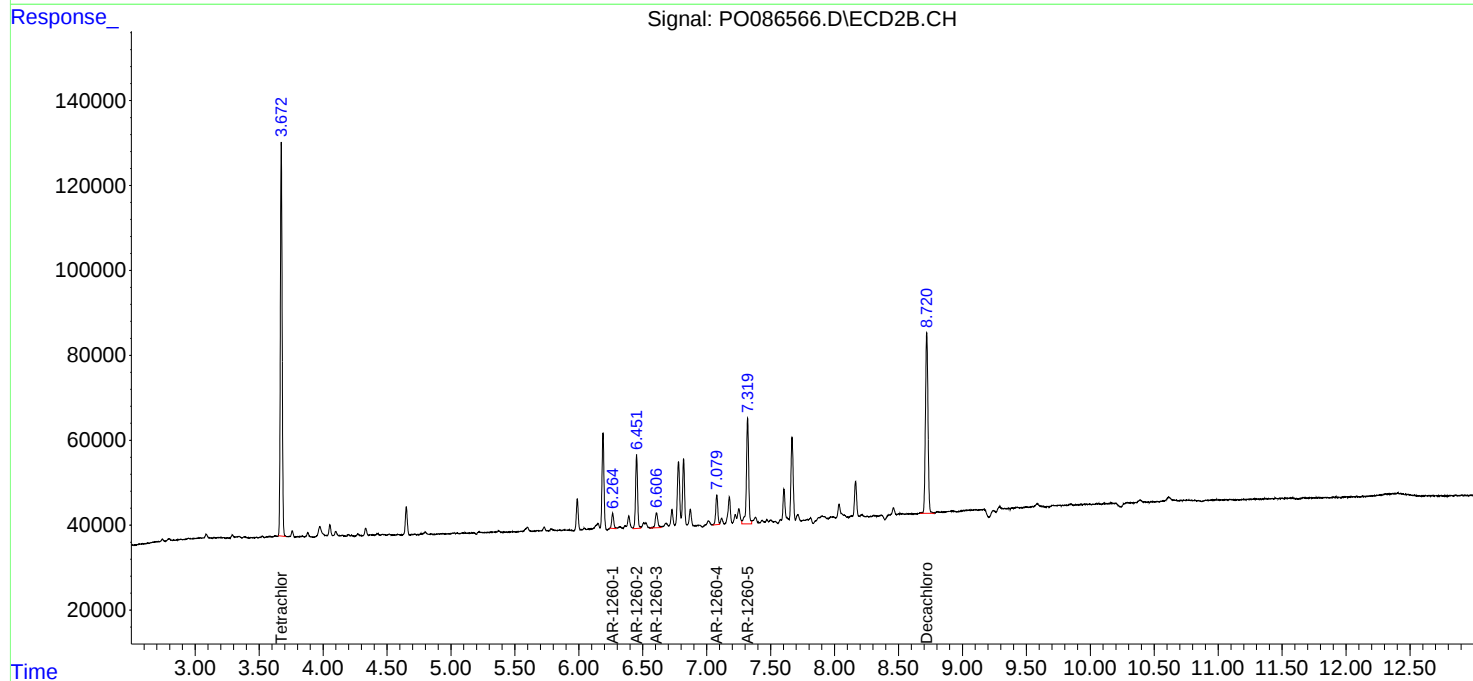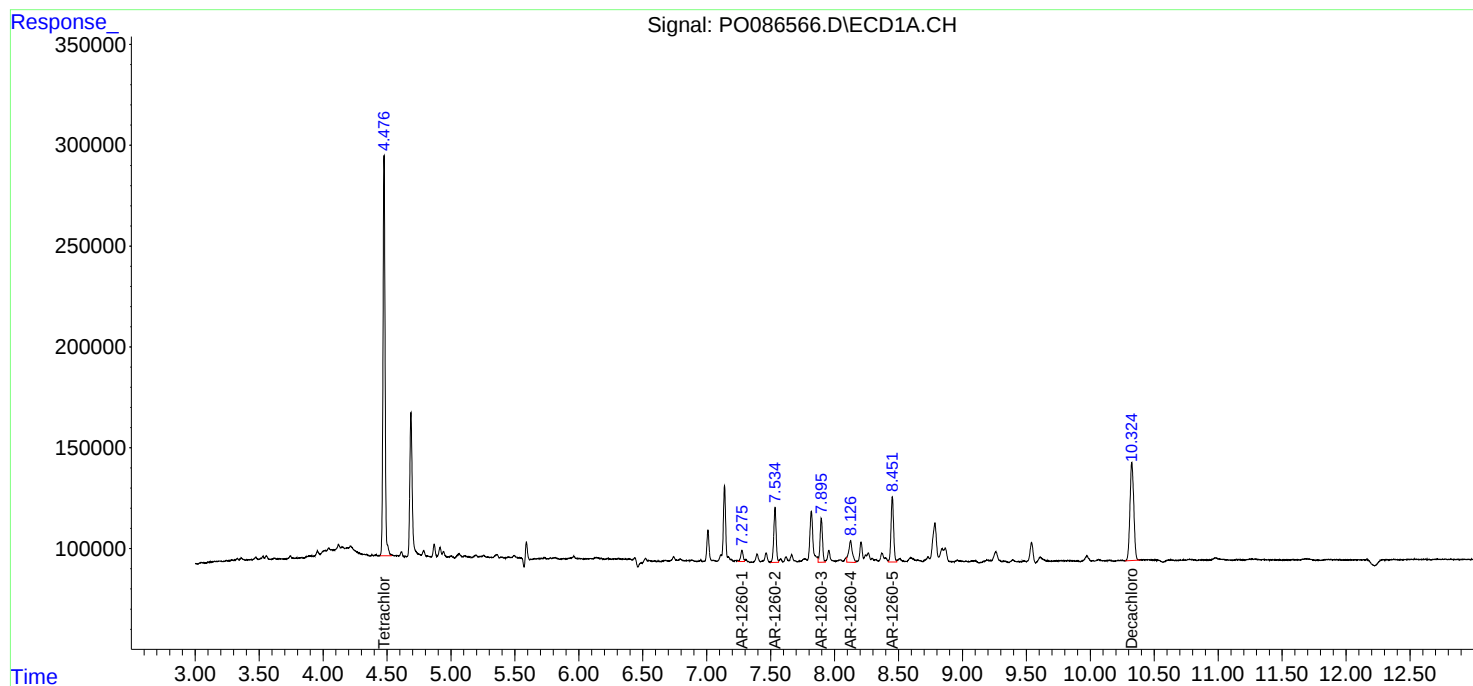

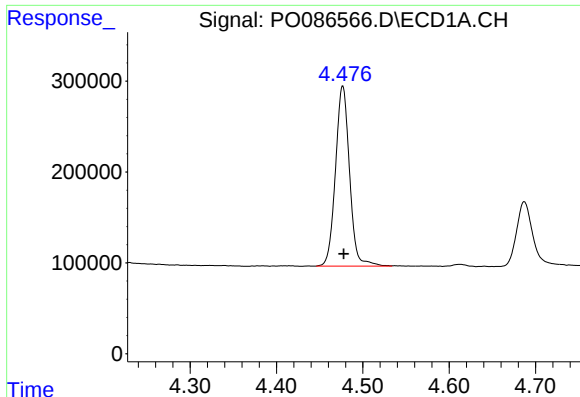


#1 Tetrachloro-m-xylene

R.T.: 4.477 min
Delta R.T.: -0.001 min
Response: 2243242
Conc: 22.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
P030-SS002-0006-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

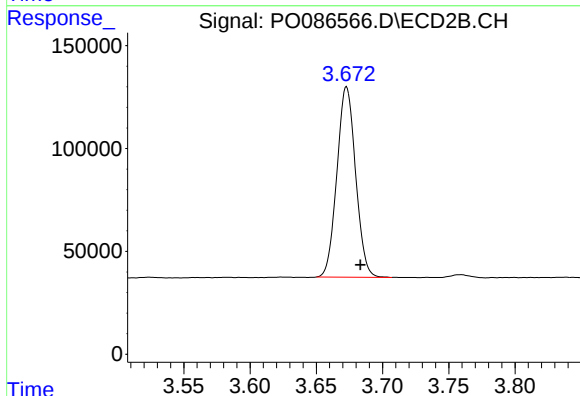


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: -0.010 min
Response: 910359
Conc: 20.90 ng/ml

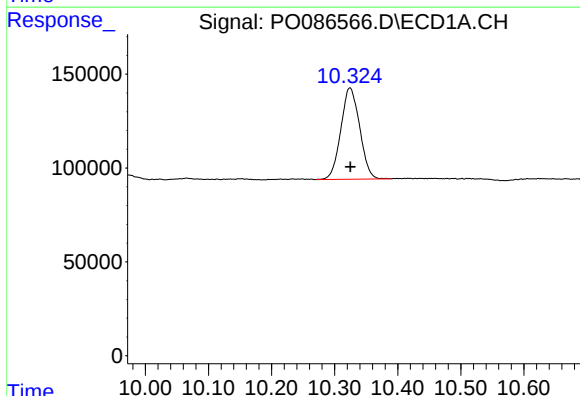


#2 Decachlorobiphenyl

R.T.: 10.324 min
Delta R.T.: 0.000 min
Response: 1009221
Conc: 18.59 ng/ml

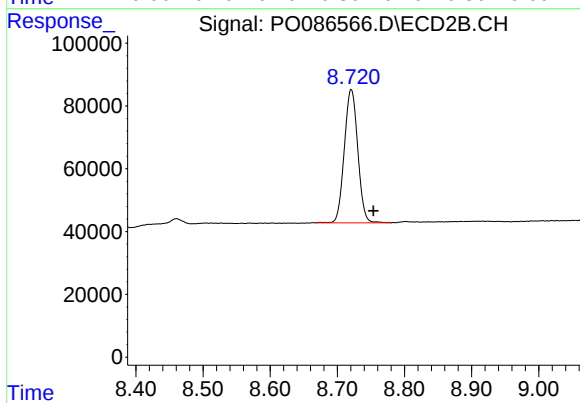

#2 Decachlorobiphenyl

R.T.: 8.721 min
Delta R.T.: -0.033 min
Response: 590285
Conc: 16.96 ng/ml

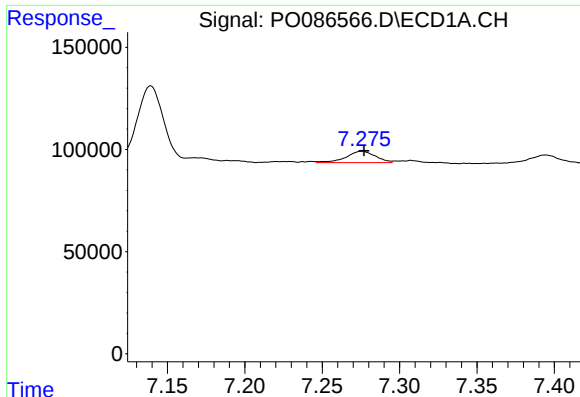


#31 AR-1260-1

R.T.: 7.276 min
Delta R.T.: -0.001 min
Response: 72797
Conc: 24.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
P030-SS002-0006-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

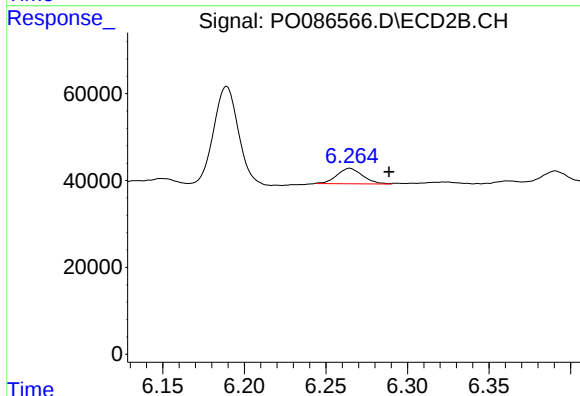


#31 AR-1260-1

R.T.: 6.264 min
Delta R.T.: -0.025 min
Response: 38777
Conc: 19.92 ng/ml m

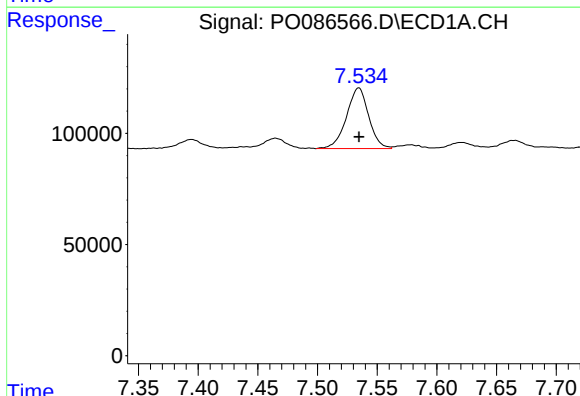


#32 AR-1260-2

R.T.: 7.535 min
Delta R.T.: 0.000 min
Response: 353268
Conc: 97.66 ng/ml

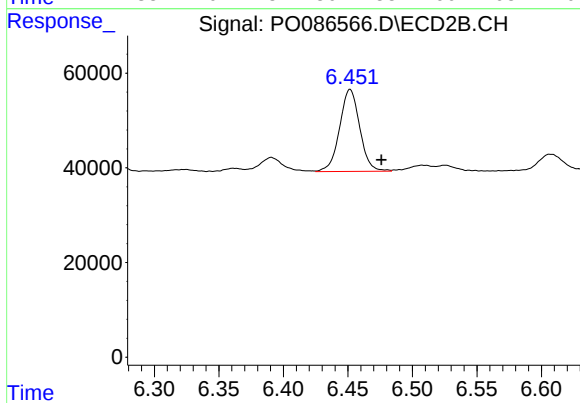

#32 AR-1260-2

R.T.: 6.452 min
Delta R.T.: -0.024 min
Response: 188621
Conc: 80.25 ng/ml

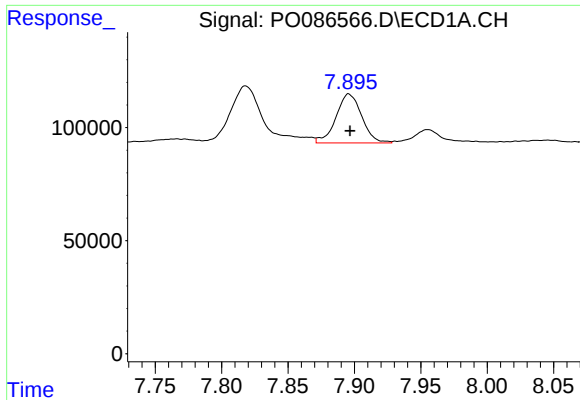


#33 AR-1260-3

R.T.: 7.896 min
Delta R.T.: -0.001 min
Response: 290980
Conc: 105.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
P030-SS002-0006-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

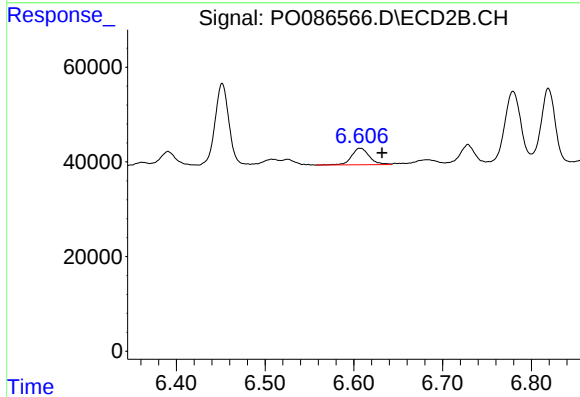


#33 AR-1260-3

R.T.: 6.607 min
Delta R.T.: -0.025 min
Response: 48805
Conc: 22.70 ng/ml

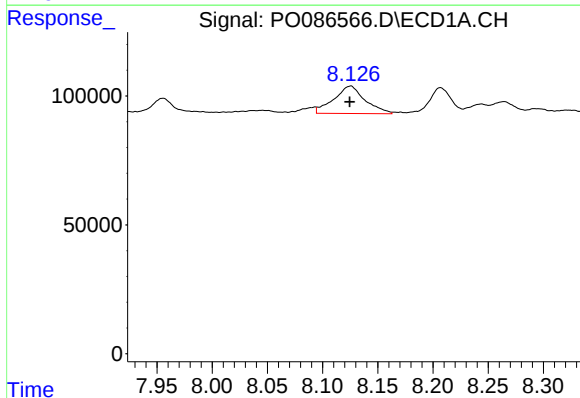


#34 AR-1260-4

R.T.: 8.126 min
Delta R.T.: 0.001 min
Response: 209546
Conc: 62.11 ng/ml m

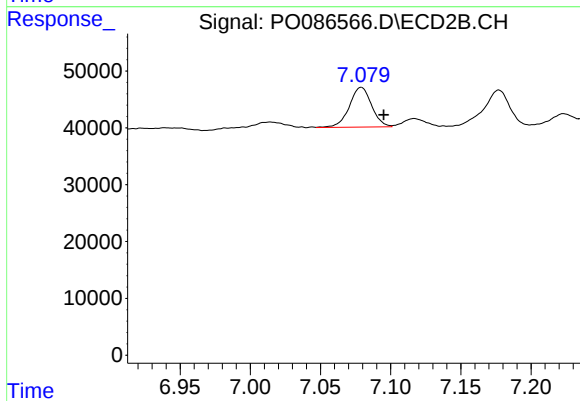

#34 AR-1260-4

R.T.: 7.079 min
Delta R.T.: -0.016 min
Response: 77771
Conc: 43.19 ng/ml

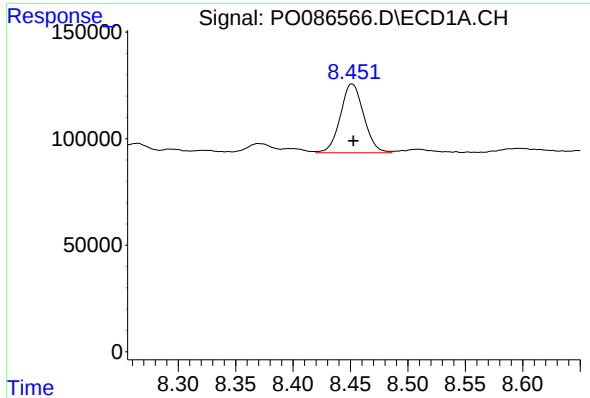


#35 AR-1260-5

R.T.: 8.451 min
Delta R.T.: -0.001 min
Response: 459514
Conc: 74.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
P030-SS002-0006-01

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

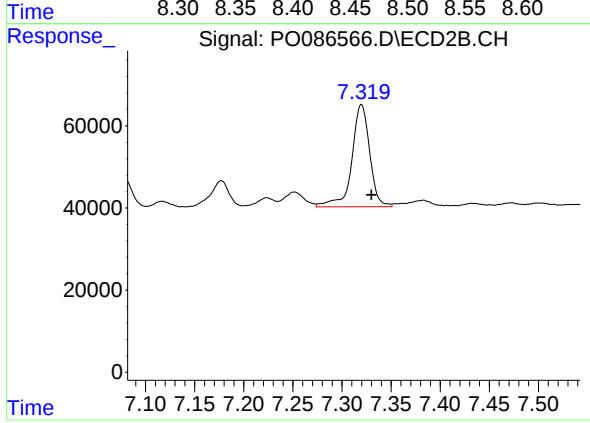

#35 AR-1260-5

R.T.: 7.320 min
Delta R.T.: -0.010 min
Response: 314626
Conc: 72.63 ng/ml