

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0052522\
 Data File : P0086571.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 May 2022 20:29
 Operator : YP\AJ
 Sample : N2895-15
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 P030-SS003-0006-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/26/2022
 Supervised By :Ankita Jodhani 05/26/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 06:49:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 19 09:06:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.477	3.673	2286750	927240	22.506	21.288
2) SA Decachlor...	10.326	8.721	993664	568207	18.300	16.327
Target Compounds						
31) L7 AR-1260-1	7.277	6.264	171241	114348	56.582	58.751
32) L7 AR-1260-2	7.535	6.452	579810	293534	160.279	124.891
33) L7 AR-1260-3	7.897	6.608	487202	137616	176.522	63.999 #
34) L7 AR-1260-4	8.123	7.080	408102	170186	120.956m	94.515
35) L7 AR-1260-5	8.452	7.321	871830	609821	141.285	140.777

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052522\
Data File : P0086571.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 May 2022 20:29
Operator : YP\AJ
Sample : N2895-15
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
P030-SS003-0006-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 06:49:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 19 09:06:34 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

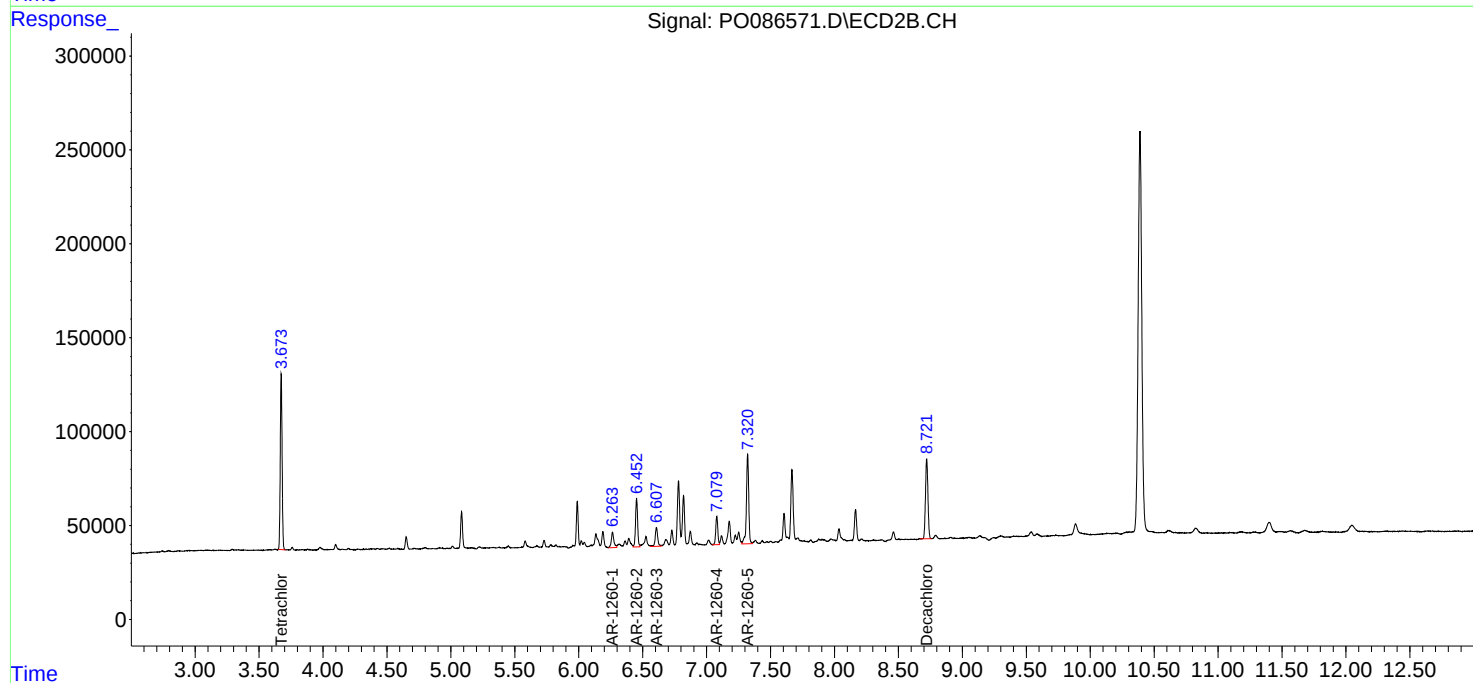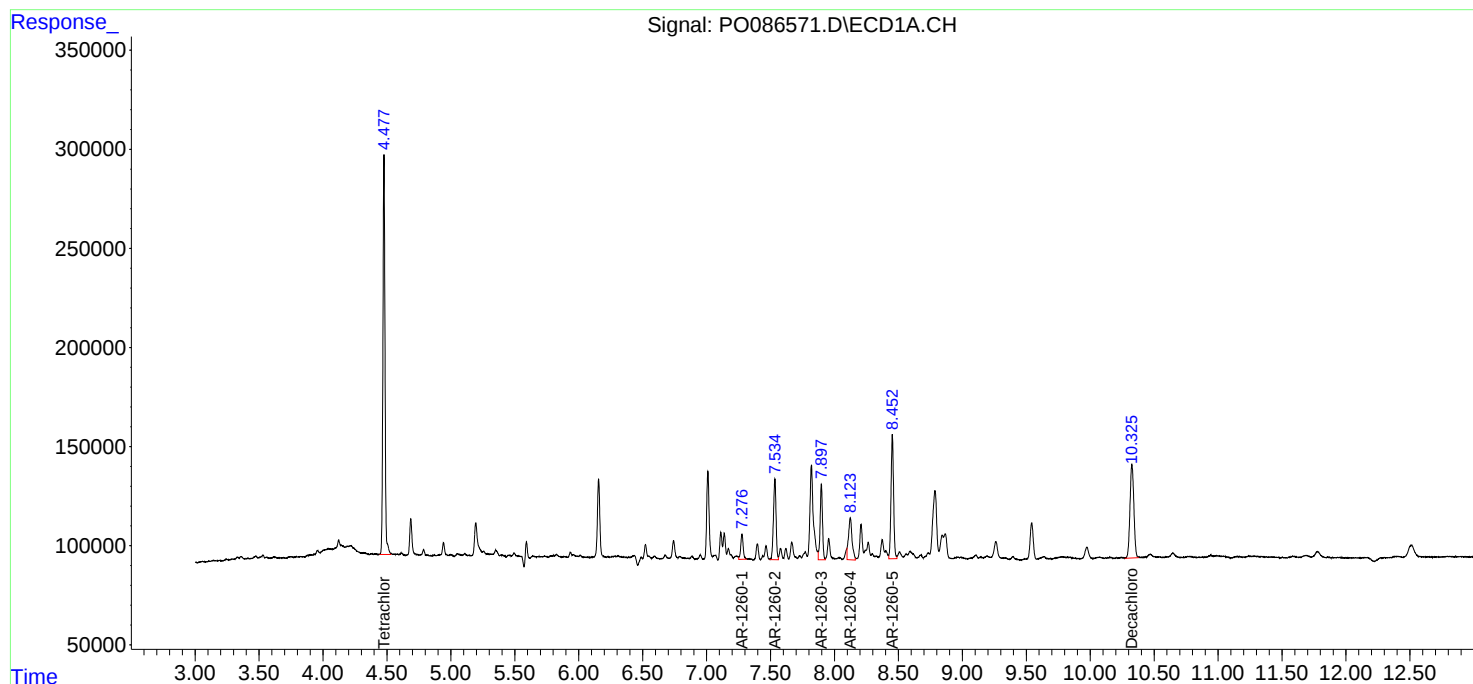

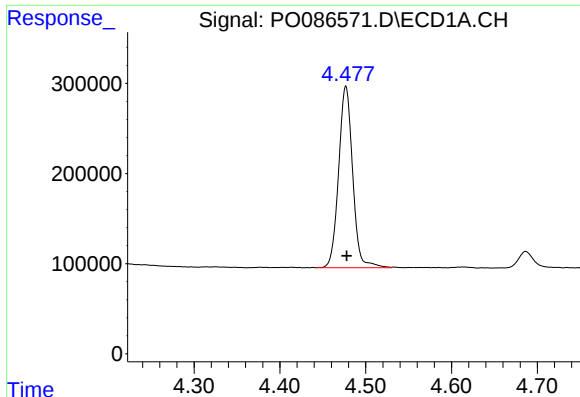


#1 Tetrachloro-m-xylene

R.T.: 4.477 min
Delta R.T.: -0.001 min
Response: 2286750
Conc: 22.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
P030-SS003-0006-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

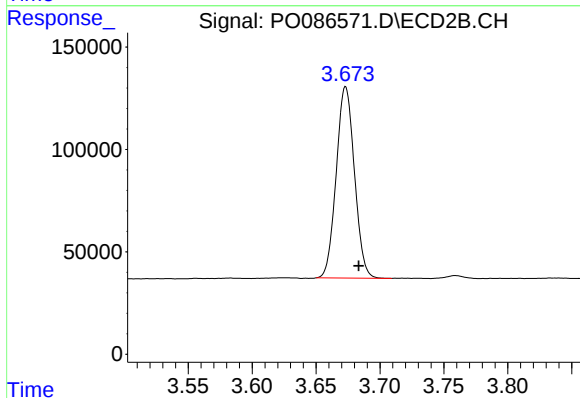


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: -0.010 min
Response: 927240
Conc: 21.29 ng/ml

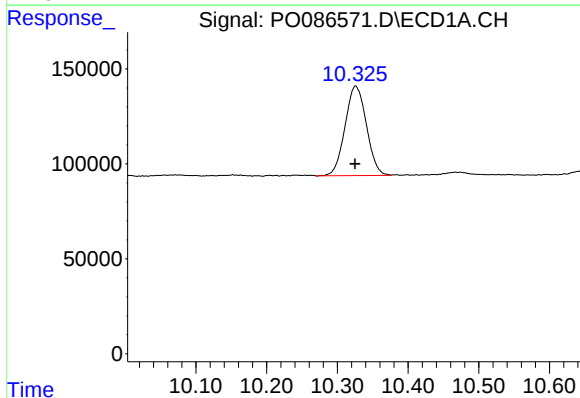


#2 Decachlorobiphenyl

R.T.: 10.326 min
Delta R.T.: 0.000 min
Response: 993664
Conc: 18.30 ng/ml

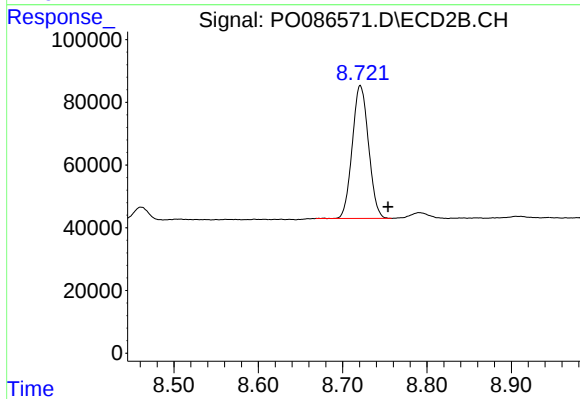

#2 Decachlorobiphenyl

R.T.: 8.721 min
Delta R.T.: -0.033 min
Response: 568207
Conc: 16.33 ng/ml

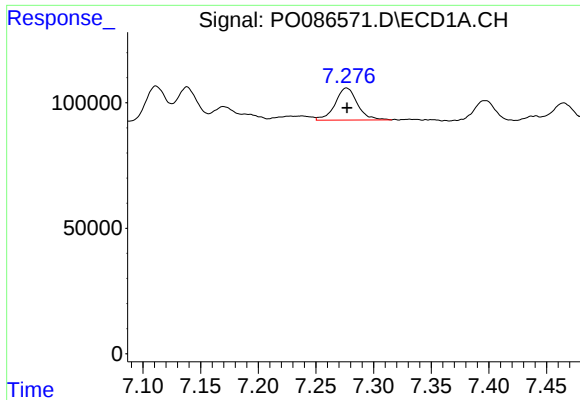


#31 AR-1260-1

R.T.: 7.277 min
Delta R.T.: 0.000 min
Response: 171241
Conc: 56.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
P030-SS003-0006-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

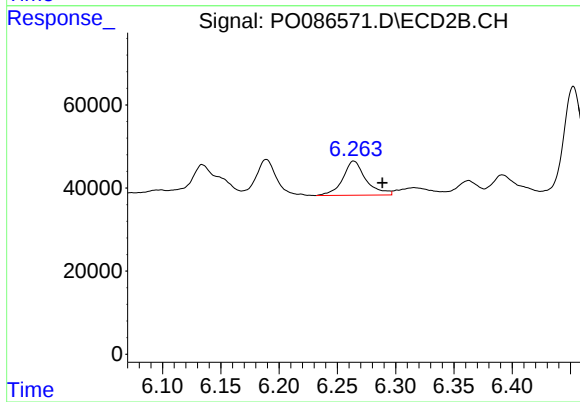


#31 AR-1260-1

R.T.: 6.264 min
Delta R.T.: -0.025 min
Response: 114348
Conc: 58.75 ng/ml

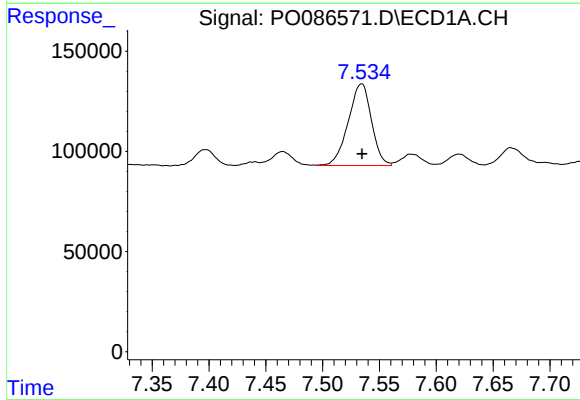


#32 AR-1260-2

R.T.: 7.535 min
Delta R.T.: 0.000 min
Response: 579810
Conc: 160.28 ng/ml

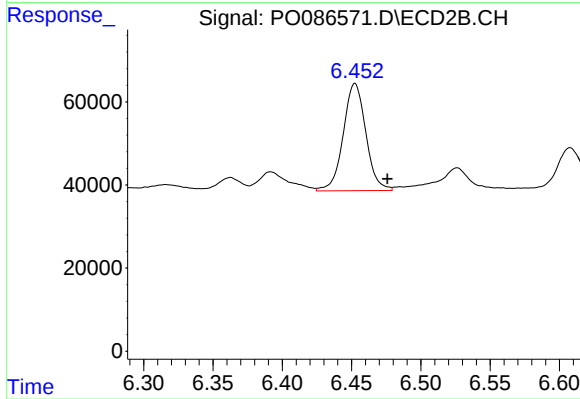

#32 AR-1260-2

R.T.: 6.452 min
Delta R.T.: -0.023 min
Response: 293534
Conc: 124.89 ng/ml

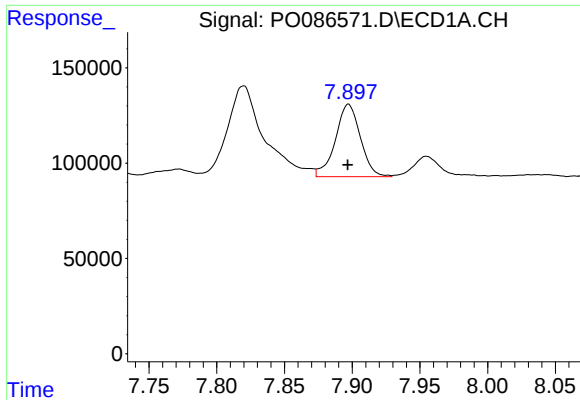


#33 AR-1260-3

R.T.: 7.897 min
Delta R.T.: 0.000 min
Response: 487202
Conc: 176.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
P030-SS003-0006-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

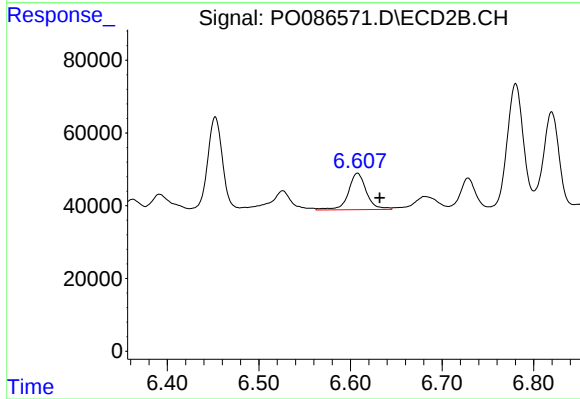


#33 AR-1260-3

R.T.: 6.608 min
Delta R.T.: -0.024 min
Response: 137616
Conc: 64.00 ng/ml

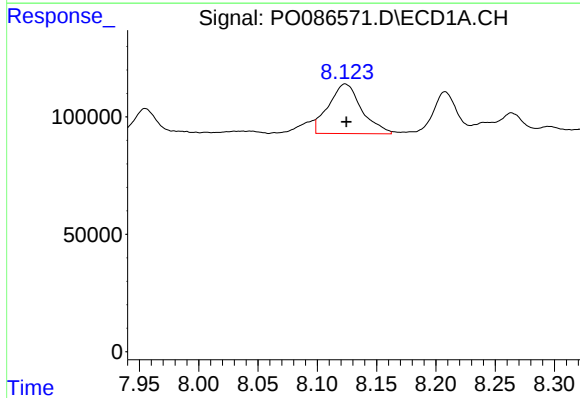


#34 AR-1260-4

R.T.: 8.123 min
Delta R.T.: -0.002 min
Response: 408102
Conc: 120.96 ng/ml m

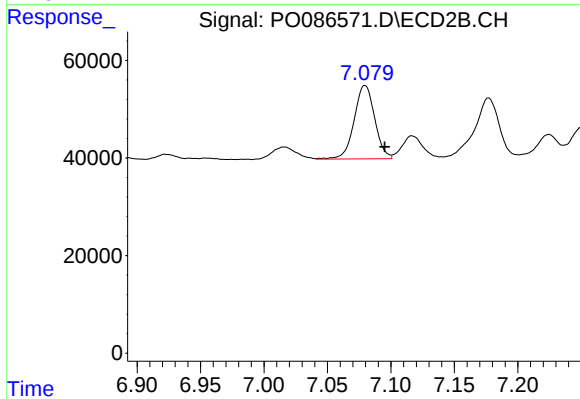

#34 AR-1260-4

R.T.: 7.080 min
Delta R.T.: -0.015 min
Response: 170186
Conc: 94.51 ng/ml

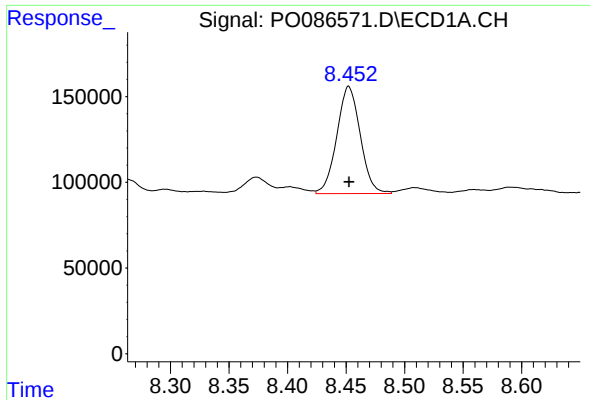


#35 AR-1260-5

R.T.: 8.452 min
Delta R.T.: 0.000 min
Response: 871830
Conc: 141.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
P030-SS003-0006-01

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

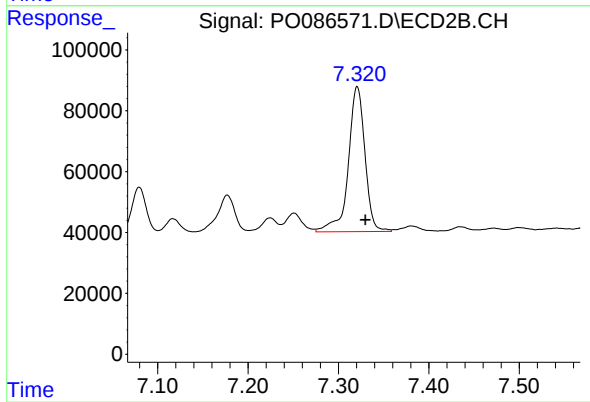

#35 AR-1260-5

R.T.: 7.321 min
Delta R.T.: -0.009 min
Response: 609821
Conc: 140.78 ng/ml