

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052522\
 Data File : P0086580.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 May 2022 23:43
 Operator : YP\AJ
 Sample : N3031-01
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PIPE-5-0524

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 06:53:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 19 09:06:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.476	3.672	2107981	878602	20.746	20.171
2) SA Decachlor...	10.325	8.719	1296739	764725	23.881	21.974

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052522\
Data File : P0086580.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 May 2022 23:43
Operator : YP\AJ
Sample : N3031-01
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PIPE-5-0524

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 06:53:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 19 09:06:34 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

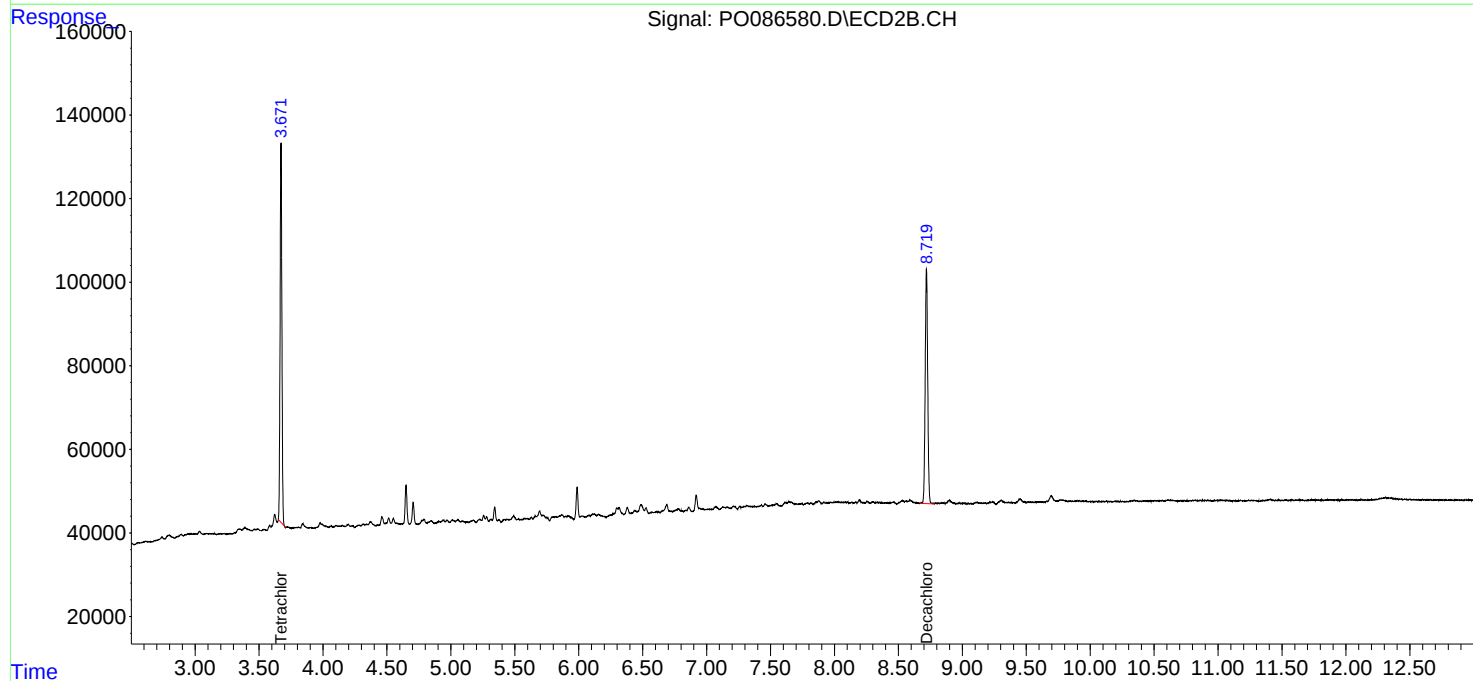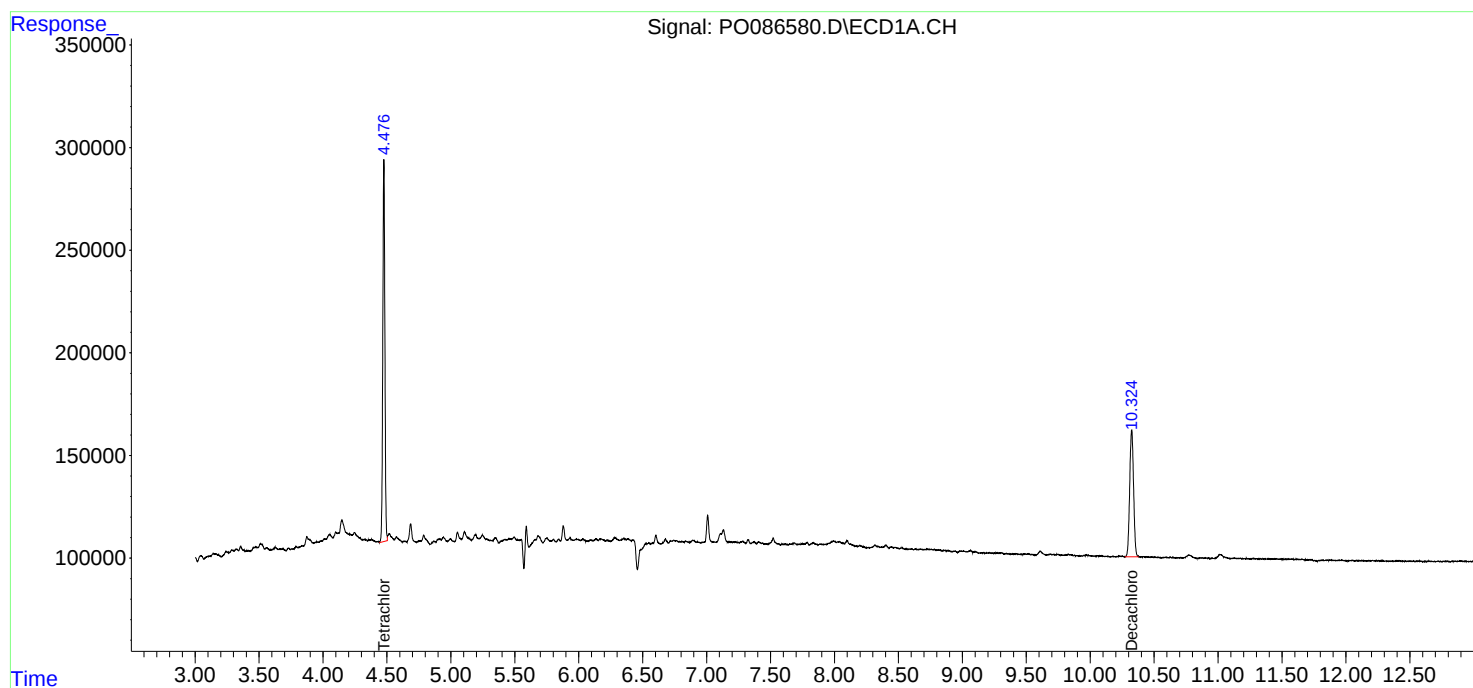


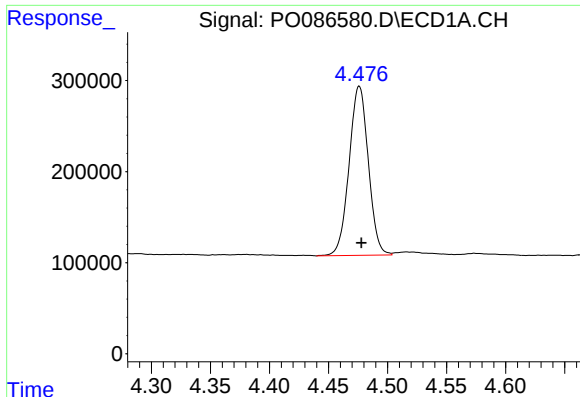

#1 Tetrachloro-m-xylene


R.T.: 4.476 min
Delta R.T.: -0.002 min
Response: 2107981
Conc: 20.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
PIPE-5-0524

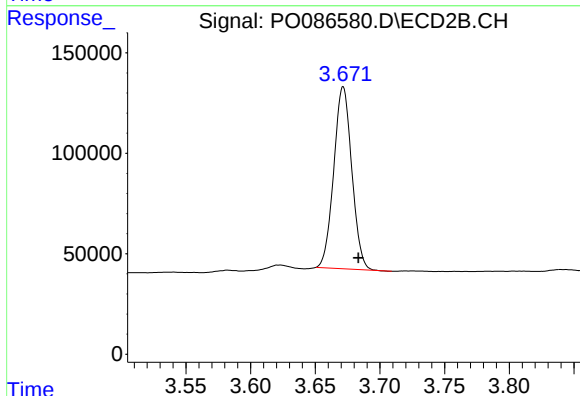


#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: -0.012 min
Response: 878602
Conc: 20.17 ng/ml

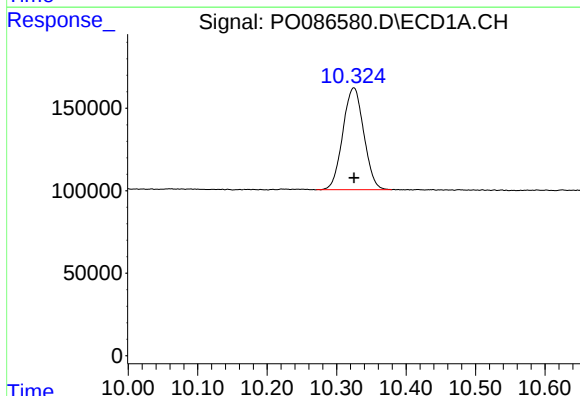

#2 Decachlorobiphenyl

R.T.: 10.325 min
Delta R.T.: 0.000 min
Response: 1296739
Conc: 23.88 ng/ml

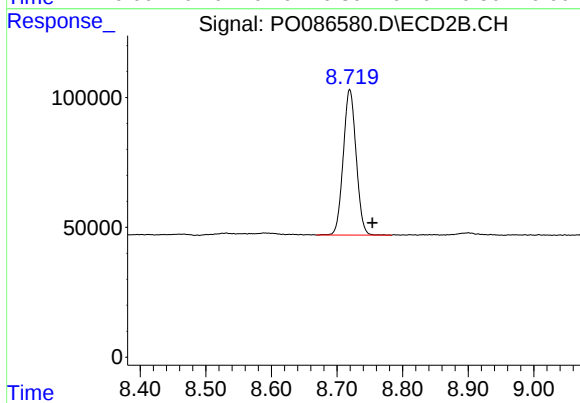

#2 Decachlorobiphenyl

R.T.: 8.719 min
Delta R.T.: -0.034 min
Response: 764725
Conc: 21.97 ng/ml