

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0052522\
 Data File : P0086585.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 May 2022 1:04
 Operator : YP\AJ
 Sample : N2895-16
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 P030-SS003-0612-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/26/2022
 Supervised By :Ankita Jodhani 05/26/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 06:56:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 19 09:06:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.475	3.671	2043995	815629	20.117	18.725
2) SA Decachlor...	10.323	8.719	657770	385921	12.114	11.089
Target Compounds						
31) L7 AR-1260-1	7.276	6.262	68839	15016	22.746	7.715m#
32) L7 AR-1260-2	7.532	6.450	85672	34785	23.683	14.800m#
33) L7 AR-1260-3	7.895	6.605	68672	21048	24.881	9.789 #
34) L7 AR-1260-4	8.121	7.077	64093	28161	18.996	15.639
35) L7 AR-1260-5	8.450	7.319	139418	81677	22.594	18.855

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052522\
Data File : P0086585.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 May 2022 1:04
Operator : YP\AJ
Sample : N2895-16
Misc :
ALS Vial : 56 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
P030-SS003-0612-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 06:56:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 19 09:06:34 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

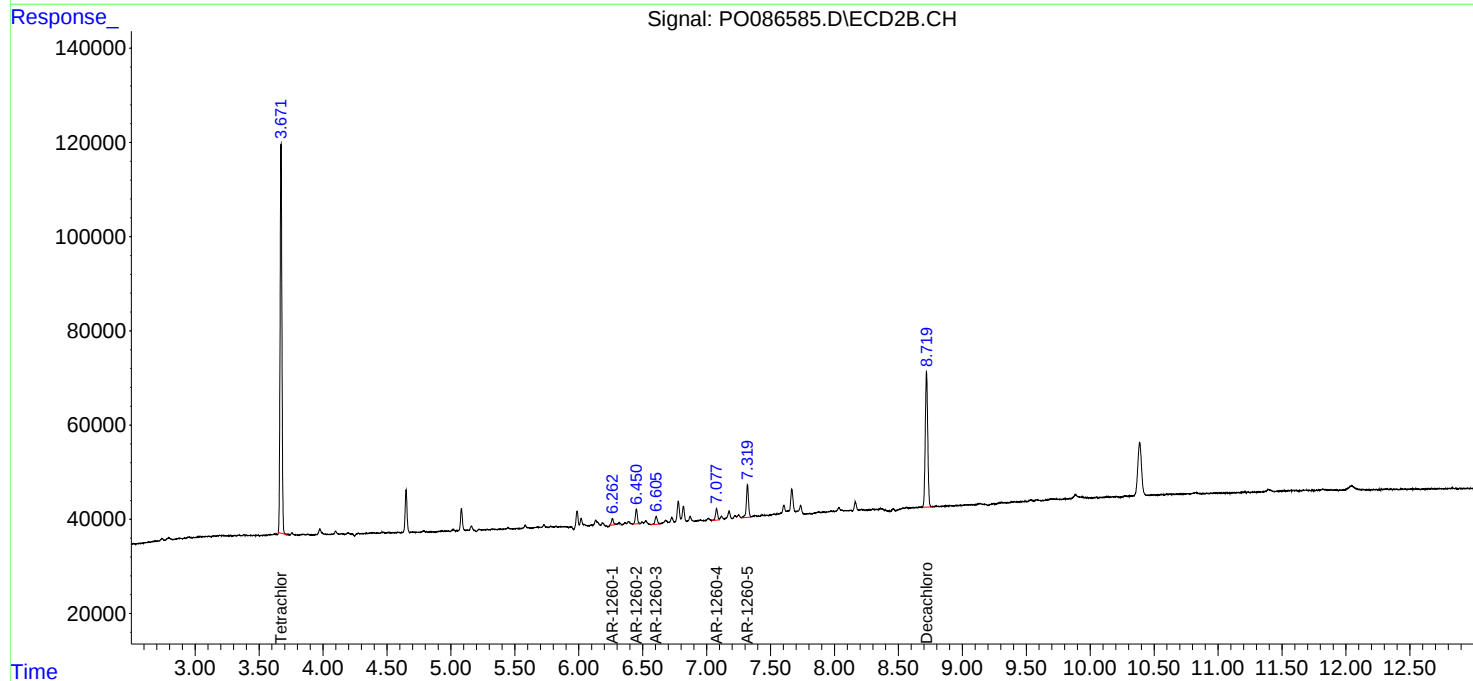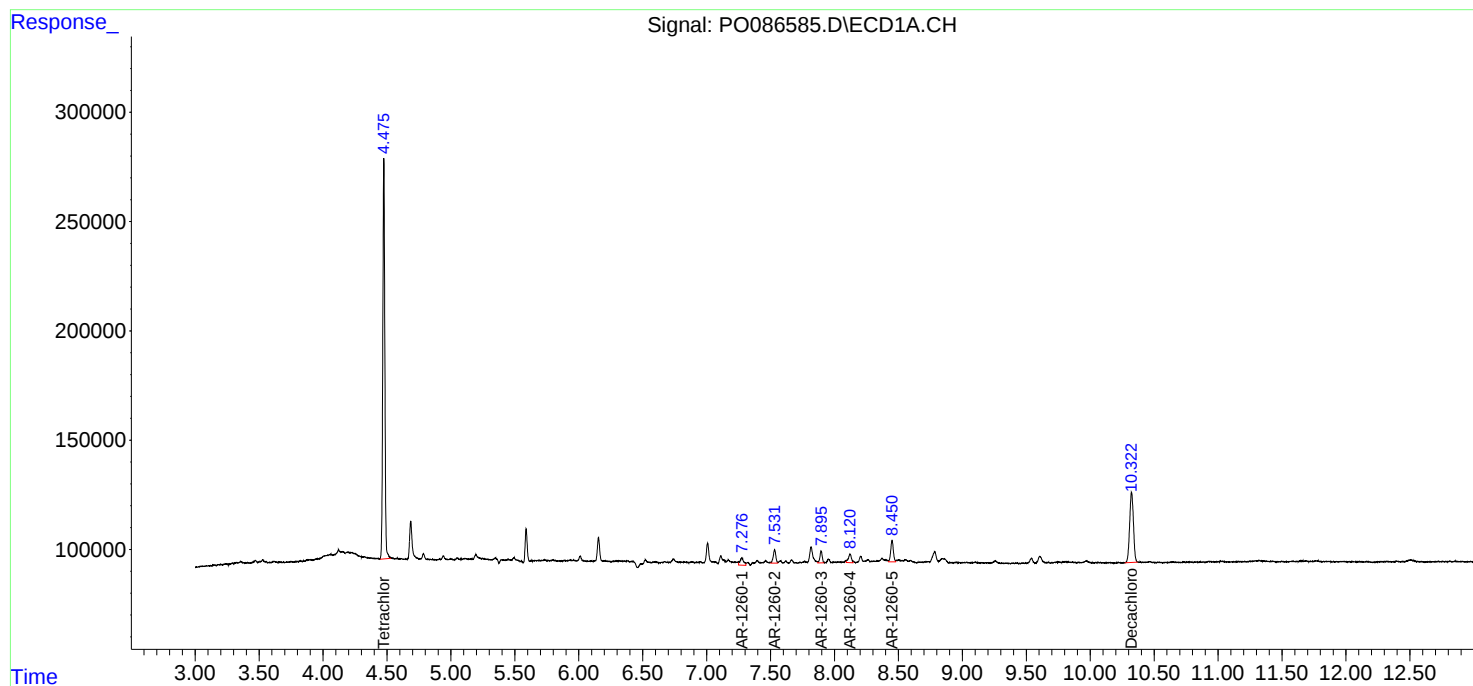

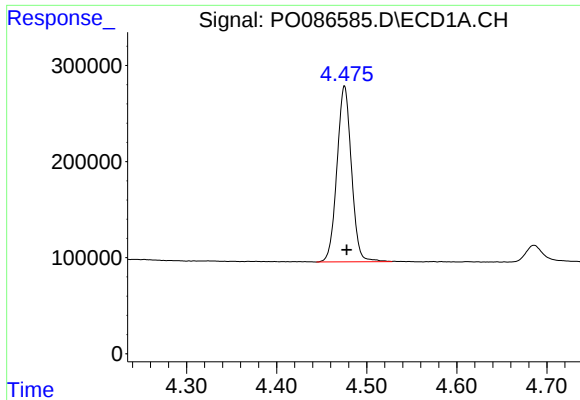


#1 Tetrachloro-m-xylene

R.T.: 4.475 min
Delta R.T.: -0.003 min
Response: 2043995
Conc: 20.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
P030-SS003-0612-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

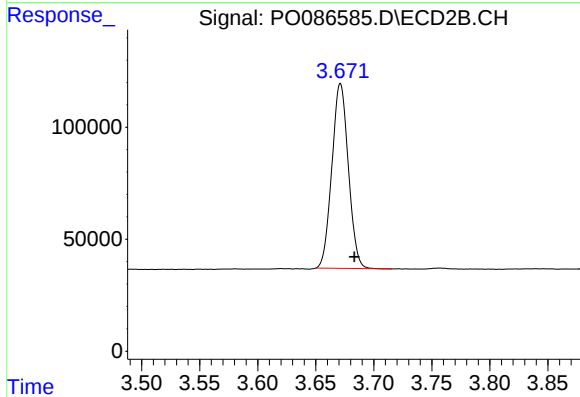


#1 Tetrachloro-m-xylene

R.T.: 3.671 min
Delta R.T.: -0.012 min
Response: 815629
Conc: 18.73 ng/ml

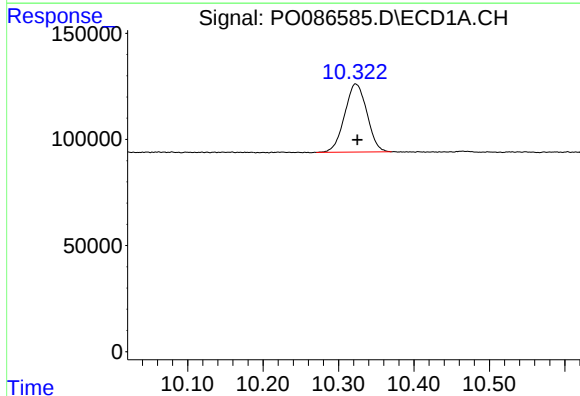


#2 Decachlorobiphenyl

R.T.: 10.323 min
Delta R.T.: -0.003 min
Response: 657770
Conc: 12.11 ng/ml

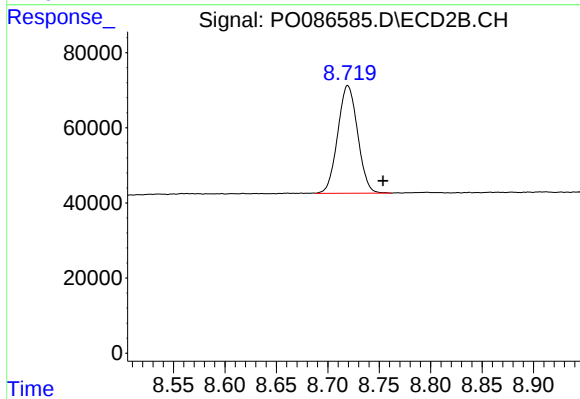

#2 Decachlorobiphenyl

R.T.: 8.719 min
Delta R.T.: -0.035 min
Response: 385921
Conc: 11.09 ng/ml

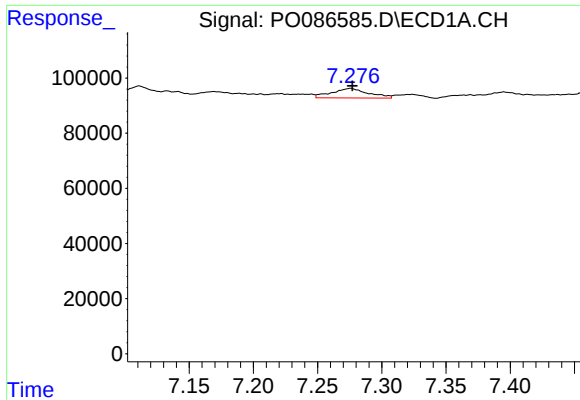


#31 AR-1260-1

R.T.: 7.276 min
Delta R.T.: -0.001 min
Response: 68839
Conc: 22.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
P030-SS003-0612-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

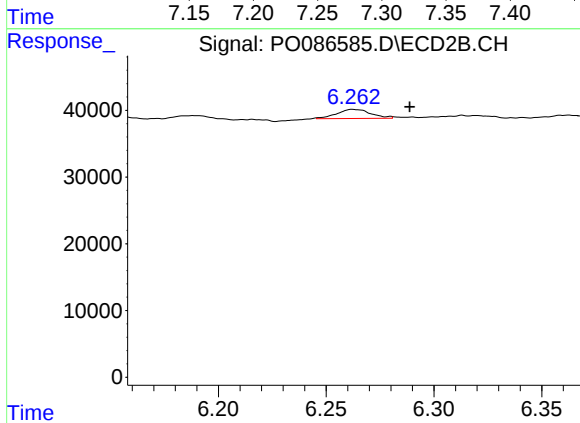


#31 AR-1260-1

R.T.: 6.262 min
Delta R.T.: -0.027 min
Response: 15016
Conc: 7.72 ng/ml m

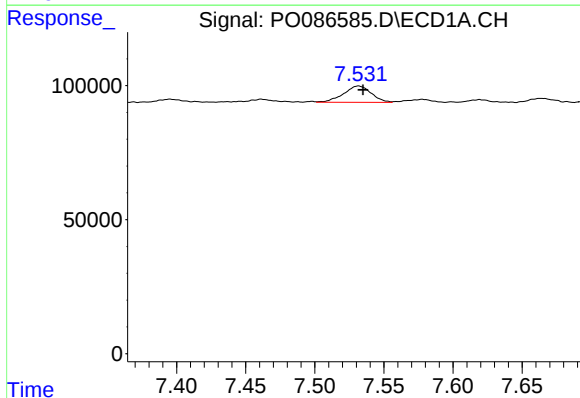


#32 AR-1260-2

R.T.: 7.532 min
Delta R.T.: -0.003 min
Response: 85672
Conc: 23.68 ng/ml

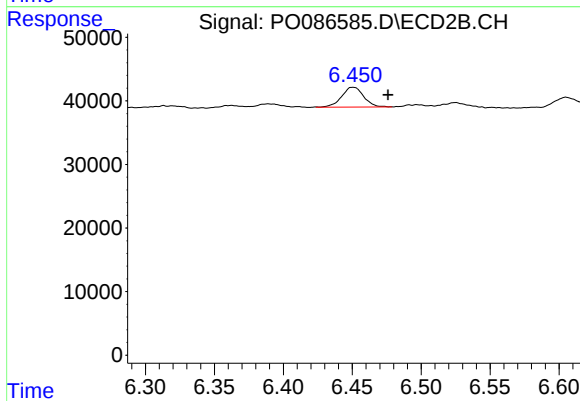

#32 AR-1260-2

R.T.: 6.450 min
Delta R.T.: -0.026 min
Response: 34785
Conc: 14.80 ng/ml m

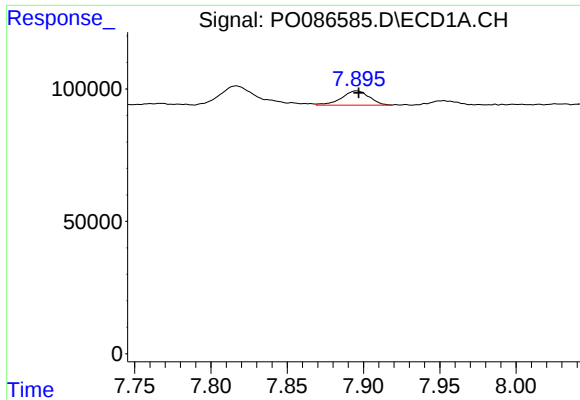


#33 AR-1260-3

R.T.: 7.895 min
Delta R.T.: -0.001 min
Response: 68672
Conc: 24.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
P030-SS003-0612-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

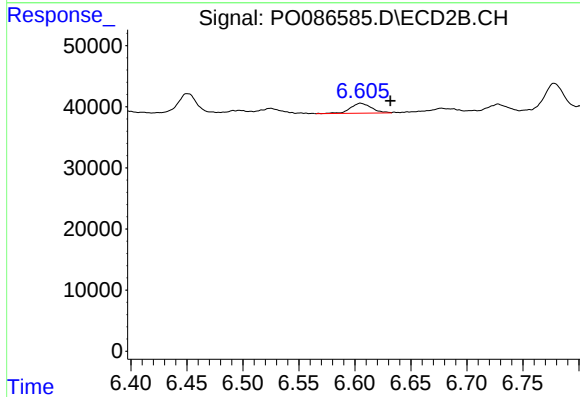


#33 AR-1260-3

R.T.: 6.605 min
Delta R.T.: -0.027 min
Response: 21048
Conc: 9.79 ng/ml

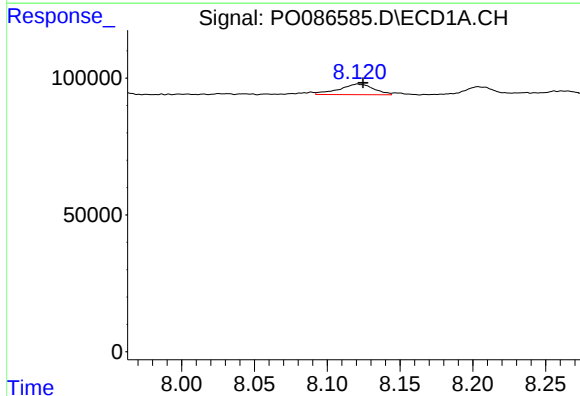


#34 AR-1260-4

R.T.: 8.121 min
Delta R.T.: -0.004 min
Response: 64093
Conc: 19.00 ng/ml

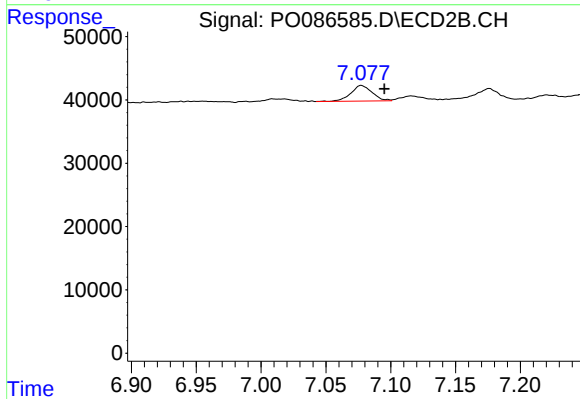

#34 AR-1260-4

R.T.: 7.077 min
Delta R.T.: -0.018 min
Response: 28161
Conc: 15.64 ng/ml

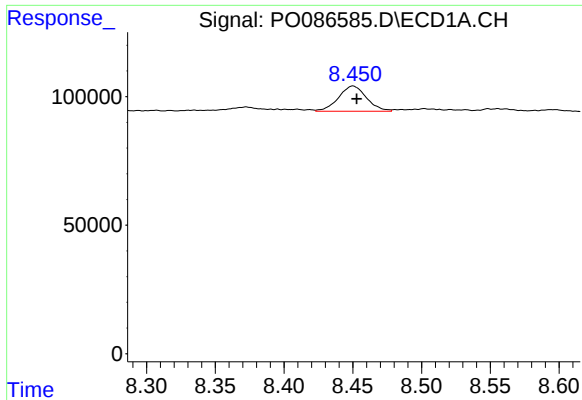


#35 AR-1260-5

R.T.: 8.450 min
Delta R.T.: -0.003 min
Response: 139418
Conc: 22.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
P030-SS003-0612-01

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

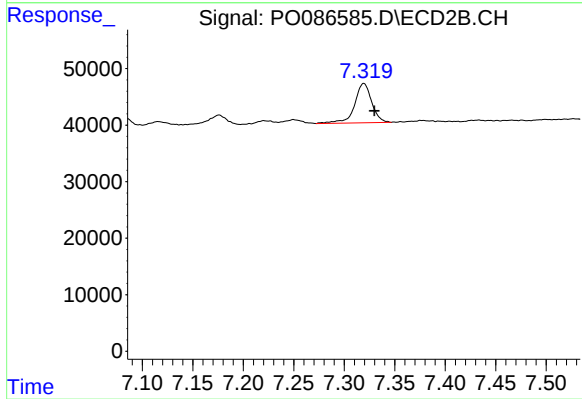

#35 AR-1260-5

R.T.: 7.319 min
Delta R.T.: -0.011 min
Response: 81677
Conc: 18.86 ng/ml