

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052620\
 Data File : P0068561.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 May 2020 19:16
 Operator : DD\AJ
 Sample : L2744-20
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NM50-COMP-2020-0-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 07:38:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 08 13:29:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.895	3.930	375408	578758	13.385	16.866 #
2) SA Decachlor...	10.840	9.200	360733	437949	9.065	11.376 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052620\
Data File : P0068561.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 May 2020 19:16
Operator : DD\AJ
Sample : L2744-20
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
NM50-COMP-2020-0-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 07:38:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 08 13:29:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

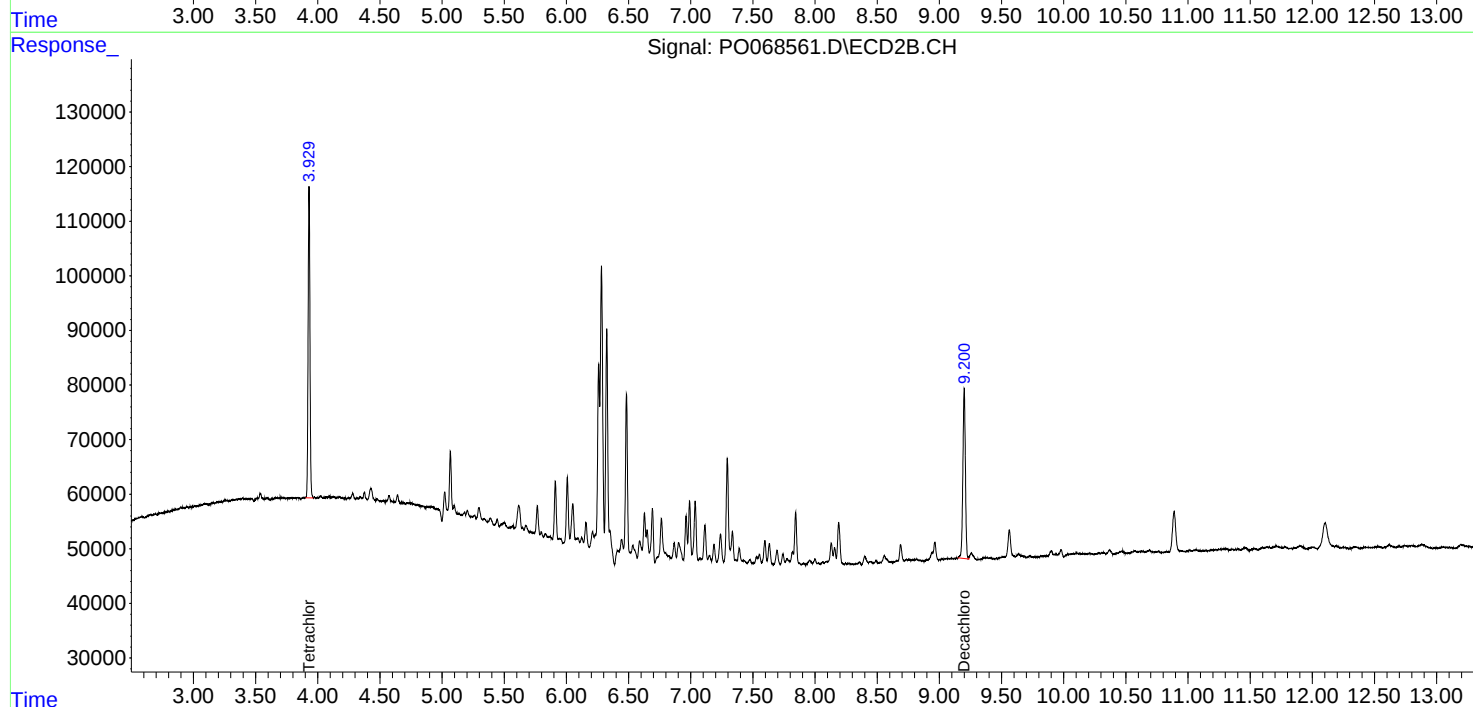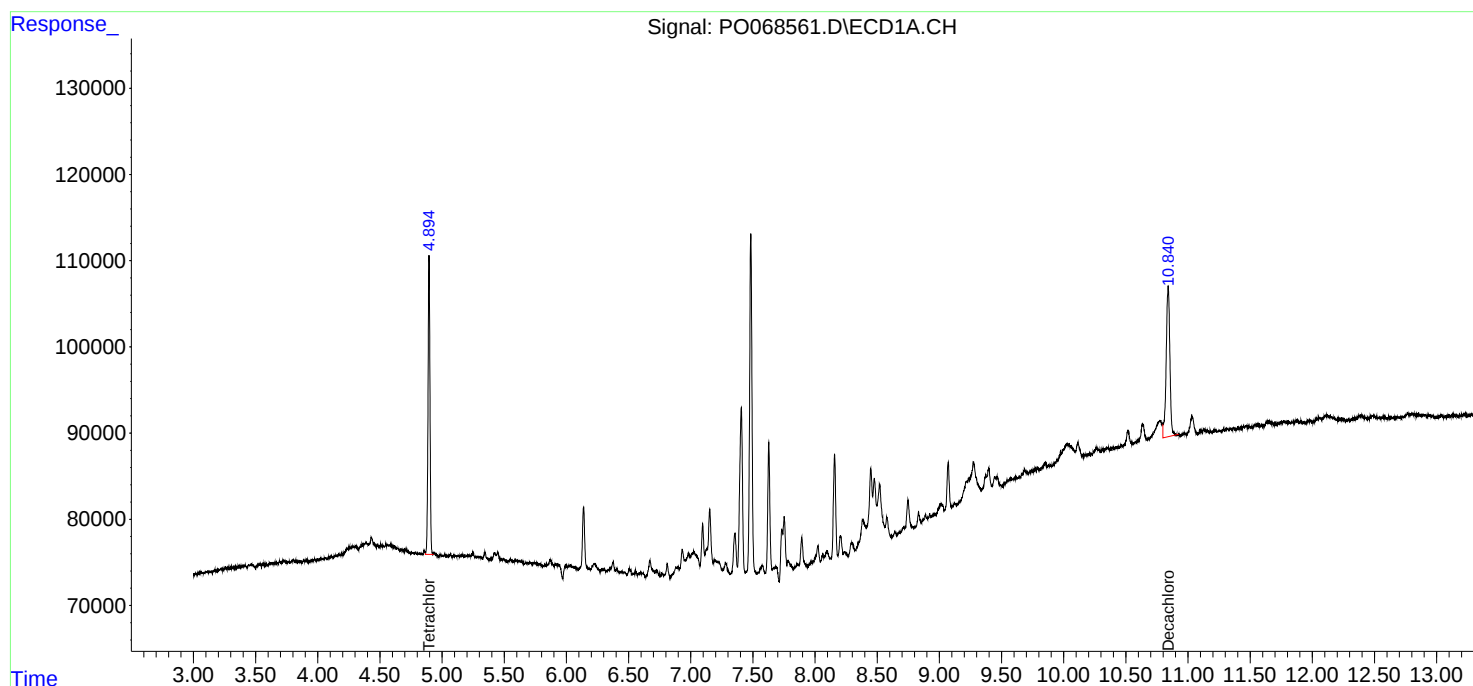


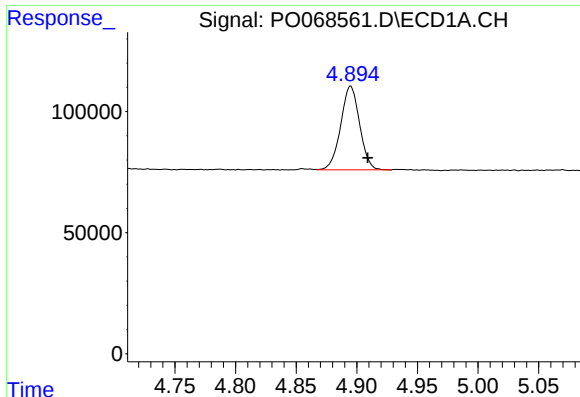

#1 Tetrachloro-m-xylene


R.T.: 4.895 min
Delta R.T.: -0.014 min
Response: 375408
Conc: 13.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
NM50-COMP-2020-0-6

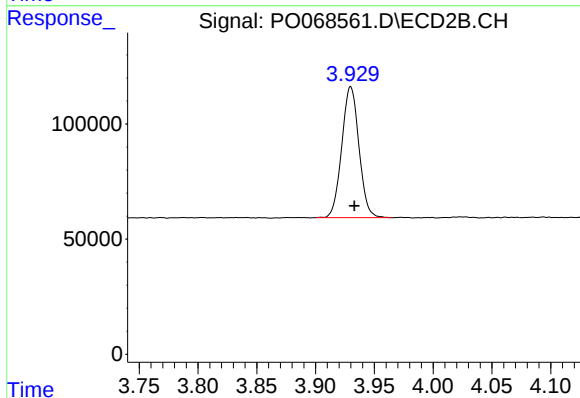


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: -0.003 min
Response: 578758
Conc: 16.87 ng/ml

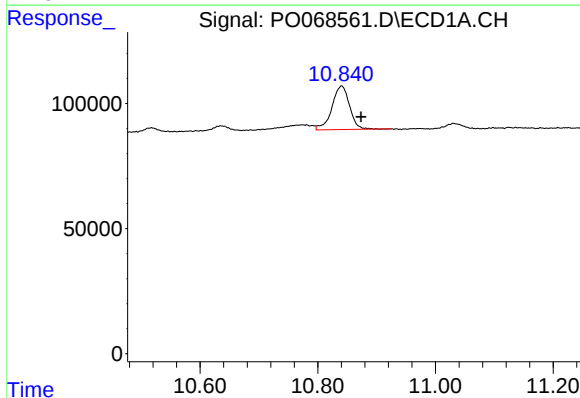

#2 Decachlorobiphenyl

R.T.: 10.840 min
Delta R.T.: -0.033 min
Response: 360733
Conc: 9.07 ng/ml

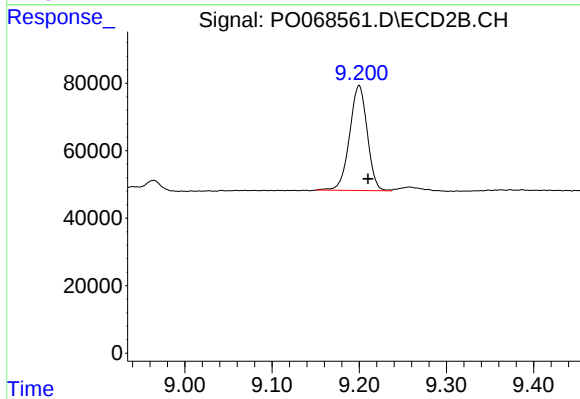

#2 Decachlorobiphenyl

R.T.: 9.200 min
Delta R.T.: -0.010 min
Response: 437949
Conc: 11.38 ng/ml