

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052621\
 Data File : P0078157.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 May 2021 11:49
 Operator : DD\AJ
 Sample : M2512-01 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-1-3

Manual Integrations
 APPROVED

Ankita
 5/27/2021 2:10:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 12:56:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.330	3.620	906101	259063	12.260m	8.574m#
2) SA Decachlor...	9.959	8.821	144834	167638	2.929m	5.765m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052621\
Data File : P0078157.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 May 2021 11:49
Operator : DD\AJ
Sample : M2512-01 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-1-3


Manual Integrations
APPROVED

Ankita
5/27/2021 2:10:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 12:56:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

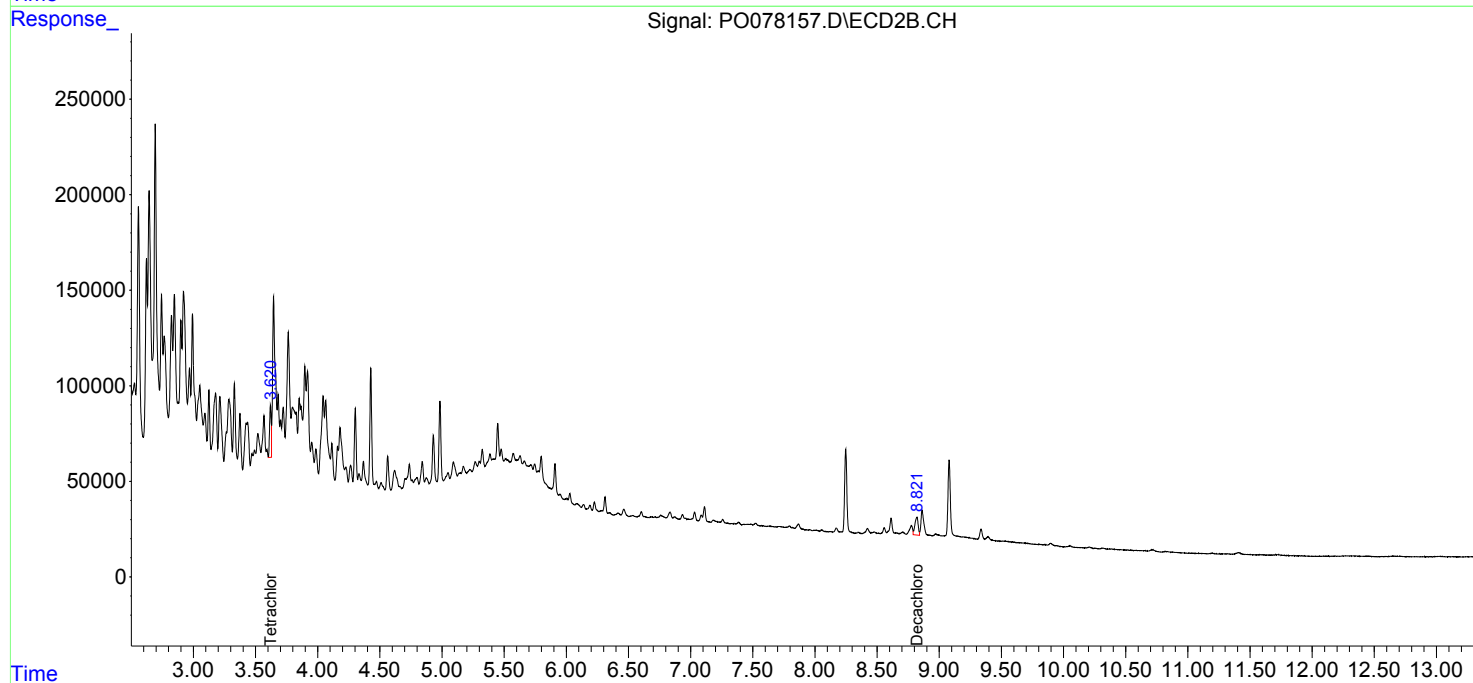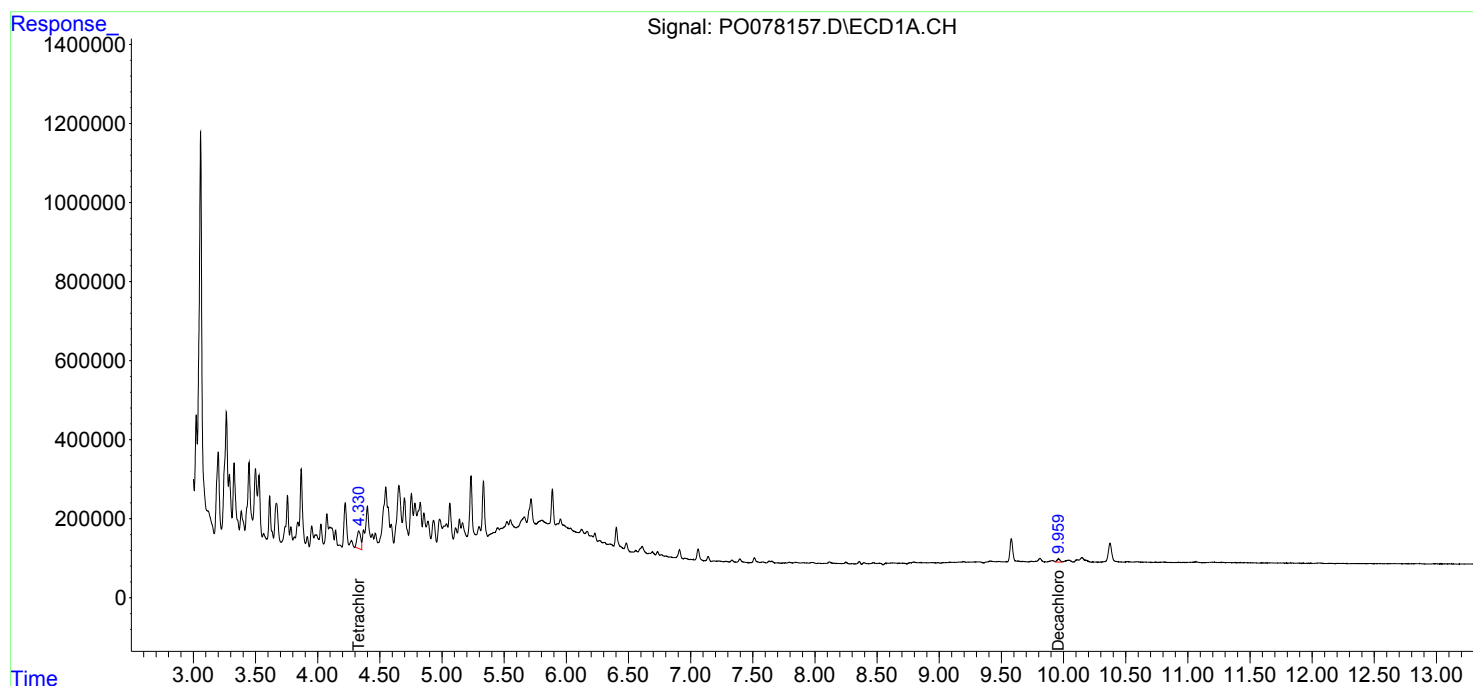

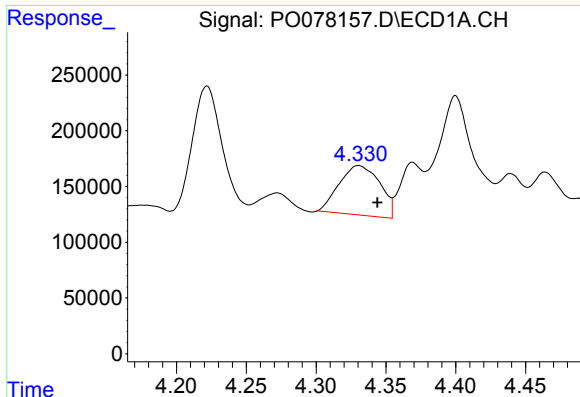


#1 Tetrachloro-m-xylene

R.T.: 4.330 min
Delta R.T.: -0.014 min
Response: 906101
Conc: 12.26 ng/ml m

Instrument :
ECD_O
ClientSampleId :
COMP-1-3


Manual Integrations
APPROVED

Ankita
5/27/2021 2:10:20 PM

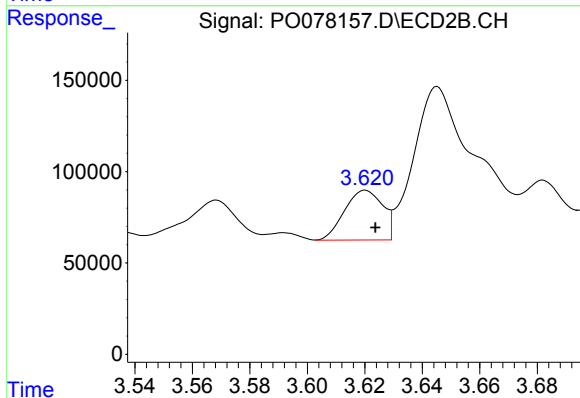


#1 Tetrachloro-m-xylene

R.T.: 3.620 min
Delta R.T.: -0.004 min
Response: 259063
Conc: 8.57 ng/ml m

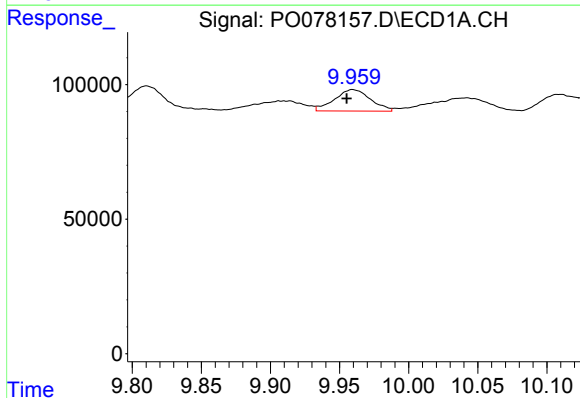

#2 Decachlorobiphenyl

R.T.: 9.959 min
Delta R.T.: 0.003 min
Response: 144834
Conc: 2.93 ng/ml m

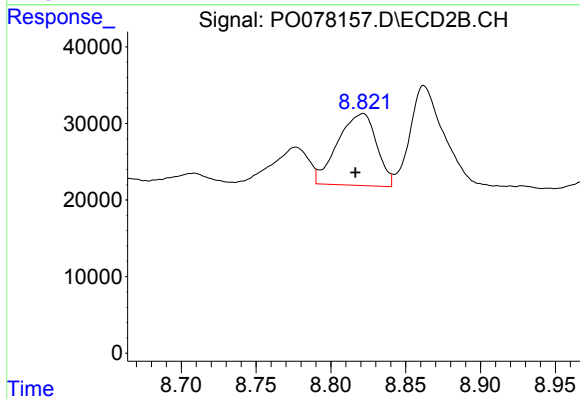

#2 Decachlorobiphenyl

R.T.: 8.821 min
Delta R.T.: 0.005 min
Response: 167638
Conc: 5.77 ng/ml m