

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052621\
 Data File : P0078163.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 May 2021 13:51
 Operator : DD\AJ
 Sample : M2512-01RE 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-1-3RE

Manual Integrations
 APPROVED

Ankita
 5/27/2021 2:10:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 14:48:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.331	3.619	808064	276050	10.933m	9.136m
2) SA Decachlor...	9.961	8.816	111695	143928	2.259m	4.950m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052621\
Data File : P0078163.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 May 2021 13:51
Operator : DD\AJ
Sample : M2512-01RE 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
COMP-1-3RE


Manual Integrations
APPROVED

Ankita
5/27/2021 2:10:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 14:48:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

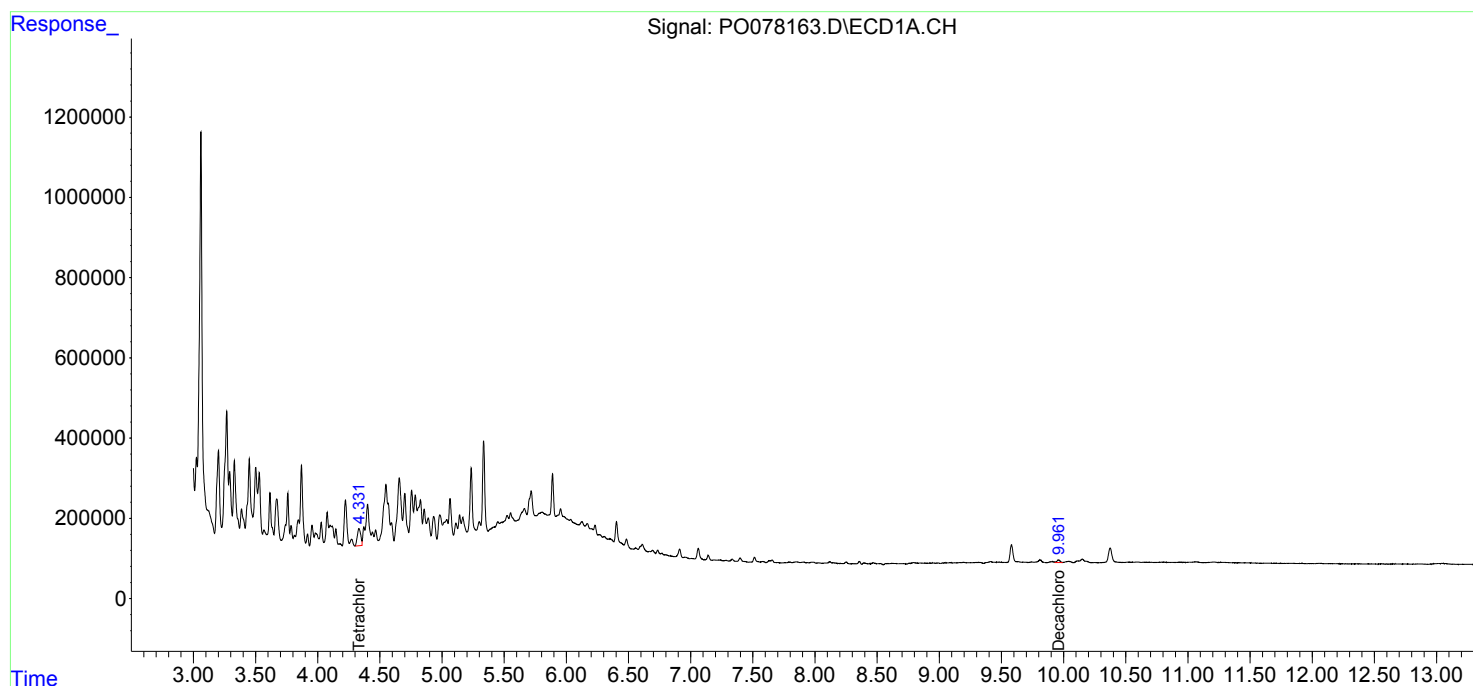

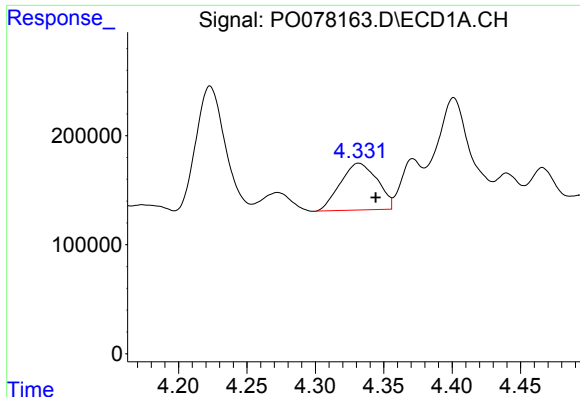


#1 Tetrachloro-m-xylene

R.T.: 4.331 min
Delta R.T.: -0.013 min
Response: 808064
Conc: 10.93 ng/ml m

Instrument :
ECD_O
ClientSampleId :
COMP-1-3RE


Manual Integrations
APPROVED

Ankita
5/27/2021 2:10:25 PM

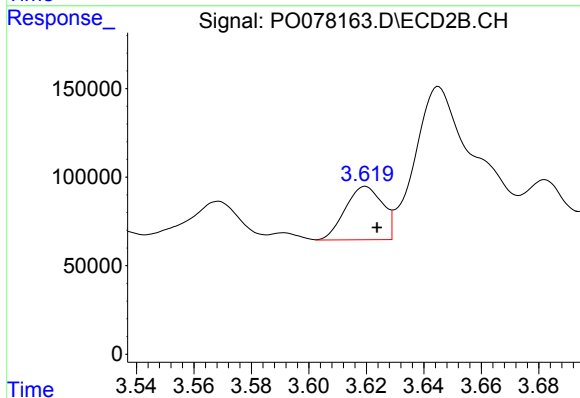


#1 Tetrachloro-m-xylene

R.T.: 3.619 min
Delta R.T.: -0.004 min
Response: 276050
Conc: 9.14 ng/ml m

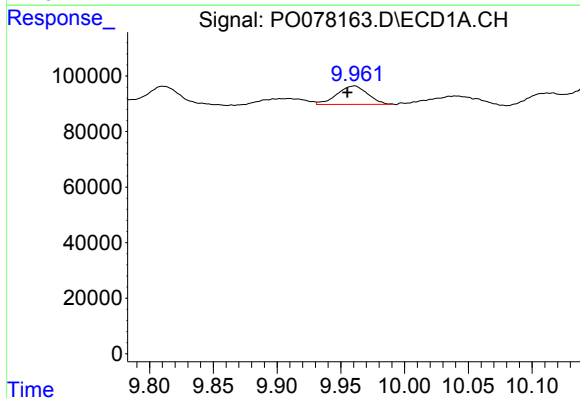

#2 Decachlorobiphenyl

R.T.: 9.961 min
Delta R.T.: 0.006 min
Response: 111695
Conc: 2.26 ng/ml m

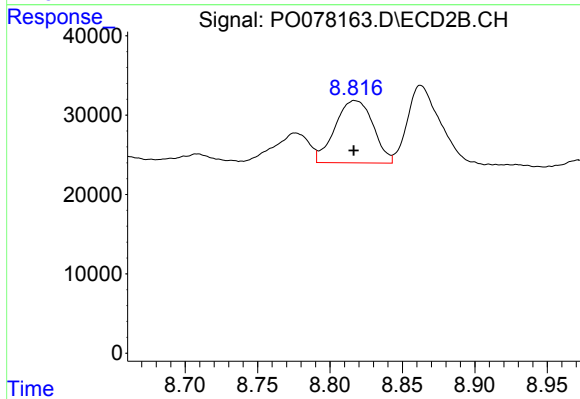

#2 Decachlorobiphenyl

R.T.: 8.816 min
Delta R.T.: 0.000 min
Response: 143928
Conc: 4.95 ng/ml m