

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052621\
 Data File : P0078164.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 May 2021 14:08
 Operator : DD\AJ
 Sample : M2512-04RE 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-4-6RE

Manual Integrations
 APPROVED

Ankita
 5/27/2021 2:10:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 14:49:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.330	3.620	890611	322577	12.050m	10.676m
2) SA Decachlor...	9.959	8.814	88058	101600	1.781m	3.494m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052621\
Data File : P0078164.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 May 2021 14:08
Operator : DD\AJ
Sample : M2512-04RE 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-4-6RE


Manual Integrations
APPROVED

Ankita
5/27/2021 2:10:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 14:49:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

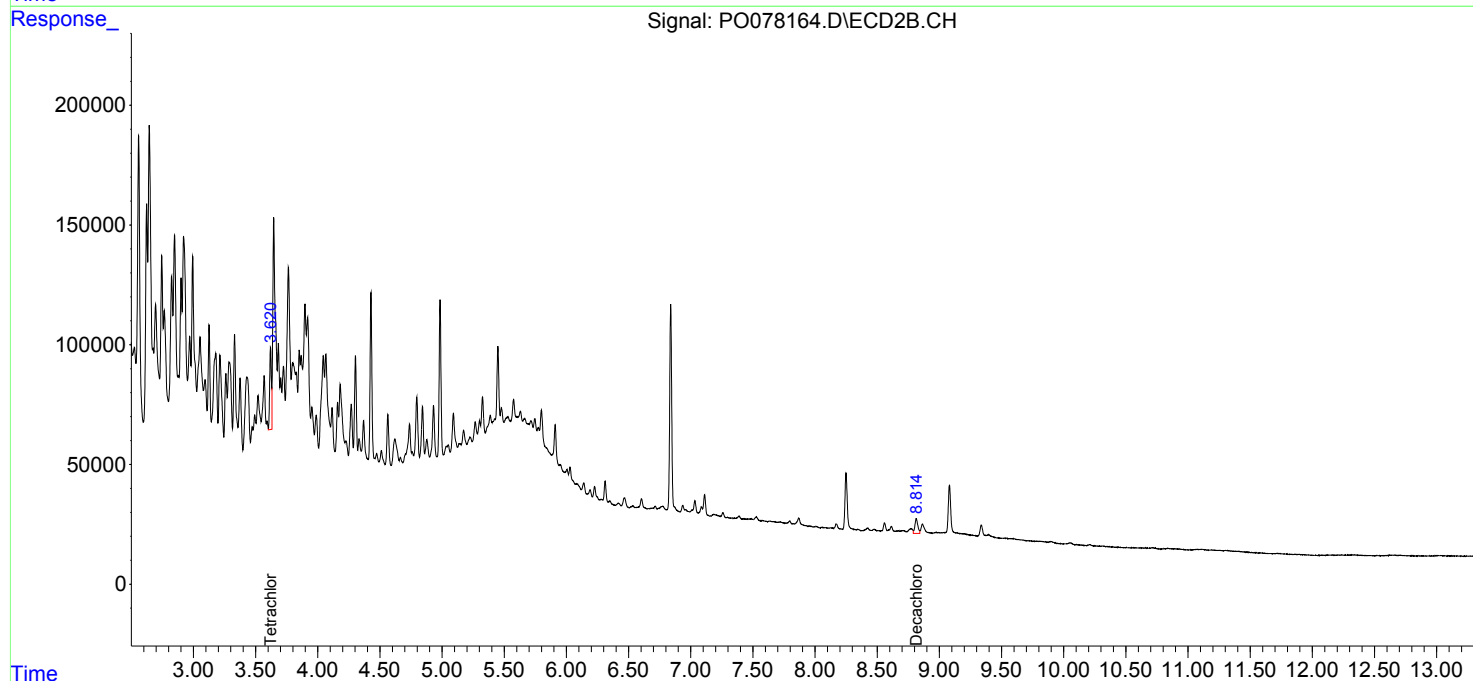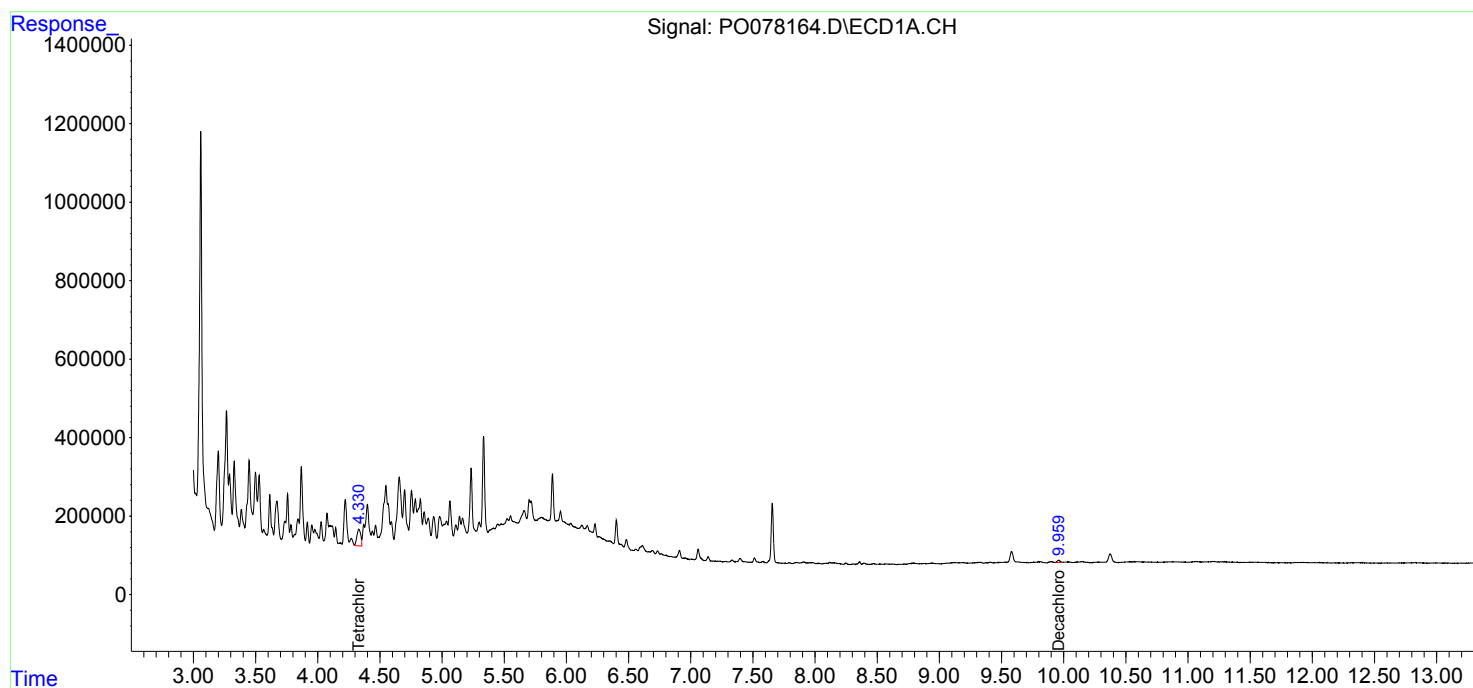

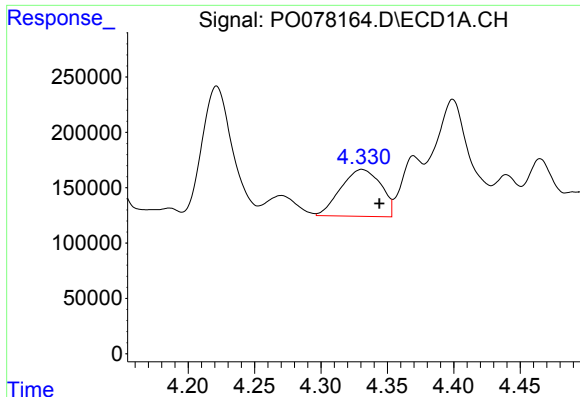


#1 Tetrachloro-m-xylene

R.T.: 4.330 min
Delta R.T.: -0.014 min
Response: 890611
Conc: 12.05 ng/ml m

Instrument :
ECD_O
ClientSampleId :
COMP-4-6RE


Manual Integrations
APPROVED

Ankita
5/27/2021 2:10:27 PM

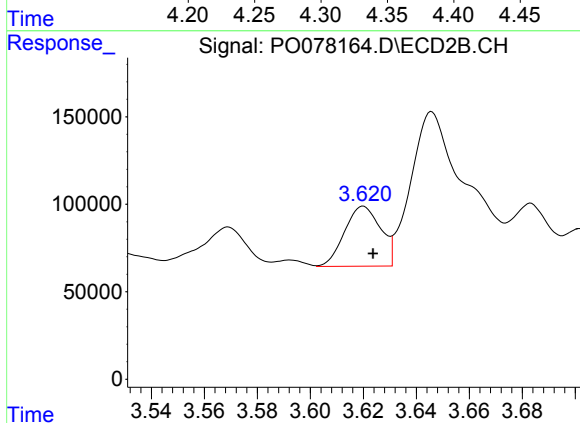


#1 Tetrachloro-m-xylene

R.T.: 3.620 min
Delta R.T.: -0.004 min
Response: 322577
Conc: 10.68 ng/ml m

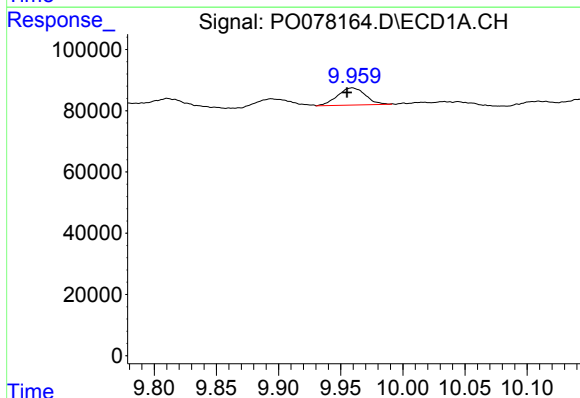

#2 Decachlorobiphenyl

R.T.: 9.959 min
Delta R.T.: 0.004 min
Response: 88058
Conc: 1.78 ng/ml m

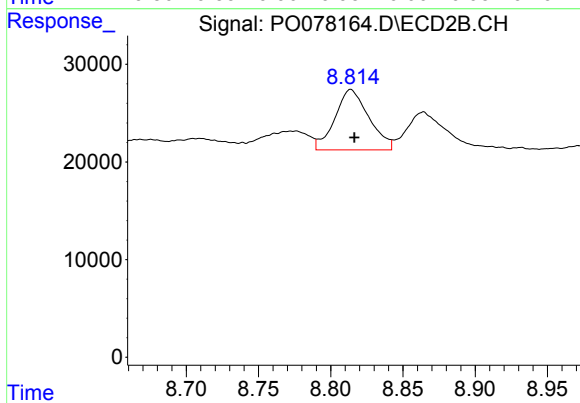

#2 Decachlorobiphenyl

R.T.: 8.814 min
Delta R.T.: -0.003 min
Response: 101600
Conc: 3.49 ng/ml m