

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0052621\
 Data File : P0078165.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 May 2021 14:25
 Operator : DD\AJ
 Sample : M2517-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 METRO-SP

Manual Integrations
 APPROVED

Ankita
 5/27/2021 2:10:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 14:50:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.343	3.621	1055804	517257	14.285	17.119
2) SA Decachlor...	9.958	8.811	749567	443820	15.161m	15.263m
Target Compounds						
31) L7 AR-1260-1	7.300	6.414	22563	28471	8.040m	17.769 #
32) L7 AR-1260-2	7.565	6.611	56565	30566	16.814	15.833
33) L7 AR-1260-3	7.920	6.760	28605	22574	11.724m	12.304
34) L7 AR-1260-4	8.148	7.236	68183	12589	25.454	8.351 #
35) L7 AR-1260-5	8.465	7.486	40604	26191	7.906	7.510

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052621\
Data File : P0078165.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 May 2021 14:25
Operator : DD\AJ
Sample : M2517-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
METRO-SP


Manual Integrations
APPROVED

Ankita
5/27/2021 2:10:28 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 14:50:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

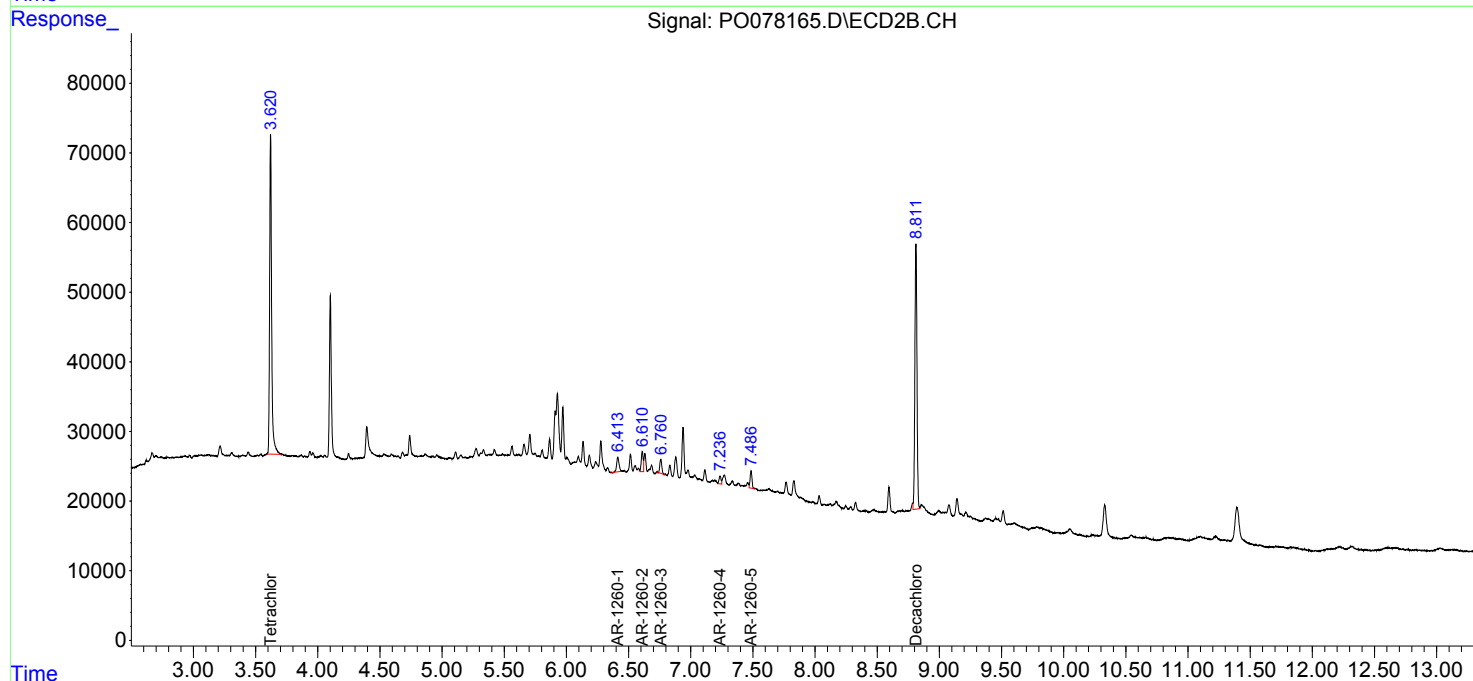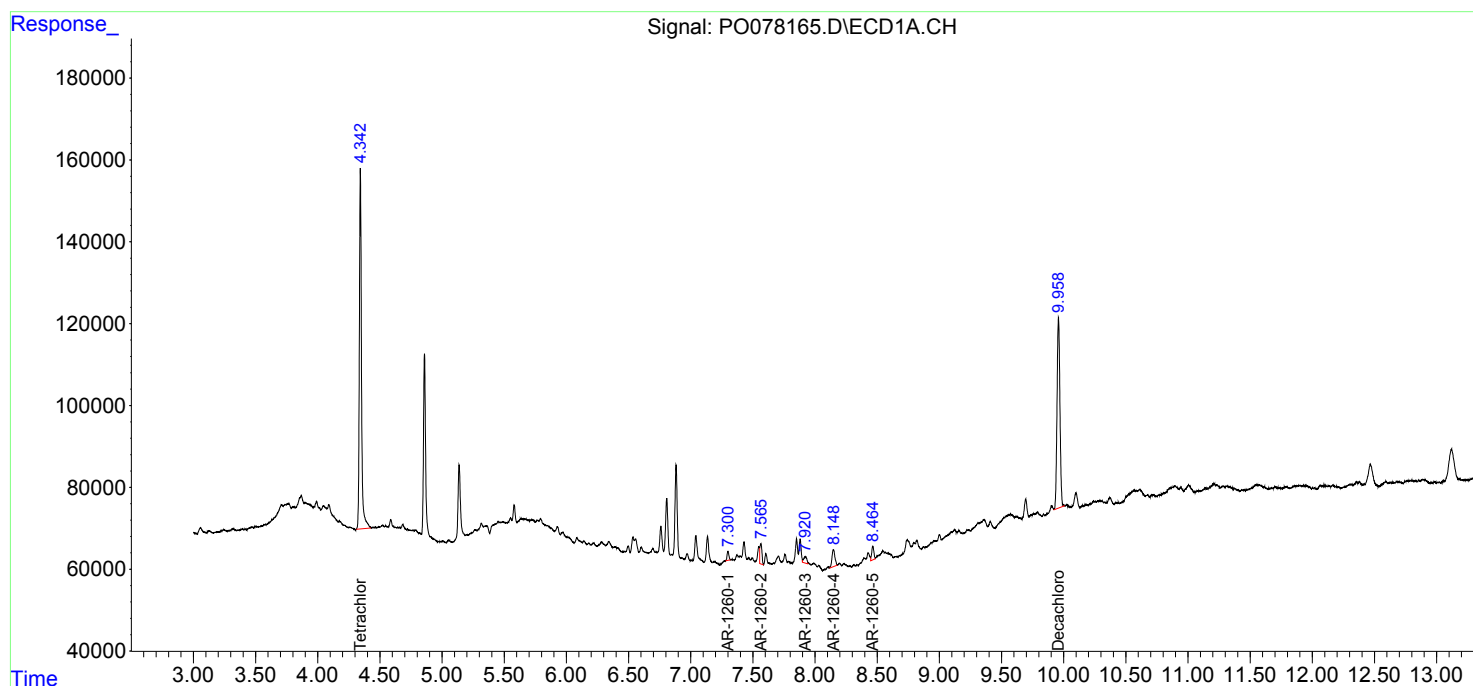

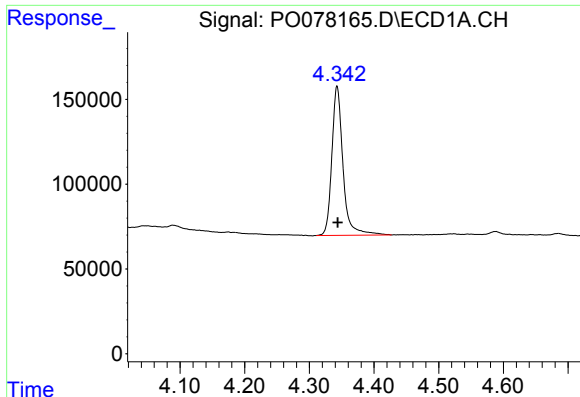


#1 Tetrachloro-m-xylene

R.T.: 4.343 min
Delta R.T.: -0.001 min
Response: 1055804
Conc: 14.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
METRO-SP


Manual Integrations
APPROVED

Ankita
5/27/2021 2:10:28 PM

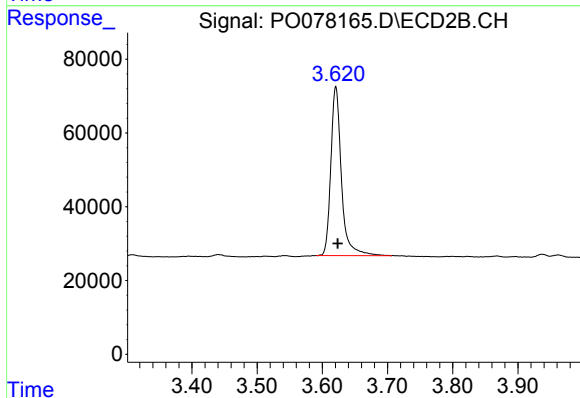


#1 Tetrachloro-m-xylene

R.T.: 3.621 min
Delta R.T.: -0.003 min
Response: 517257
Conc: 17.12 ng/ml

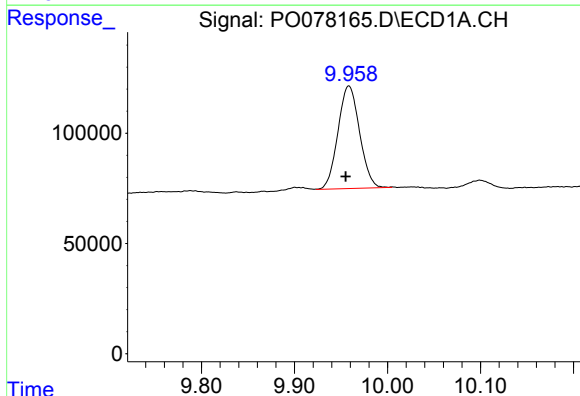


#2 Decachlorobiphenyl

R.T.: 9.958 min
Delta R.T.: 0.003 min
Response: 749567
Conc: 15.16 ng/ml m

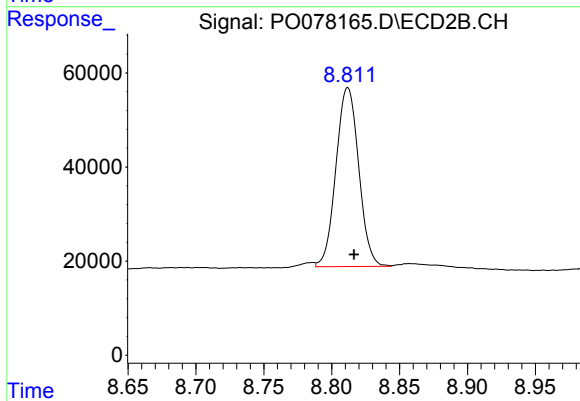

#2 Decachlorobiphenyl

R.T.: 8.811 min
Delta R.T.: -0.005 min
Response: 443820
Conc: 15.26 ng/ml m

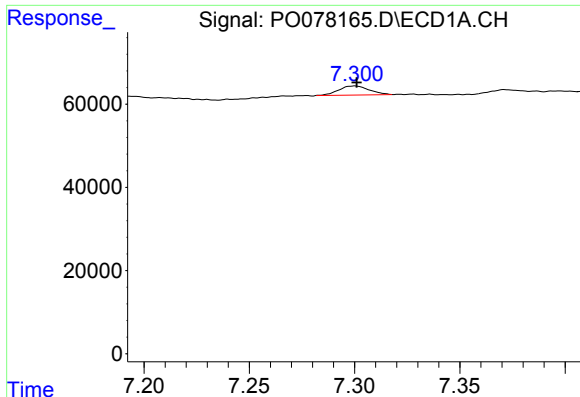


#31 AR-1260-1

R.T.: 7.300 min
Delta R.T.: -0.001 min
Response: 22563
Conc: 8.04 ng/ml m

Instrument :
ECD_O
ClientSampleId :
METRO-SP


Manual Integrations
APPROVED

Ankita
5/27/2021 2:10:28 PM

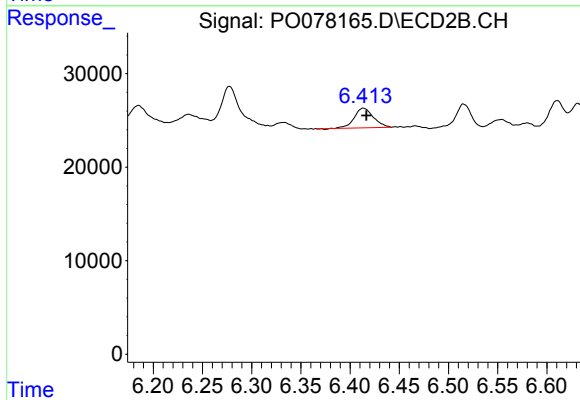


#31 AR-1260-1

R.T.: 6.414 min
Delta R.T.: -0.003 min
Response: 28471
Conc: 17.77 ng/ml

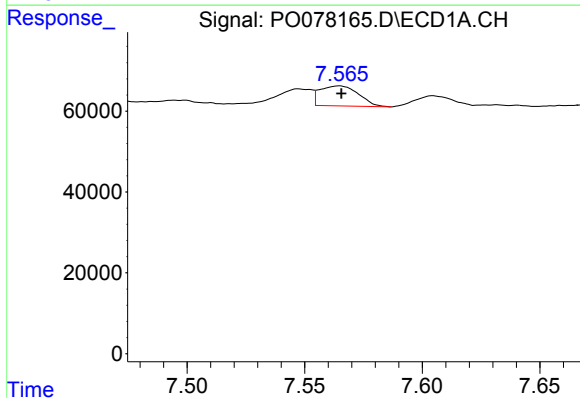


#32 AR-1260-2

R.T.: 7.565 min
Delta R.T.: 0.000 min
Response: 56565
Conc: 16.81 ng/ml

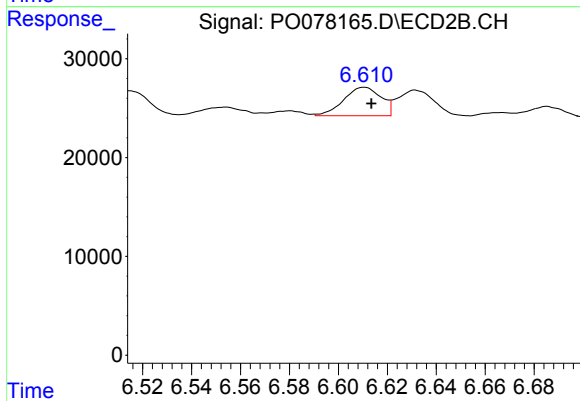

#32 AR-1260-2

R.T.: 6.611 min
Delta R.T.: -0.003 min
Response: 30566
Conc: 15.83 ng/ml

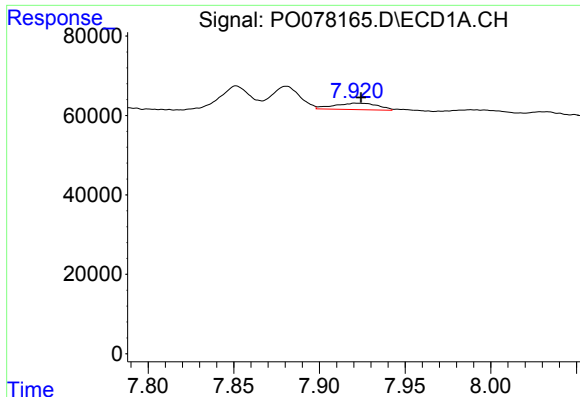


#33 AR-1260-3

R.T.: 7.920 min
Delta R.T.: -0.004 min
Response: 28605
Conc: 11.72 ng/ml m

Instrument :
ECD_O
ClientSampleId :
METRO-SP


Manual Integrations
APPROVED

Ankita
5/27/2021 2:10:28 PM

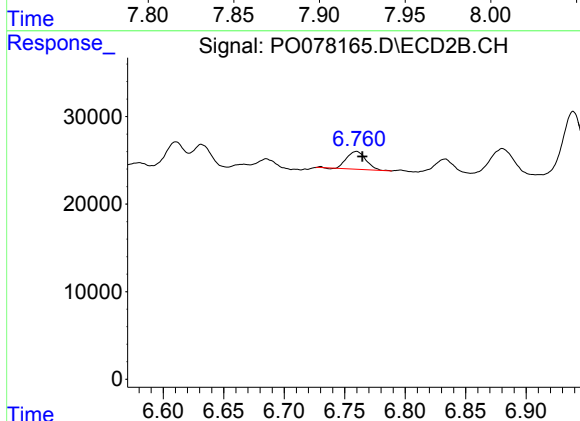


#33 AR-1260-3

R.T.: 6.760 min
Delta R.T.: -0.005 min
Response: 22574
Conc: 12.30 ng/ml

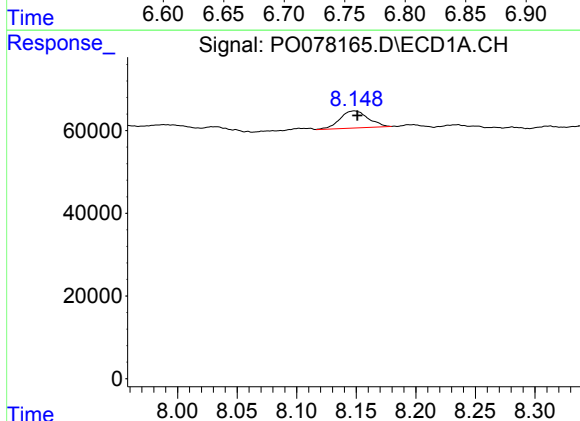


#34 AR-1260-4

R.T.: 8.148 min
Delta R.T.: -0.003 min
Response: 68183
Conc: 25.45 ng/ml

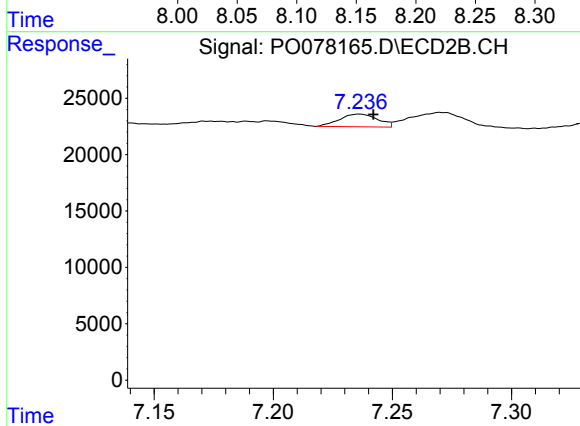

#34 AR-1260-4

R.T.: 7.236 min
Delta R.T.: -0.006 min
Response: 12589
Conc: 8.35 ng/ml

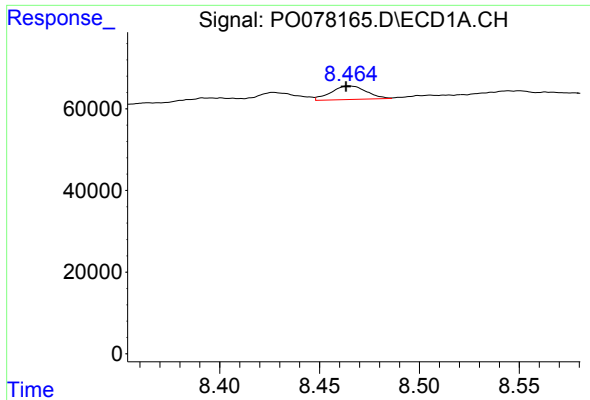


#35 AR-1260-5

R.T.: 8.465 min
Delta R.T.: 0.002 min
Response: 40604
Conc: 7.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
METRO-SP

Manual Integrations
APPROVED

Ankita
5/27/2021 2:10:28 PM

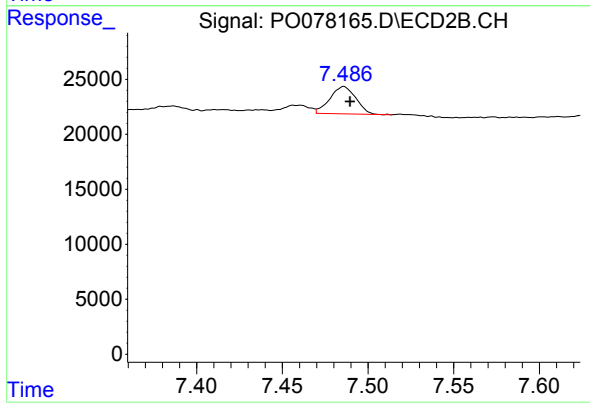

#35 AR-1260-5

R.T.: 7.486 min
Delta R.T.: -0.004 min
Response: 26191
Conc: 7.51 ng/ml